
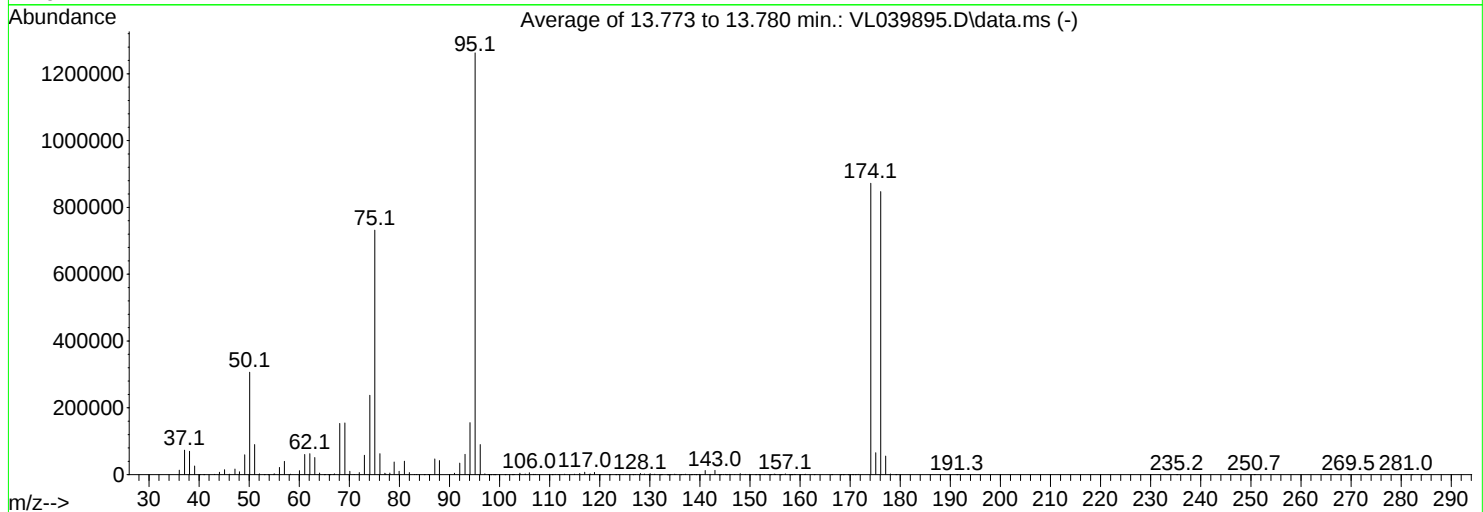


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL111822\
 Data File : VL039895.D
 Acq On : 18 Nov 2022 7:43
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111822AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Fri Nov 18 14:05:14 2022

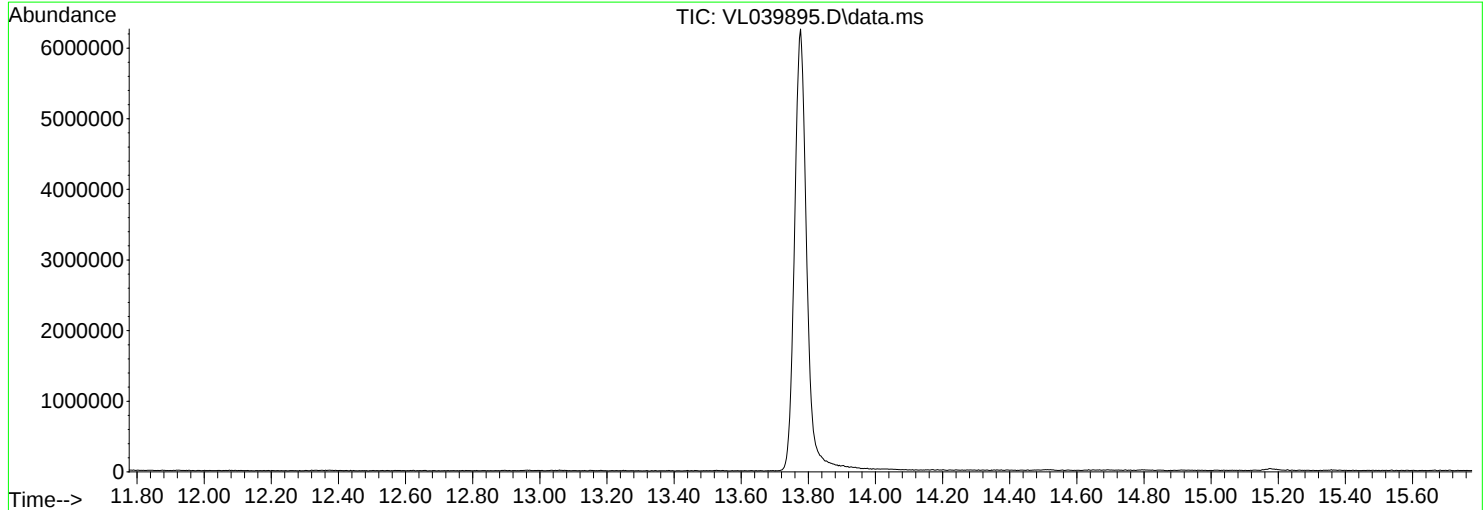

AutoFind: Scans 3474, 3475, 3476; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	306517	PASS
75	95	30	66	57.9	731733	PASS
95	95	100	100	100.0	1262763	PASS
96	95	5	9	7.1	90195	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.1	872256	PASS
175	174	4	9	7.5	65752	PASS
176	174	93	101	97.2	847403	PASS
177	176	5	9	6.6	55517	PASS

Average of 13.773 to 13.780 min.: VL039895.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	13452	48.05	8596	58.25	1623	67.05	223
37.10	73296	49.10	59352	60.05	11817	68.10	15321
38.10	69920	50.10	306517	61.10	60483	69.10	15449
39.10	26037	51.10	90323	62.10	62645	70.10	1004
40.05	49	52.05	2558	63.10	51323	70.95	388
40.95	57	53.00	108	64.05	4661	72.00	6202
43.10	841	53.80	246	65.00	205	73.00	58047
44.05	7019	54.90	1468	65.20	267	74.10	237440
45.10	14875	55.10	2332	65.90	83	75.10	731733
46.10	1422	56.05	21707	66.10	93	76.10	62939
47.15	16775	57.05	40029	66.90	991	77.10	4109

Average of 13.773 to 13.780 min.: VL039895.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.30	1844	87.05	46925	98.80	104	109.95	908
78.10	4861	88.00	42136	99.10	101	110.50	248
78.95	37871	91.00	4298	101.10	71	111.10	1155
79.95	10225	92.05	34667	102.60	81	111.70	355
81.00	40272	93.10	60861	103.00	291	111.95	571
82.00	6502	94.10	155605	103.90	1182	113.00	1404
83.05	598	95.10	1.26276e+006	104.05	4178	114.95	1306
83.40	275	96.15	90195	105.10	2156	116.00	3507
84.95	152	97.05	2623	105.95	5609	117.00	7219
85.80	732	97.80	208	106.80	962	117.90	1278
86.10	495	98.25	177	107.10	903	118.10	2110

Average of 13.773 to 13.780 min.: VL039895.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	6792	128.10	3580	135.20	982	143.80	227
120.00	236	128.90	1745	136.20	94	144.00	222
121.95	250	129.80	1205	136.80	541	144.25	551
123.20	251	130.05	2876	137.15	1713	144.70	338
123.80	371	131.00	1564	138.30	113	145.10	865
124.10	527	132.00	73	138.90	256	145.30	155
124.65	417	132.30	54	139.20	248	145.85	906
125.25	508	133.50	104	139.95	948	146.10	559
126.05	709	133.65	204	141.05	12374	146.95	721
126.65	157	134.00	70	142.05	1060	148.05	2760
127.10	284	134.95	1559	143.00	12797	149.05	869

Average of 13.773 to 13.780 min.: VL039895.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
149.90	902	155.95	180	162.80	94	175.10	65752
150.10	450	156.20	90	166.30	55	176.10	847403
151.10	60	157.05	2180	168.10	53	177.10	55517
151.80	254	157.90	77	168.60	144	178.05	1814
152.05	362	158.10	137	168.95	321	179.10	72
152.85	746	158.40	115	169.60	100	191.30	55
153.65	486	158.90	816	170.05	590	235.20	81
154.00	174	159.10	478	170.50	243	250.70	77
154.20	547	160.00	269	171.00	123	269.50	58
154.85	1836	160.90	514	171.60	1025	281.00	281
155.10	1047	161.05	1411	174.10	872256	282.10	79

Average of 13.773 to 13.780 min.: VL039895.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
284.10	220						