

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL111919\
Data File : VL034385.D
Acq On : 19 Nov 2019 18:52
Operator : SY/AP
Sample : OC110419 CAN 10332
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC110419 CAN 10332

Quant Time: Nov 20 11:03:18 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL111919AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Nov 20 03:30:54 2019
QLast Update : Wed Nov 20 03:30:54 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.68	49	999196	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.20	114	1955543	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.14	117	1874151	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.47	95	1618966	10.27	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.70%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL111919\
Data File : VL034385.D
Acq On : 19 Nov 2019 18:52
Operator : SY/AP
Sample : OC110419 CAN 10332
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC110419 CAN 10332

Quant Time: Nov 20 11:03:18 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL111919AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Nov 20 03:30:54 2019
QLast Update : Wed Nov 20 03:30:54 2019
Response via : Initial Calibration

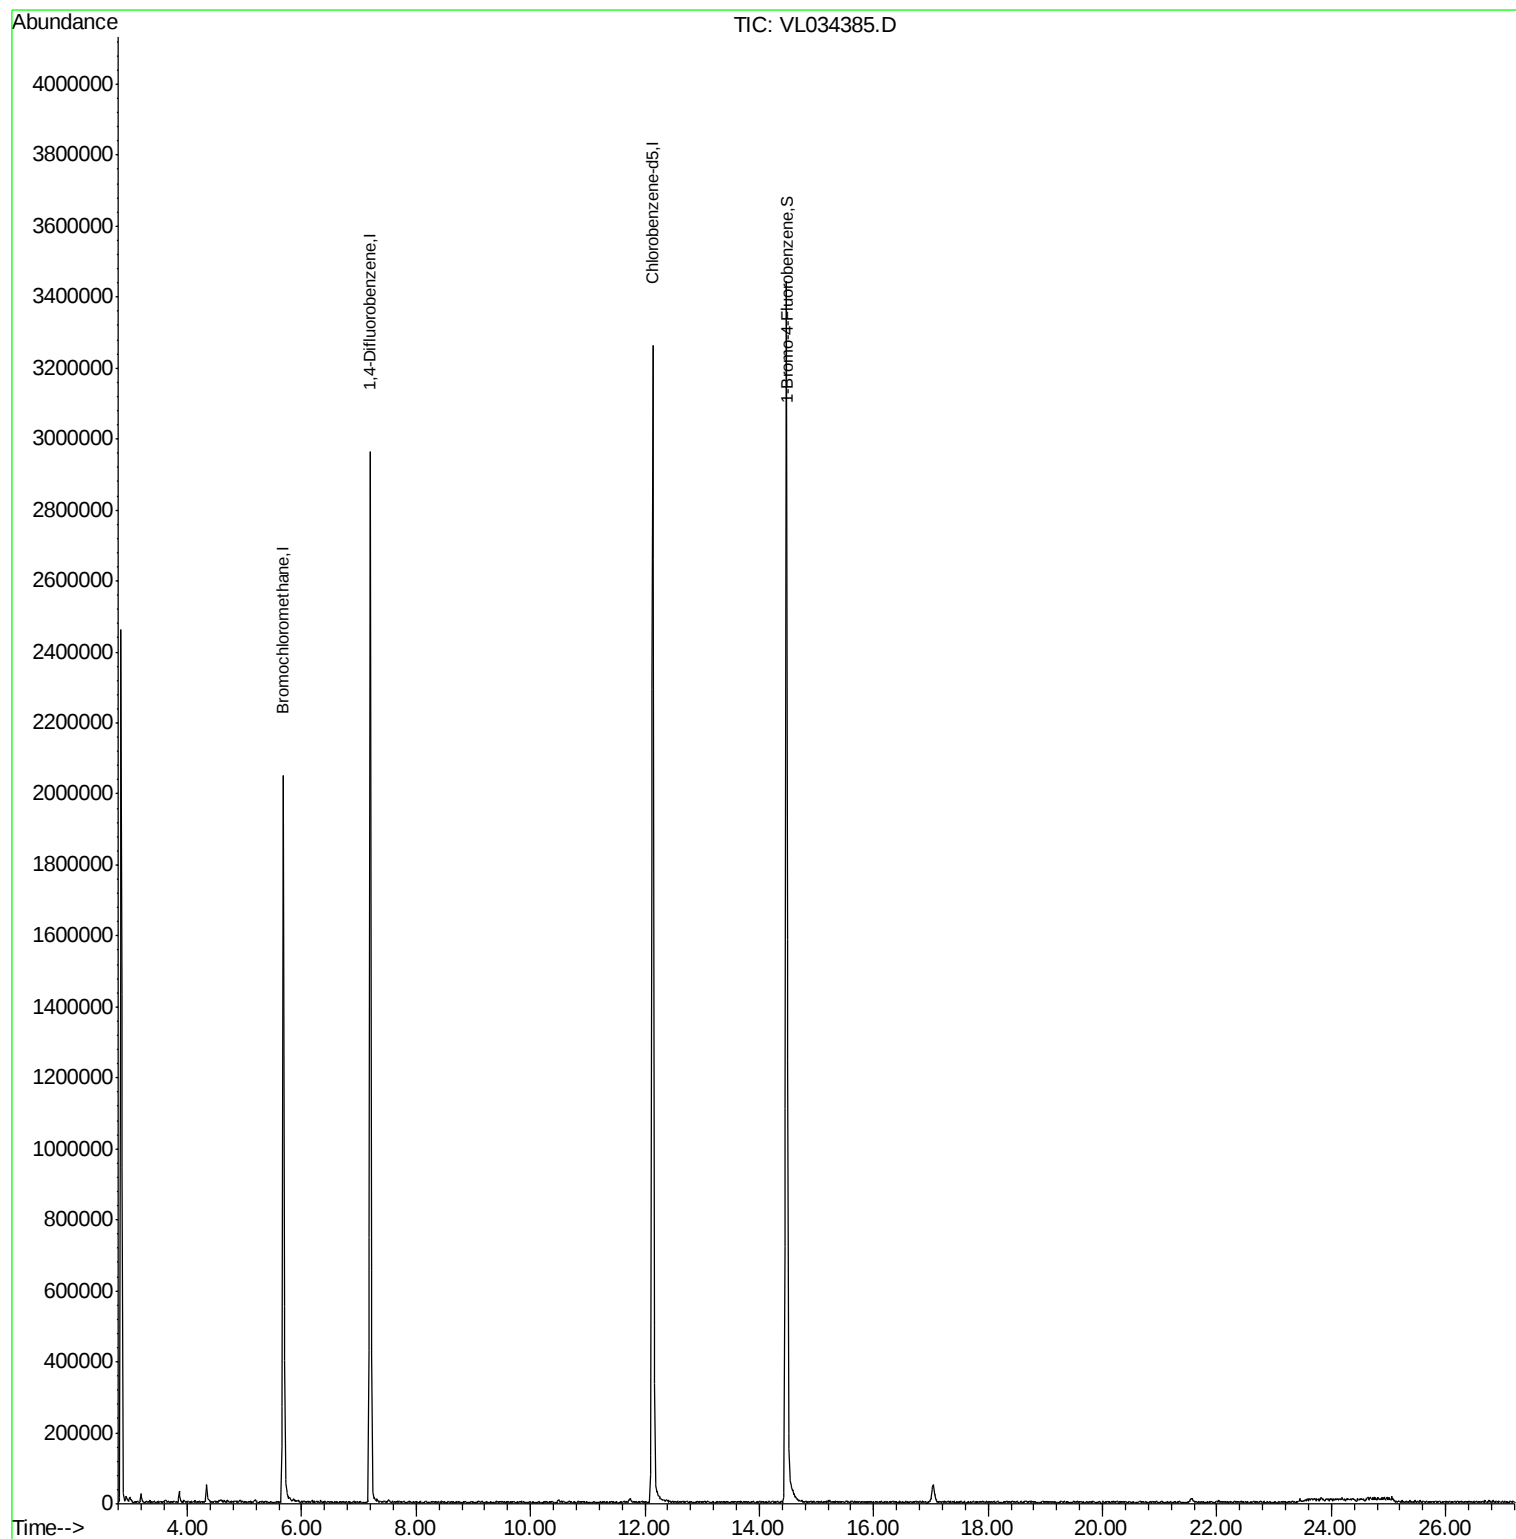

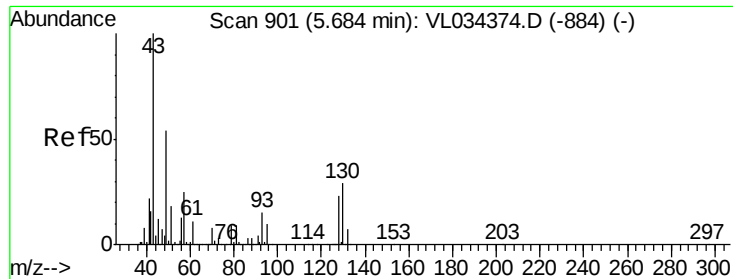

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.68 min Scan# 899

Delta R.T. -0.01 min

Lab File: VL034385.D

Acq: 19 Nov 2019 18:52

Instrument :

MSVOA_L

ClientSampleId :

QC110419 CAN 10332


Tot Ion: 49 Resp: 999196

Ion Ratio Lower Upper

49 100

128 42.6 21.8 65.3




130 54.7 28.0 84.0

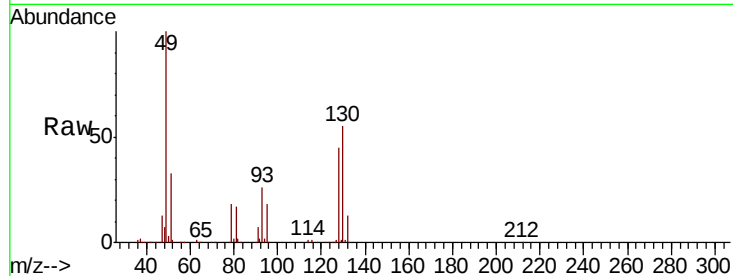

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

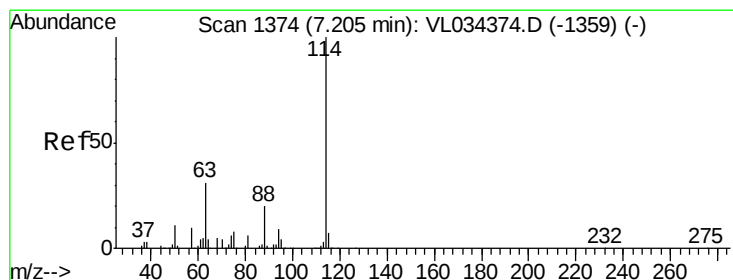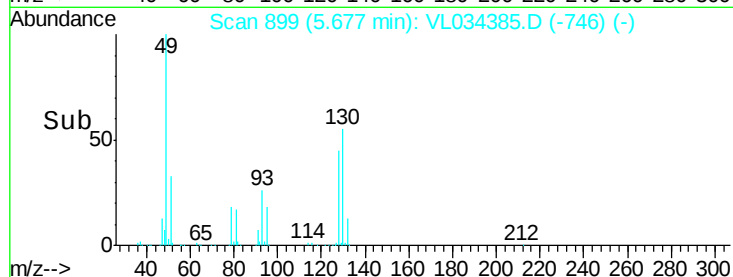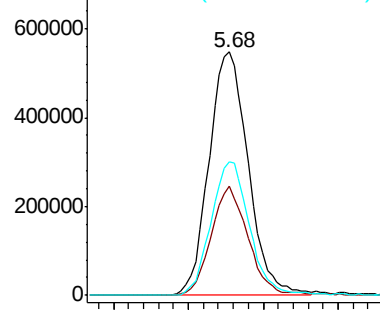

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.20 min Scan# 1373

Delta R.T. -0.00 min

Lab File: VL034385.D

Acq: 19 Nov 2019 18:52


Tgt Ion: 114 Resp: 1955543

Ion Ratio Lower Upper

114 100

63 29.7 24.2 36.4



88 20.0 15.9 23.9

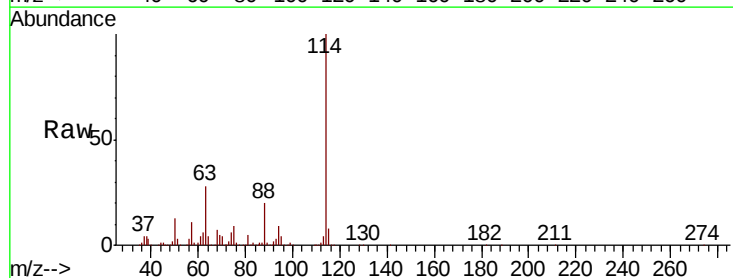


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



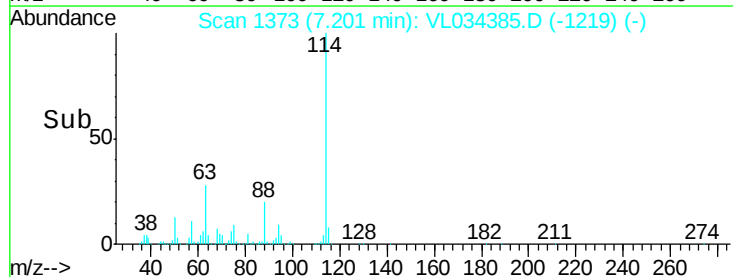
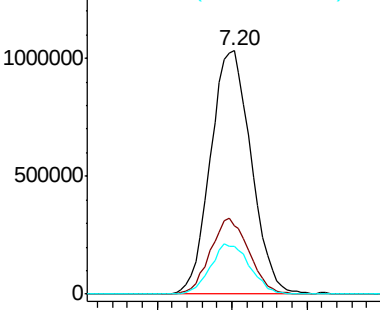


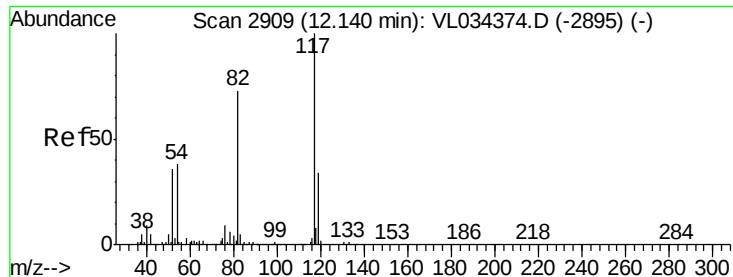

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.14 min Scan# 2908
Delta R.T. -0.00 min
Lab File: VL034385.D
Acq: 19 Nov 2019 18:52

Instrument :
MSVOA_L
ClientSampleId :
QC110419 CAN 10332

Tot Ion:117 Resp: 1874151
Ion Ratio Lower Upper
117 100
82 73.5 57.5 86.3
119 33.6 25.4 38.2

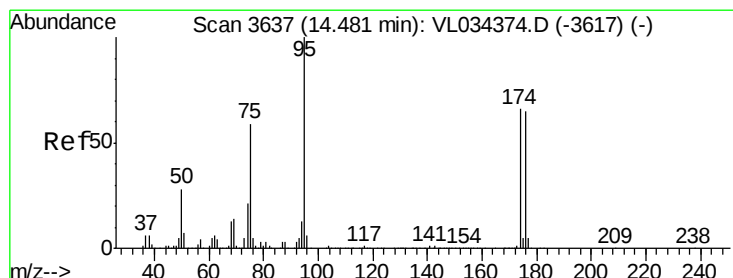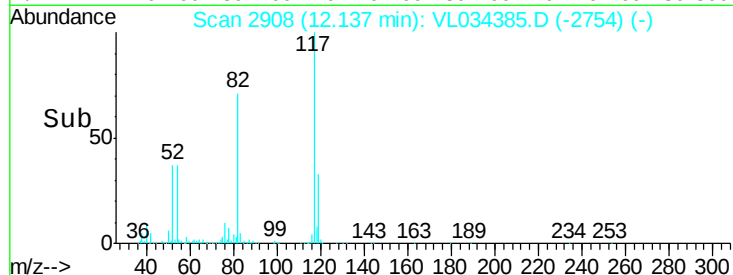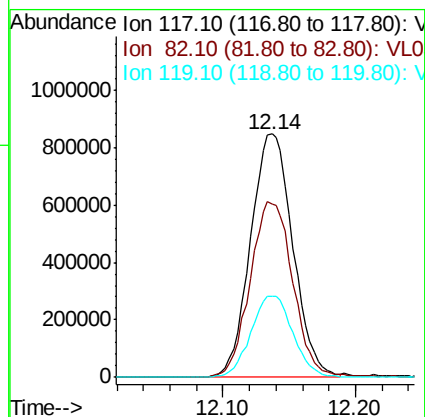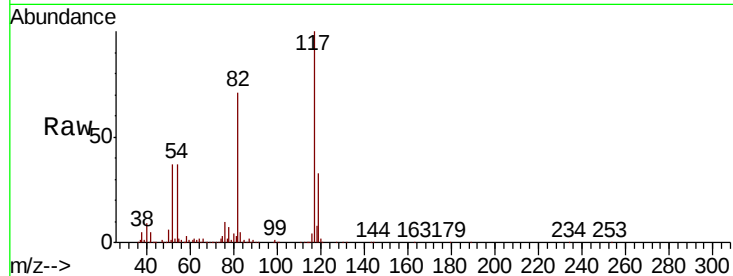

#68
1-Bromo-4-Fluorobenzene
Concen: 10.268 ppbv
RT: 14.47 min Scan# 3634
Delta R.T. -0.01 min
Lab File: VL034385.D
Acq: 19 Nov 2019 18:52

Tgt Ion: 95 Resp: 1618966
Ion Ratio Lower Upper
95 100
174 65.9 52.2 78.2
175 4.8 3.8 5.8

