


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL111919\
Data File : VL034373.D
Acq On : 19 Nov 2019 9:10
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111919AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Oct 17 05:12:37 2019
Last Update : Thu Oct 17 05:12:37 2019

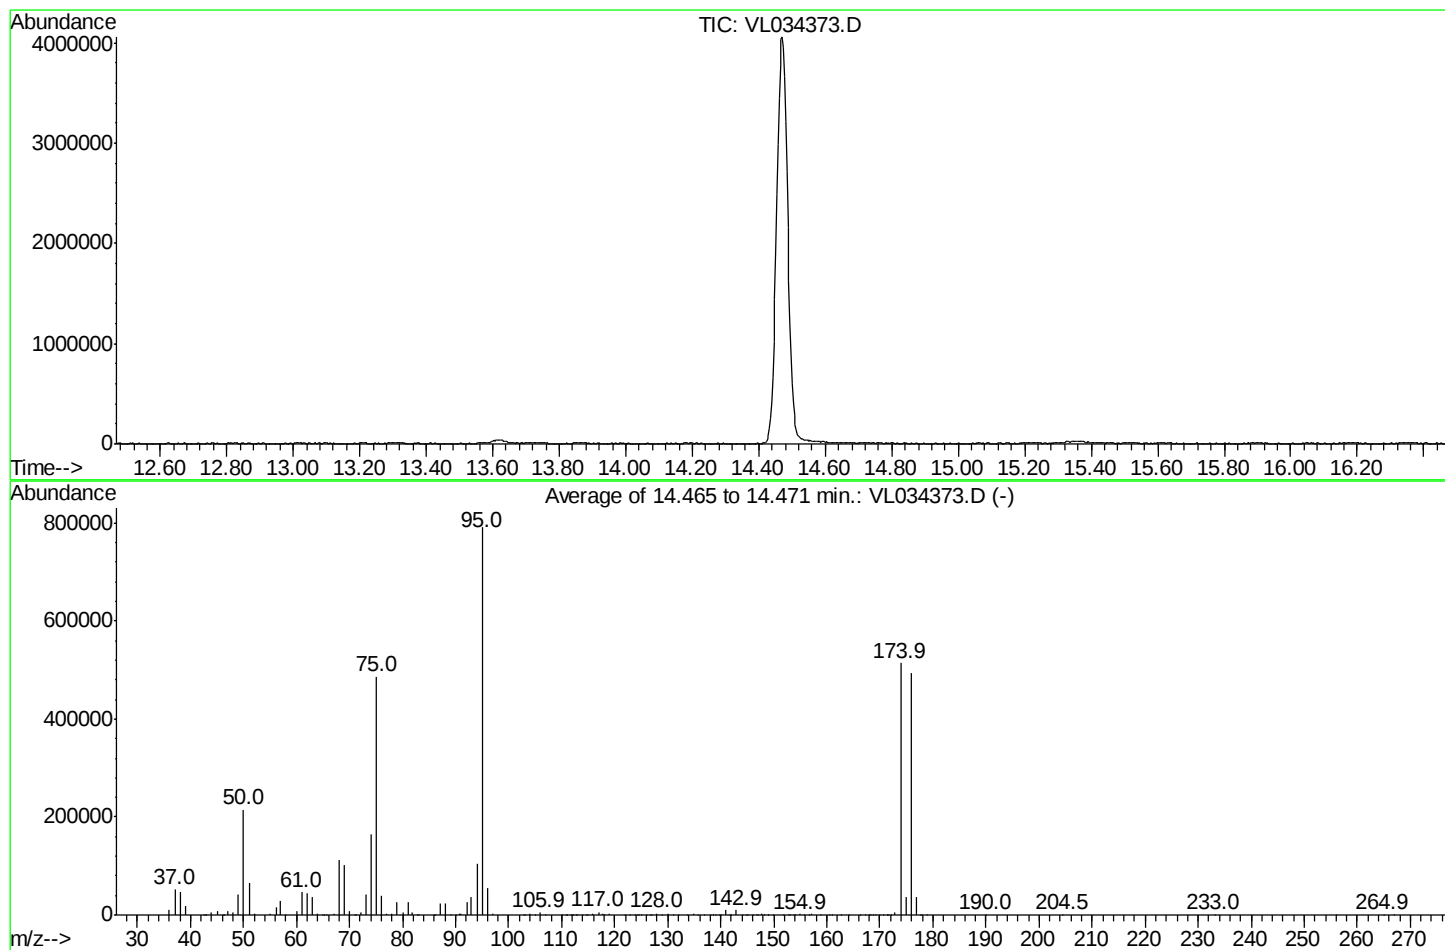

AutoFind: Scans 3632, 3633, 3634; Background Corrected with Scan 3609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.2	215210	PASS
75	95	30	66	61.5	487104	PASS
95	95	100	100	100.0	791402	PASS
96	95	5	9	7.0	55552	PASS
173	174	0.00	2	0.9	4552	PASS
174	95	50	120	65.0	514112	PASS
175	174	4	9	7.1	36700	PASS
176	174	93	101	96.3	495232	PASS
177	176	5	9	7.5	37378	PASS