


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL112018\
 Data File : VL032775.D
 Acq On : 20 Nov 2018 9:49
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111418AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Nov 14 07:00:23 2018
 Last Update : Wed Nov 14 07:00:23 2018

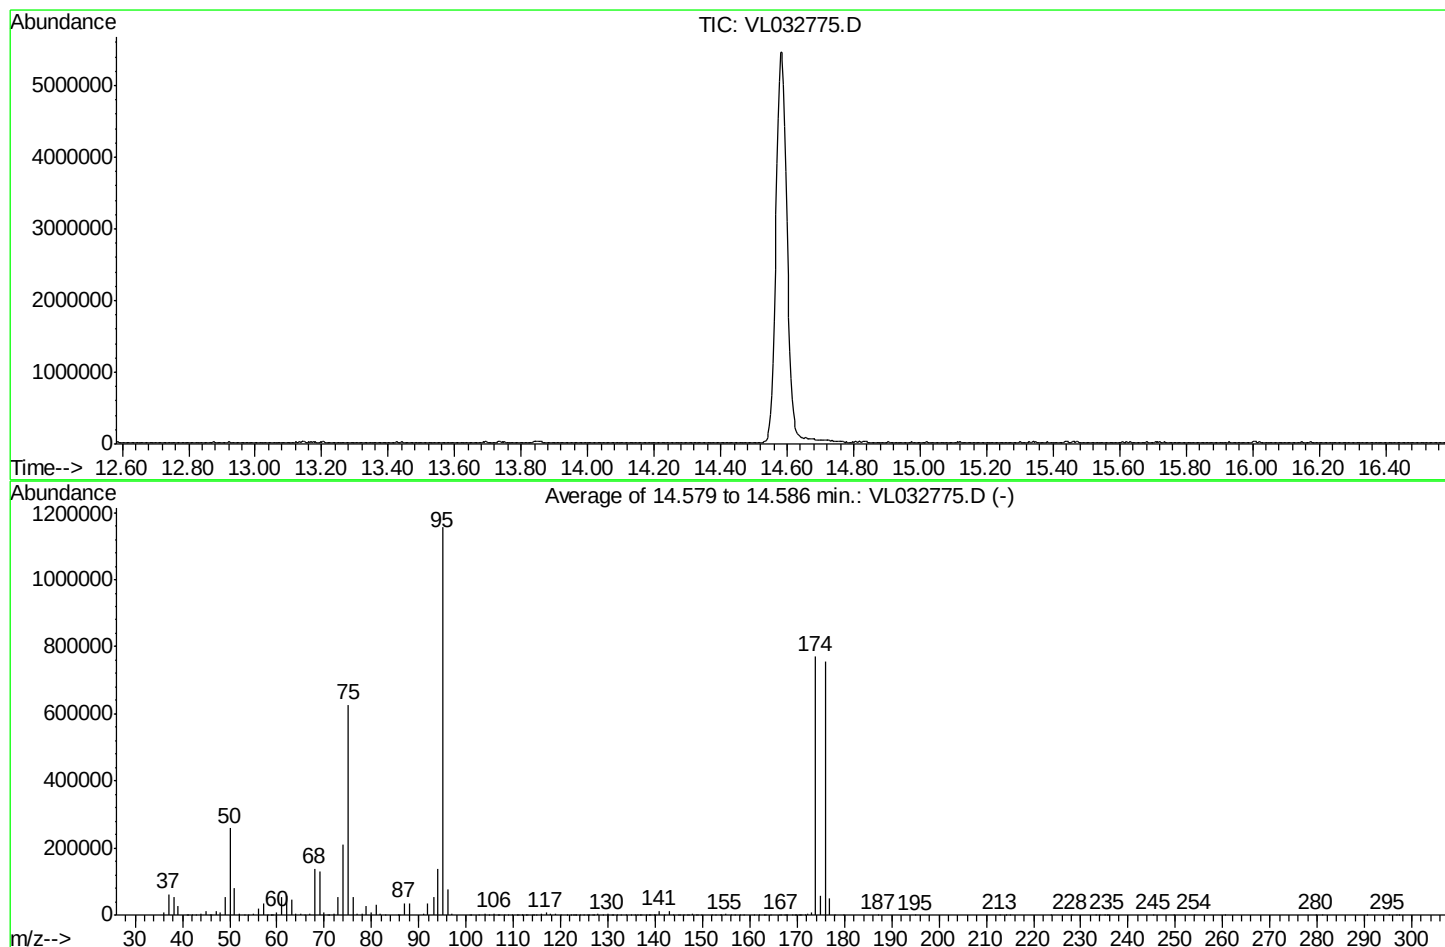

AutoFind: Scans 3621, 3622, 3623; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.3	257941	PASS
75	95	30	66	54.3	627712	PASS
95	95	100	100	100.0	1155925	PASS
96	95	5	9	6.6	75770	PASS
173	174	0.00	2	1.2	9270	PASS
174	95	50	120	66.7	770688	PASS
175	174	4	9	7.6	58322	PASS
176	174	93	101	97.9	754816	PASS
177	176	5	9	6.4	48634	PASS