
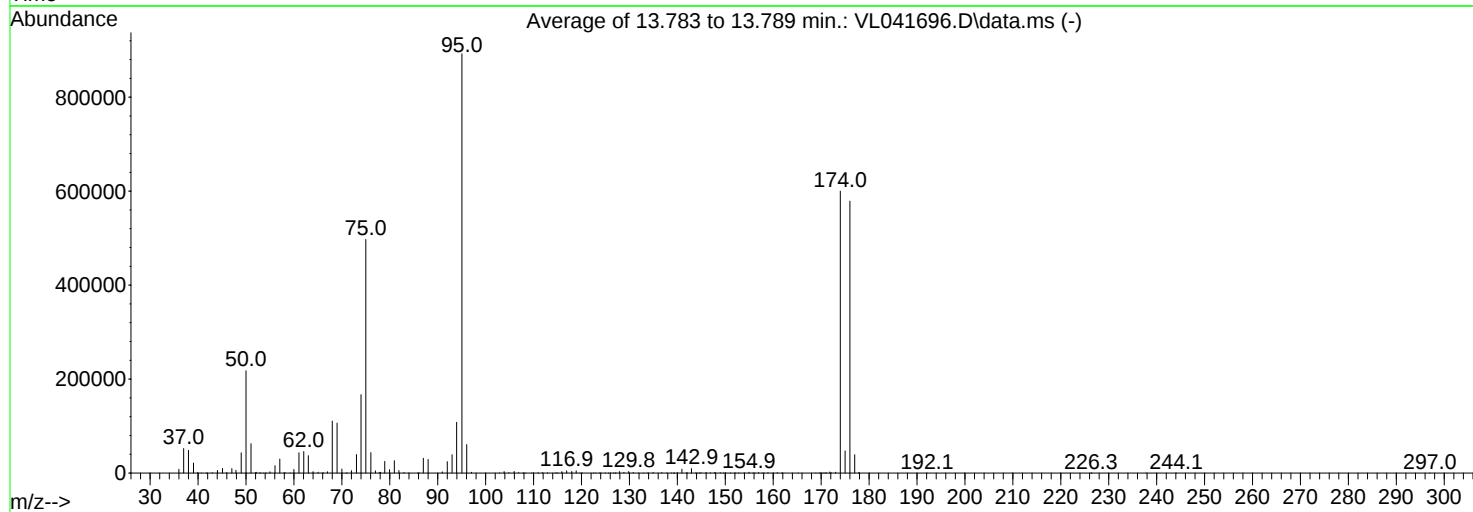


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112024\
Data File : VL041696.D
Acq On : 20 Nov 2024 7:31
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL110724AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Nov 08 01:01:00 2024

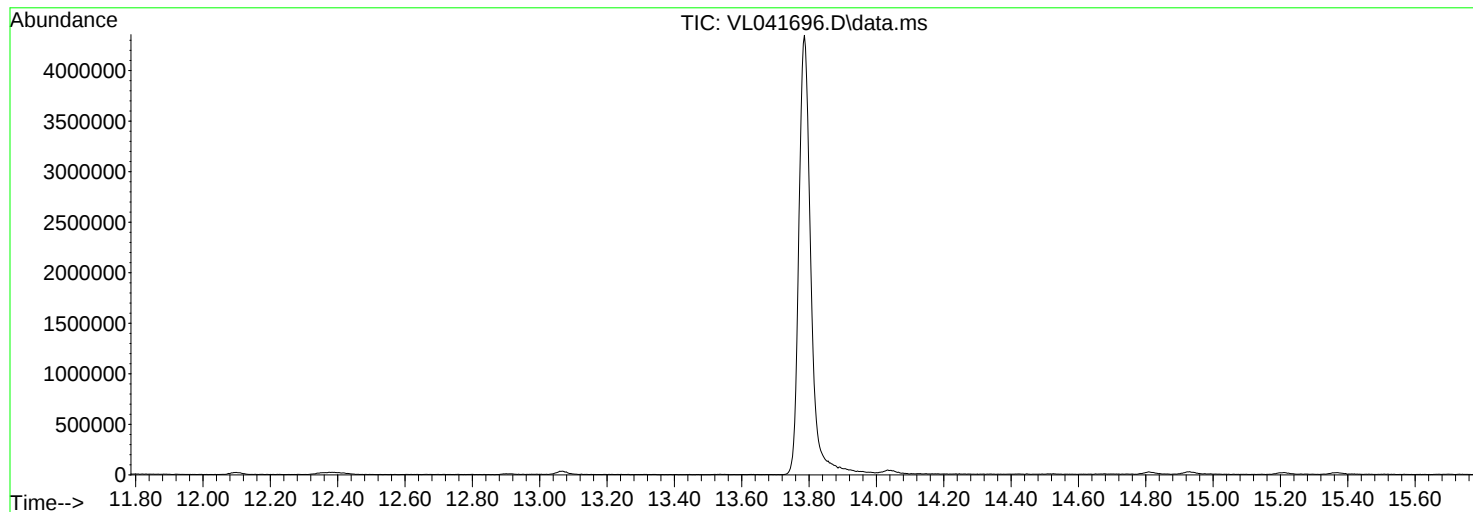

AutoFind: Scans 3477, 3478, 3479; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	217813	PASS
75	95	30	66	55.7	497237	PASS
95	95	100	100	100.0	892416	PASS
96	95	5	9	6.8	60592	PASS
173	174	0.00	2	0.3	1835	PASS
174	95	50	120	67.2	600000	PASS
175	174	4	9	7.9	47296	PASS
176	174	93	101	96.5	578859	PASS
177	176	5	9	6.8	39176	PASS

Average of 13.783 to 13.789 min.: VL041696.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8251	46.00	1026	54.30	114	64.00	3111
37.00	52235	47.05	9596	55.00	2752	65.05	1903
38.00	48469	47.90	6063	56.05	15847	65.90	273
39.05	21312	49.00	43029	57.05	29797	66.15	316
39.90	679	50.00	217813	57.95	754	67.00	2842
40.70	64	51.05	62659	58.15	931	68.00	110813
41.70	65	52.00	946	59.20	81	69.00	106349
41.90	245	52.15	1759	60.00	7830	70.00	8649
42.95	725	52.90	435	61.05	43317	70.90	86
44.05	5620	53.10	208	62.05	45819	71.10	178
45.10	9887	53.70	105	63.00	37128	72.00	5250

Average of 13.783 to 13.789 min.: VL041696.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.05	39397	82.95	1097	96.05	60592	110.95	823
74.00	166933	84.00	66	97.05	1751	111.85	863
75.00	497237	85.80	157	102.90	355	112.95	864
76.05	43528	86.10	651	103.85	3258	114.50	240
77.00	4714	87.00	31560	104.85	1021	114.85	616
77.80	1272	88.00	29016	105.95	3572	115.10	132
78.05	1823	90.95	2669	106.90	871	115.90	3080
78.95	24888	92.00	24453	107.80	53	116.90	4941
79.95	7398	93.00	39117	108.40	86	117.95	3422
80.95	26347	93.95	108158	109.60	78	118.90	4840
81.90	5302	95.05	892416	109.95	466	119.70	197

Average of 13.783 to 13.789 min.: VL041696.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
120.20	65	128.85	1573	139.20	55	146.90	563
122.55	302	129.85	3392	140.00	744	147.80	1404
123.00	167	130.80	1347	140.95	8272	148.00	660
123.70	339	131.90	97	141.90	505	148.95	849
124.05	302	133.00	108	142.10	321	149.65	499
124.95	185	133.70	195	142.95	9521	150.10	588
125.65	169	134.00	88	143.85	393	151.10	180
126.05	193	134.95	1315	144.20	217	152.00	156
126.65	198	136.75	1293	144.60	219	152.20	137
127.00	55	137.80	75	144.90	930	152.80	601
127.95	3317	138.75	270	146.00	1255	153.95	552

Average of 13.783 to 13.789 min.: VL041696.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.95	1736	168.90	150	175.00	47296		
155.80	429	169.60	194	176.00	578859		
156.20	262	169.90	158	177.00	39176		
156.95	1340	170.20	67	177.80	691		
157.70	425	170.60	330	178.00	454		
158.10	148	170.90	181	192.10	75		
158.90	1116	171.10	316	226.30	62		
160.00	69	171.80	2316	237.80	67		
160.85	857	172.10	775	244.10	92		
161.80	55	173.00	1835	297.00	95		
165.20	74	174.00	600000				

Instrument :

MSVOA_L

ClientSampleId :

BFB