



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112122\
Data File : VL039904.D
Acq On : 21 Nov 2022 9:49
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111822AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Nov 22 03:45:31 2022

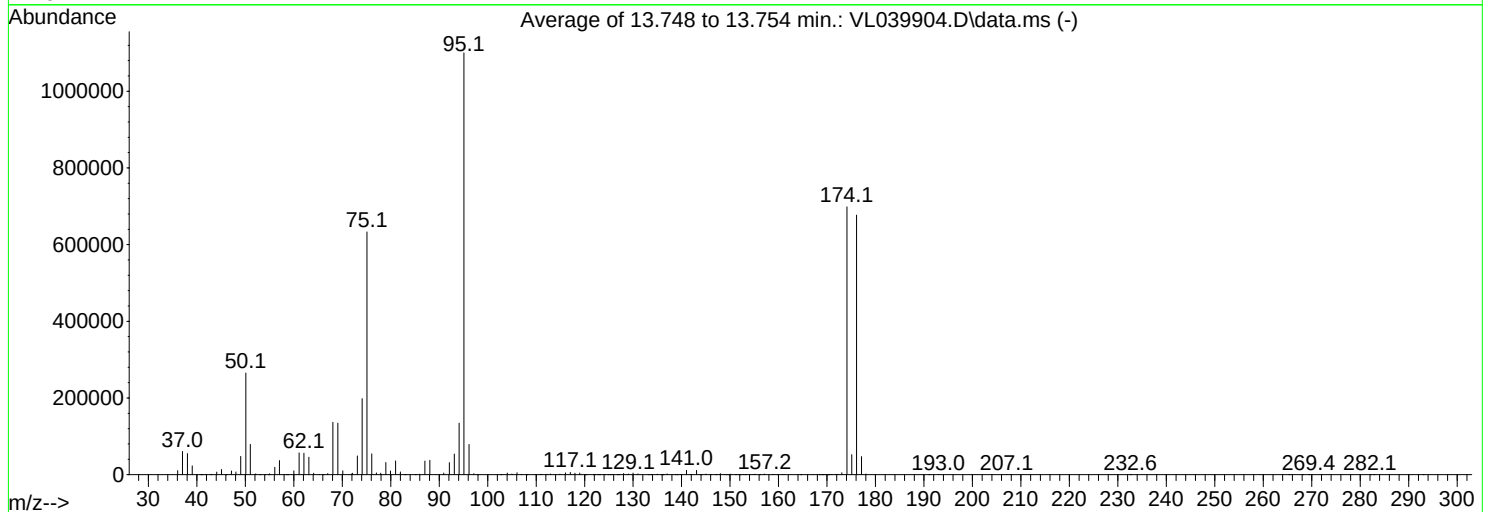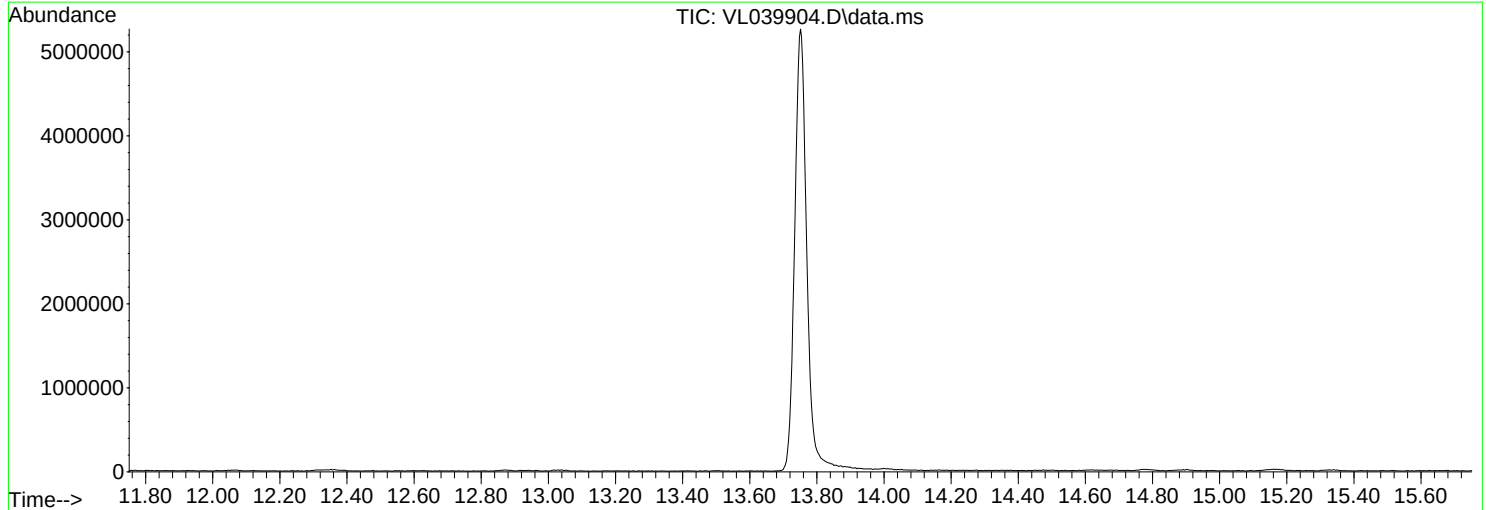

AutoFind: Scans 3466, 3467, 3468; Background Corrected with Scan 3441

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.1	264853	PASS
75	95	30	66	57.5	633024	PASS
95	95	100	100	100.0	1100288	PASS
96	95	5	9	7.2	79040	PASS
173	174	0.00	2	0.7	4930	PASS
174	95	50	120	63.5	698923	PASS
175	174	4	9	7.5	52240	PASS
176	174	93	101	96.9	677163	PASS
177	176	5	9	7.0	47384	PASS

Average of 13.748 to 13.754 min.: VL039904.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	10355	45.10	13269	54.05	186	62.10	5585
37.05	60509	46.00	184	54.80	213	63.10	4550
38.05	55141	46.20	349	55.00	1949	64.10	361
39.05	23113	47.15	9824	55.30	481	65.25	36
40.05	766	48.05	7237	56.10	19080	66.10	117
40.80	59	49.05	47635	57.05	36968	67.00	3153
41.10	121	50.10	264853	58.00	1058	68.05	136693
41.90	176	51.05	78899	58.50	232	69.10	134472
42.85	126	52.00	948	58.80	80	70.10	9888
43.10	488	52.15	2023	60.00	10164	71.90	1720
44.10	6669	53.00	109	61.10	56643	72.10	3742

Average of 13.748 to 13.754 min.: VL039904.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.10	48916	83.00	375	96.15	79040	110.10	332
74.10	198507	83.15	418	97.15	2678	110.85	814
75.10	633024	85.05	136	97.90	106	111.00	299
76.10	54168	86.00	1157	102.70	183	111.20	489
77.05	4560	87.05	35419	102.95	447	112.05	900
77.95	3873	88.05	37637	104.05	4112	112.40	349
79.00	31621	90.95	4199	105.00	1661	113.00	1557
79.95	9454	92.10	31533	106.05	4965	114.90	1257
81.00	35917	93.10	53733	107.00	797	116.05	4464
82.00	7185	94.10	134493	108.10	64	117.05	5926
82.90	209	95.10	1.10029e+006	109.85	339	118.00	3686

Average of 13.748 to 13.754 min.: VL039904.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.00	4290	125.80	399	134.80	378	141.80	445
120.00	144	126.70	155	135.05	1237	142.05	876
120.20	155	127.05	170	135.80	121	143.10	11334
121.80	128	128.05	3031	136.00	86	143.80	397
122.10	66	128.80	466	136.20	103	144.00	200
122.70	211	129.05	1558	136.80	1271	145.05	1746
123.10	78	130.00	4352	137.10	1767	145.90	483
123.80	532	131.00	1979	138.70	96	146.15	548
124.10	154	133.10	62	139.10	140	146.90	464
124.80	114	133.60	57	139.85	776	147.10	84
125.30	73	133.95	402	141.00	11458	147.80	709

Average of 13.748 to 13.754 min.: VL039904.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.05	2597	154.90	611	167.10	344	172.25	1035
148.80	482	155.15	1253	168.45	151	173.05	4930
149.20	129	156.10	177	168.90	176	174.10	698923
149.70	81	156.90	467	169.20	173	175.10	52240
150.15	1093	157.15	1601	169.70	127	176.10	677163
151.15	150	158.80	770	170.10	92	177.10	47384
151.80	129	159.10	457	170.30	224	178.05	1775
152.10	80	159.80	149	170.60	328	191.05	123
152.75	583	160.80	323	170.90	340	193.00	360
153.10	168	161.15	606	171.20	420	207.10	382
154.05	683	164.60	127	171.75	841	207.90	116

Average of 13.748 to 13.754 min.: VL039904.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
232.60	54						
265.30	76						
268.10	72						
269.40	97						
282.10	104						
282.80	96						
293.00	63						

Instrument :
MSVOA_L
ClientSampleId :
BFB