
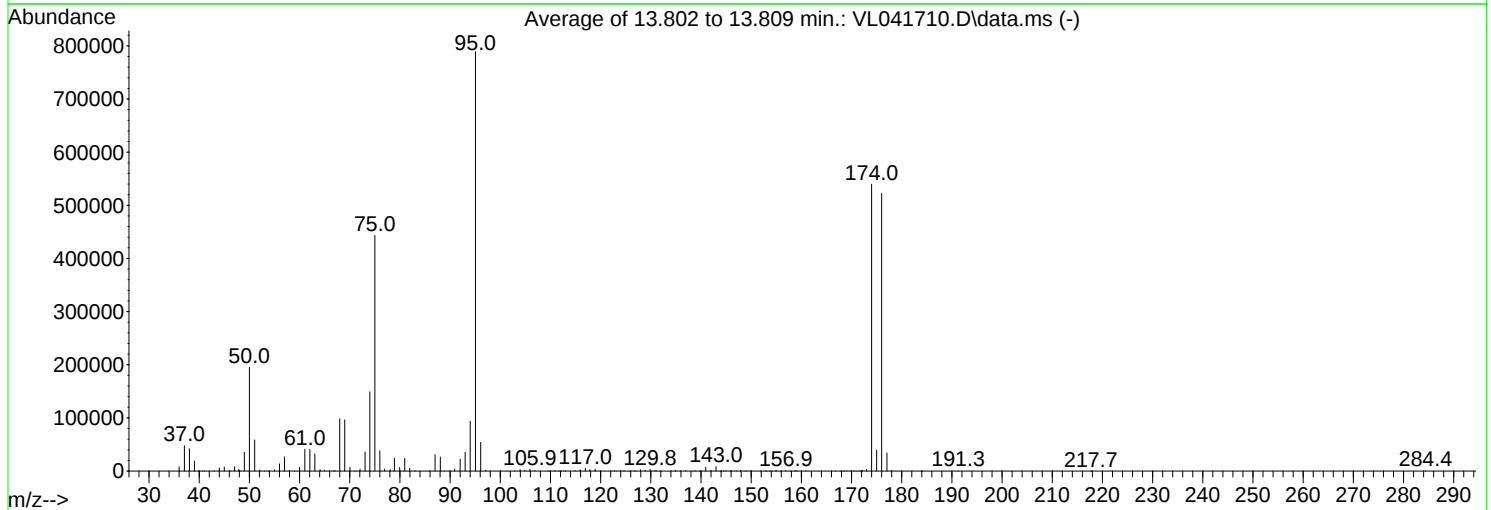


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112124\
Data File : VL041710.D
Acq On : 21 Nov 2024 8:12
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL110724AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Nov 22 01:00:55 2024

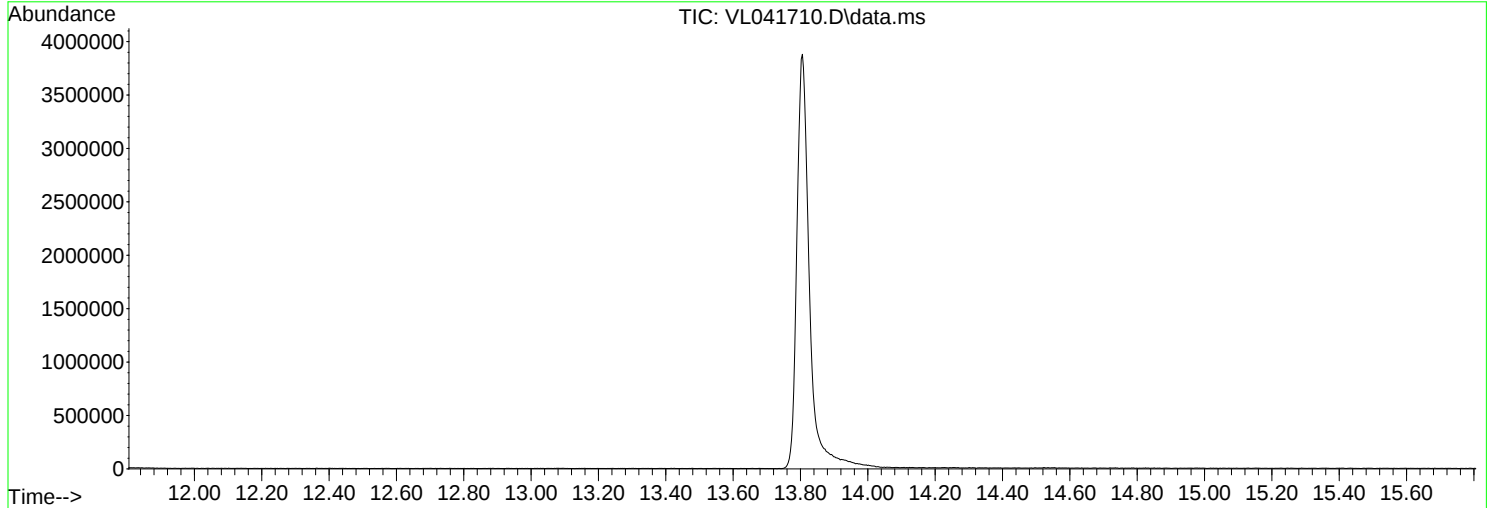

AutoFind: Scans 3483, 3484, 3485; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.7	195264	PASS
75	95	30	66	56.2	443477	PASS
95	95	100	100	100.0	788992	PASS
96	95	5	9	6.9	54053	PASS
173	174	0.00	2	0.6	3163	PASS
174	95	50	120	68.4	539733	PASS
175	174	4	9	7.3	39331	PASS
176	174	93	101	96.8	522347	PASS
177	176	5	9	6.5	33968	PASS

Average of 13.802 to 13.809 min.: VL041710.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8216	46.30	166	56.00	13774	66.80	449
37.05	47515	47.05	8324	57.00	26565	67.05	1129
38.05	42168	47.90	3183	57.95	1219	68.00	9849
39.05	18531	48.10	1529	59.00	304	69.00	9631
40.00	1059	49.00	35365	60.00	7105	70.05	7362
40.70	72	50.00	195264	61.05	40837	71.05	323
41.10	70	51.05	58472	62.05	40691	72.05	3636
42.95	451	52.10	2235	63.05	32344	73.05	35728
44.00	5879	53.05	347	64.10	2744	74.00	149120
45.00	7505	53.80	263	65.00	1527	75.00	443477
46.00	667	55.00	2500	65.95	328	76.00	38333

Average of 13.802 to 13.809 min.: VL041710.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.95	3831	90.90	3467	106.90	817	117.85	2934
78.05	2771	92.00	22525	109.50	115	118.90	3454
78.90	24147	93.00	35400	109.75	309	119.95	199
79.95	6873	94.00	93773	110.90	1005	122.05	218
80.95	23835	95.05	788992	111.70	392	122.75	465
81.95	5280	96.10	54053	112.15	364	123.10	118
83.00	627	97.10	1711	112.70	211	123.95	595
85.90	552	102.85	401	113.00	454	124.50	96
87.00	31035	103.95	2837	114.90	832	124.85	224
88.05	26379	104.90	1507	115.90	2655	125.70	121
88.80	169	105.90	2984	116.95	5159	126.05	143

Average of 13.802 to 13.809 min.: VL041710.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.80	156	135.90	177	144.50	119	153.10	151
126.95	325	136.95	1173	144.95	558	153.75	363
127.95	2526	138.60	140	145.85	715	154.20	88
128.90	1345	138.95	214	146.10	616	154.80	357
129.85	2899	139.70	121	147.05	549	155.00	1048
130.85	639	140.00	242	147.90	1592	155.80	68
131.10	521	140.95	7650	148.80	226	156.05	253
131.80	95	142.00	1100	149.10	127	156.90	1201
132.05	217	143.00	8485	149.95	974	157.80	172
134.00	83	143.90	63	151.90	373	158.60	127
134.90	1432	144.05	281	152.80	308	158.90	671

Average of 13.802 to 13.809 min.: VL041710.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
159.10	317	171.50	266	217.70	56		
160.05	196	171.90	1634	284.40	119		
160.90	799	172.20	1097				
166.80	137	173.00	3163				
167.85	186	174.00	539733				
168.35	150	175.00	39331				
168.60	94	176.00	522347				
169.05	186	177.05	33968				
169.85	385	177.95	734				
170.45	326	183.90	63				
170.90	199	191.25	135				

Instrument :

MSVOA_L

ClientSampleId :

BFB