


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL112321\
 Data File : VL038093.D
 Acq On : 23 Nov 2021 9:44
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111821AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Nov 18 13:16:09 2021
 Last Update : Thu Nov 18 13:16:09 2021

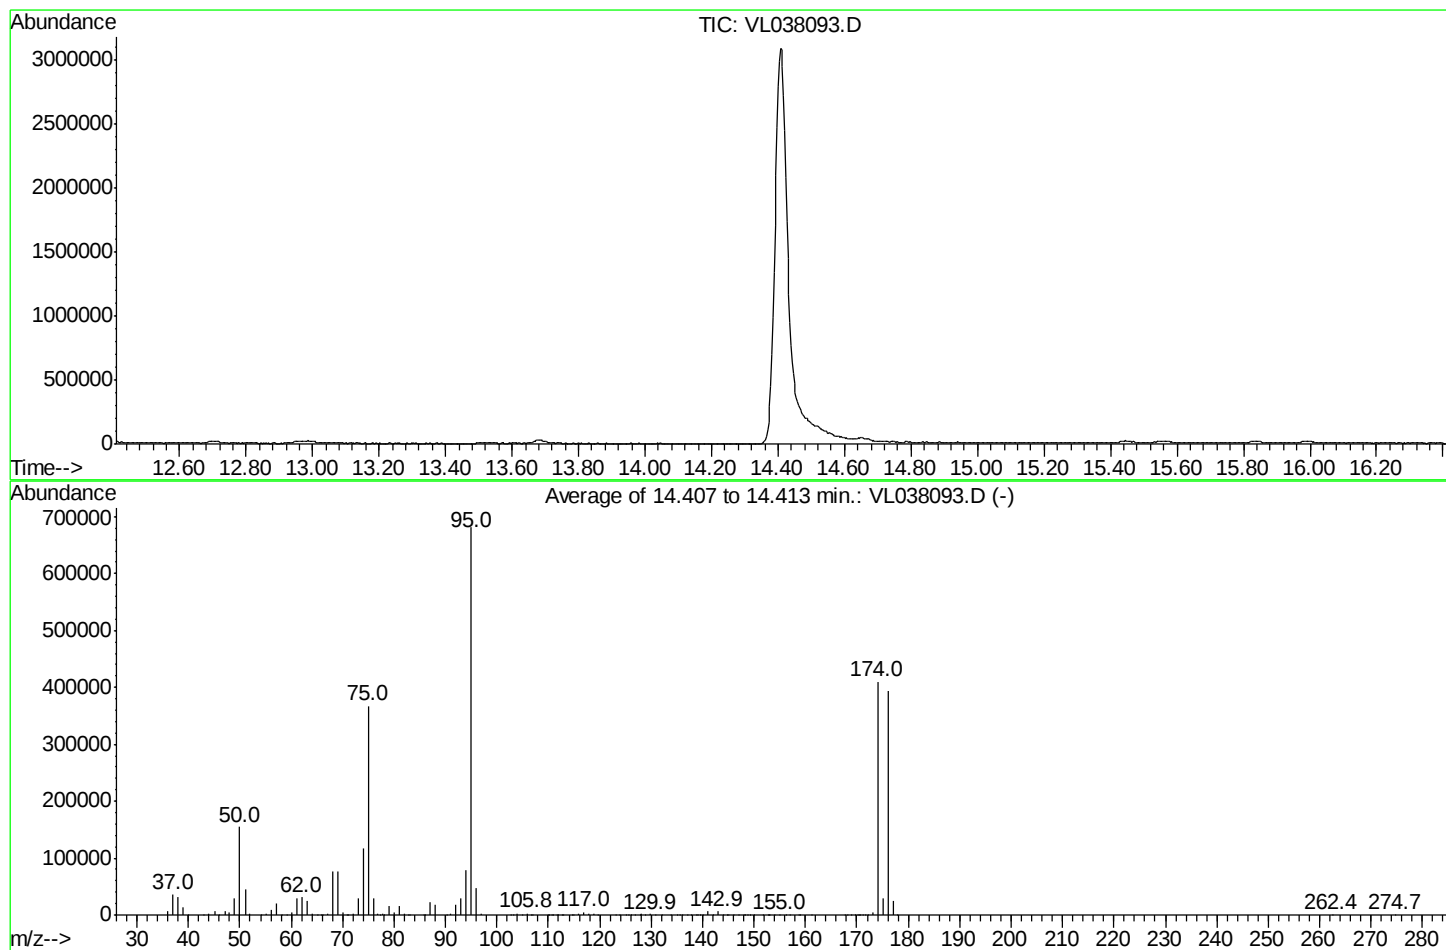

AutoFind: Scans 3614, 3615, 3616; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.7	154304	PASS
75	95	30	66	53.9	367296	PASS
95	95	100	100	100.0	681237	PASS
96	95	5	9	7.0	47528	PASS
173	174	0.00	2	1.1	4459	PASS
174	95	50	120	60.2	410112	PASS
175	174	4	9	7.2	29664	PASS
176	174	93	101	96.2	394474	PASS
177	176	5	9	6.3	25018	PASS