


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL112519\
Data File : VL034400.D
Acq On : 25 Nov 2019 9:27
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111919AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Nov 19 14:15:35 2019
Last Update : Tue Nov 19 14:15:35 2019

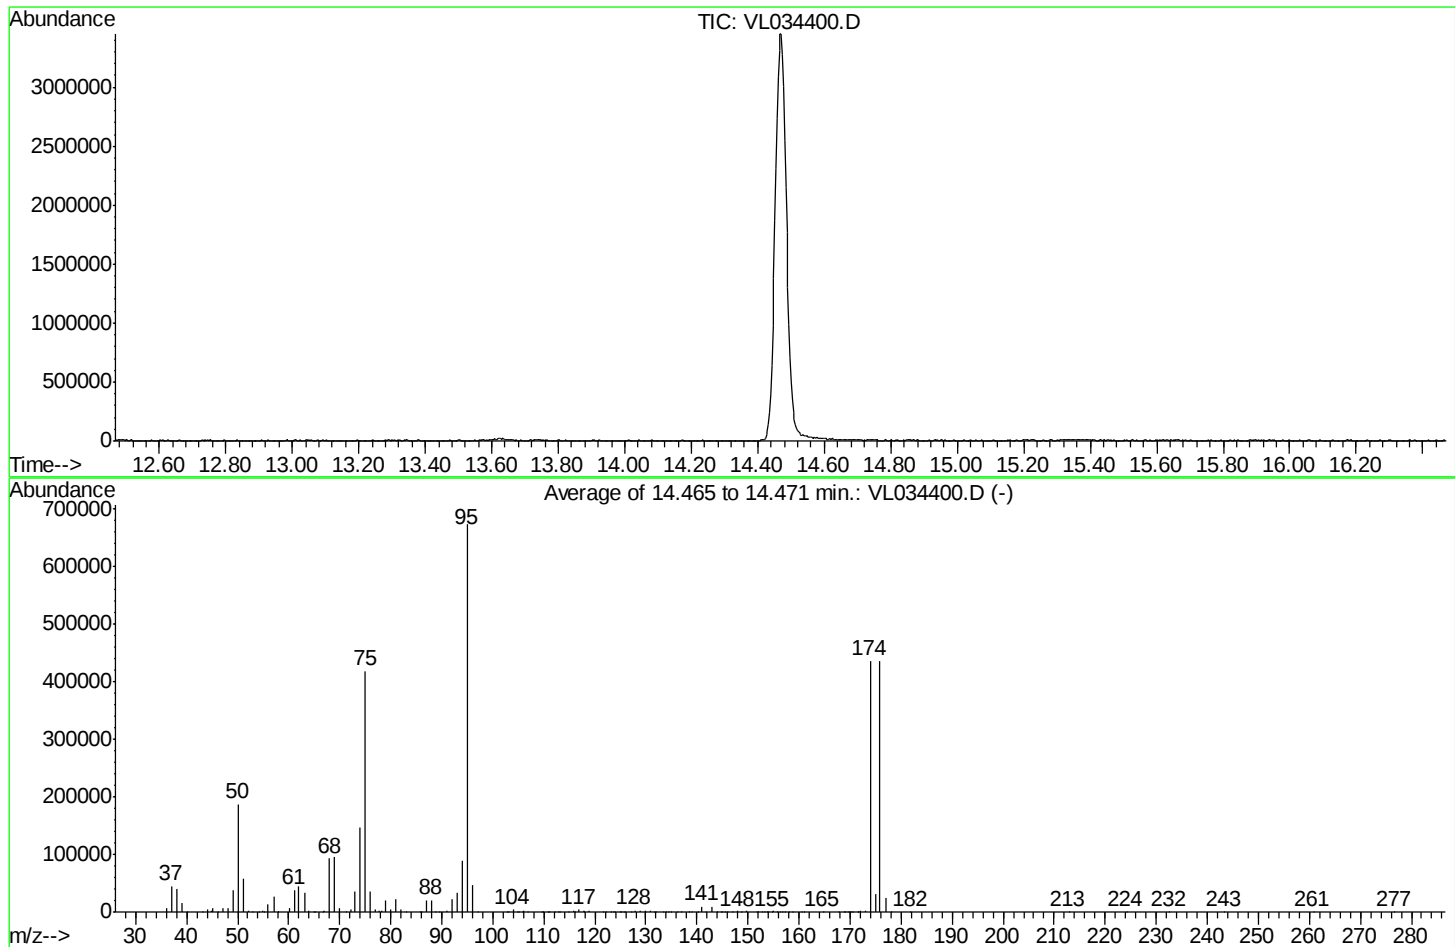

AutoFind: Scans 3632, 3633, 3634; Background Corrected with Scan 3609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.8	186986	PASS
75	95	30	66	62.1	417856	PASS
95	95	100	100	100.0	672533	PASS
96	95	5	9	6.8	45637	PASS
173	174	0.00	2	0.7	3153	PASS
174	95	50	120	64.8	435541	PASS
175	174	4	9	6.9	30122	PASS
176	174	93	101	99.7	434432	PASS
177	176	5	9	5.9	25426	PASS