


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112718\
 Data File : VL032807.D
 Acq On : 27 Nov 2018 12:17
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111418AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Nov 14 07:00:23 2018
 Last Update : Wed Nov 14 07:00:23 2018

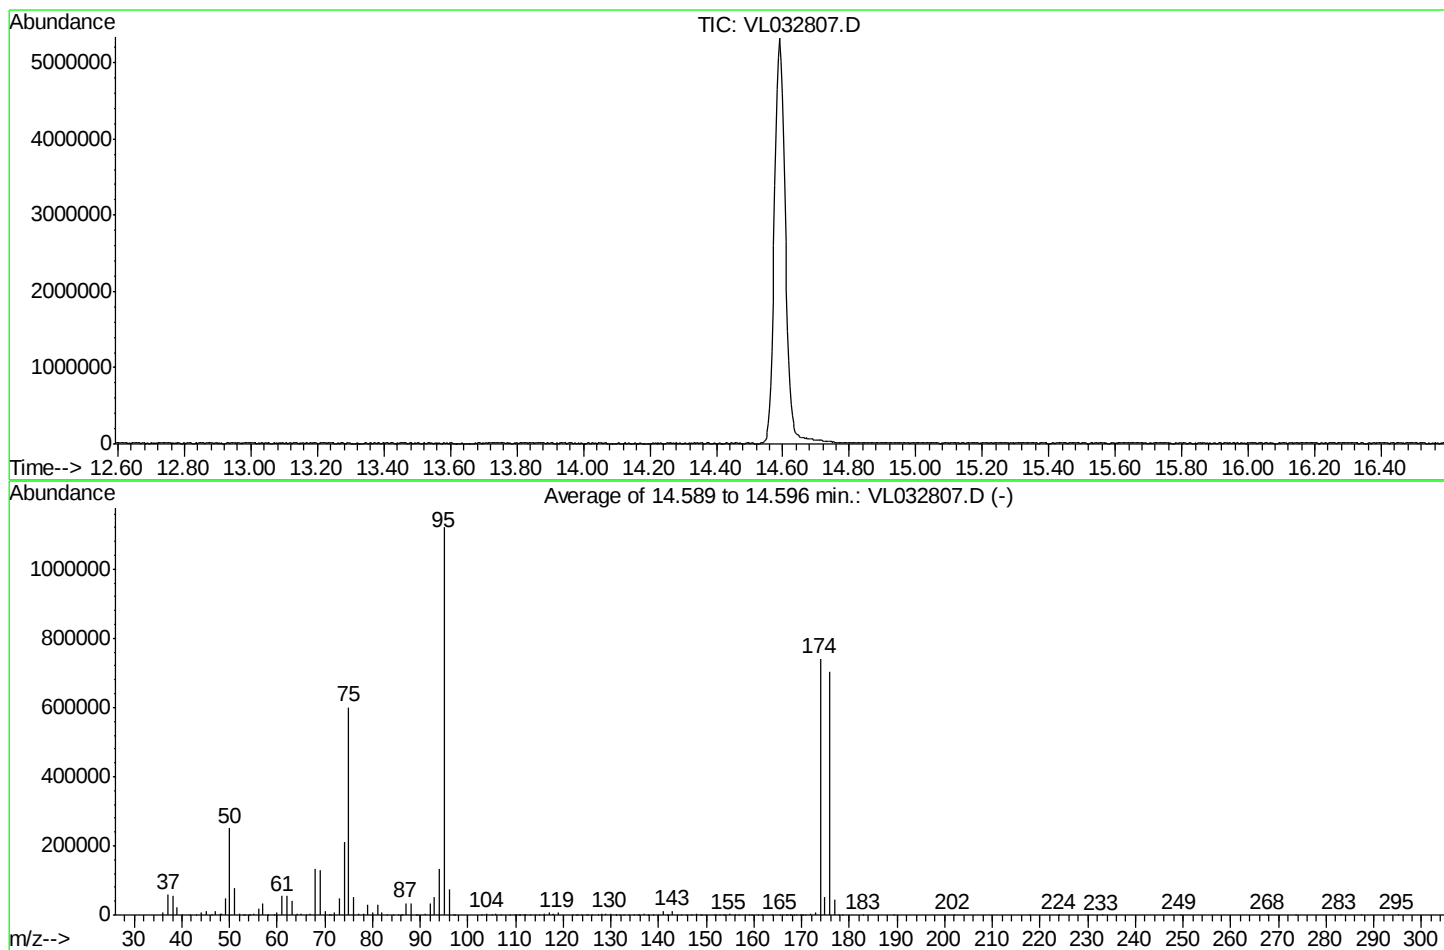

AutoFind: Scans 3624, 3625, 3626; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.4	251157	PASS
75	95	30	66	53.6	600341	PASS
95	95	100	100	100.0	1120768	PASS
96	95	5	9	6.6	74322	PASS
173	174	0.00	2	1.2	8753	PASS
174	95	50	120	66.1	740757	PASS
175	174	4	9	7.1	52570	PASS
176	174	93	101	95.1	704448	PASS
177	176	5	9	6.2	43712	PASS