


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL112921\
 Data File : VL038127.D
 Acq On : 29 Nov 2021 9:29
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111821AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Nov 18 13:16:09 2021
 Last Update : Thu Nov 18 13:16:09 2021

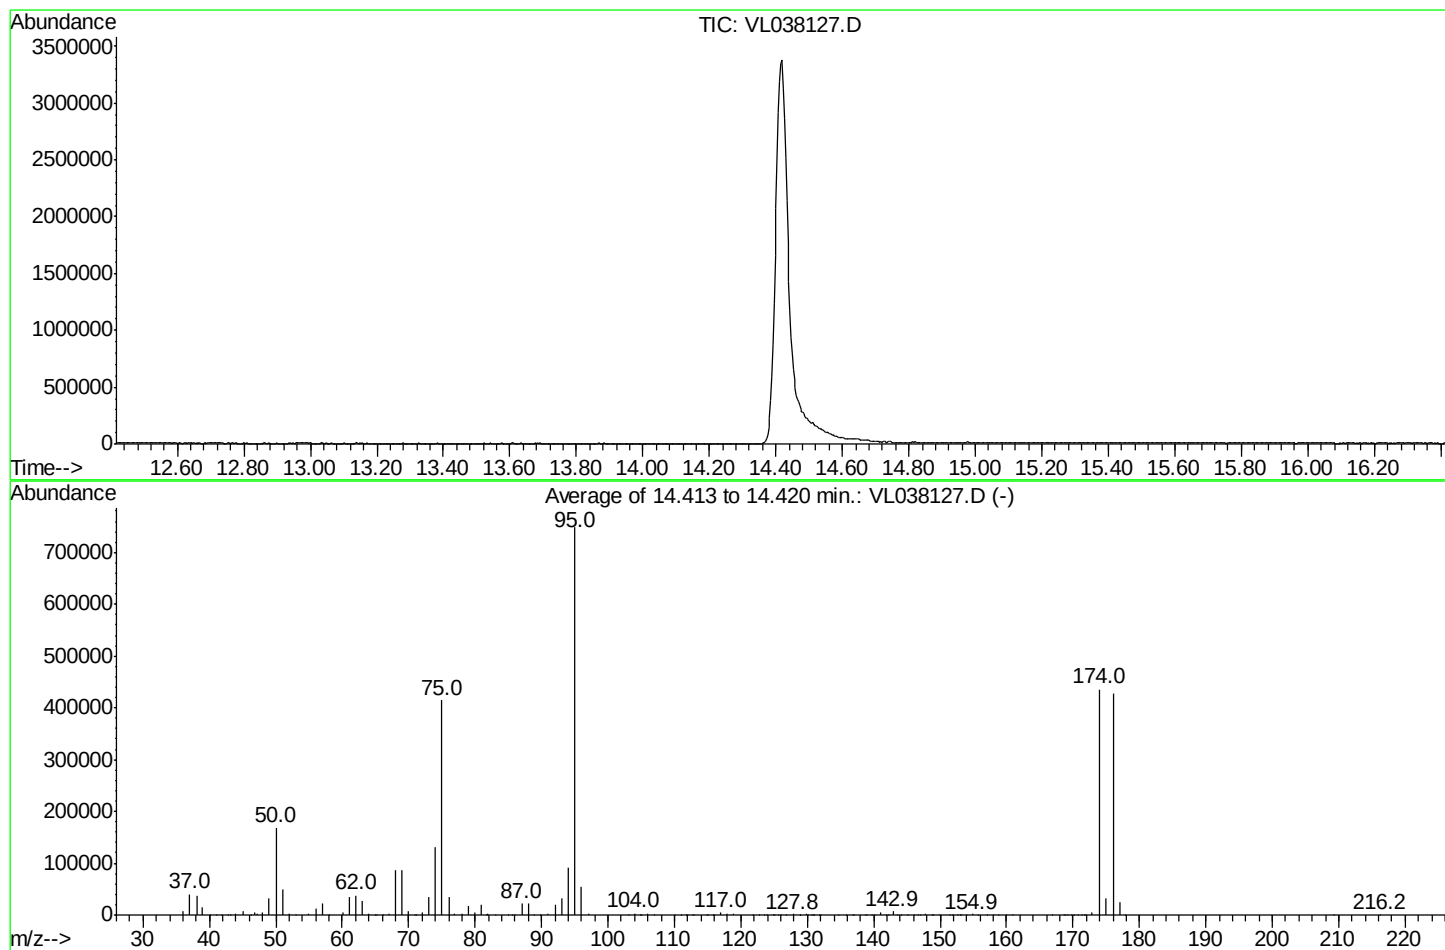

AutoFind: Scans 3616, 3617, 3618; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.5	168725	PASS
75	95	30	66	55.4	414741	PASS
95	95	100	100	100.0	748522	PASS
96	95	5	9	7.2	53898	PASS
173	174	0.00	2	1.1	4742	PASS
174	95	50	120	58.1	435136	PASS
175	174	4	9	7.1	31029	PASS
176	174	93	101	98.4	428138	PASS
177	176	5	9	6.0	25642	PASS