
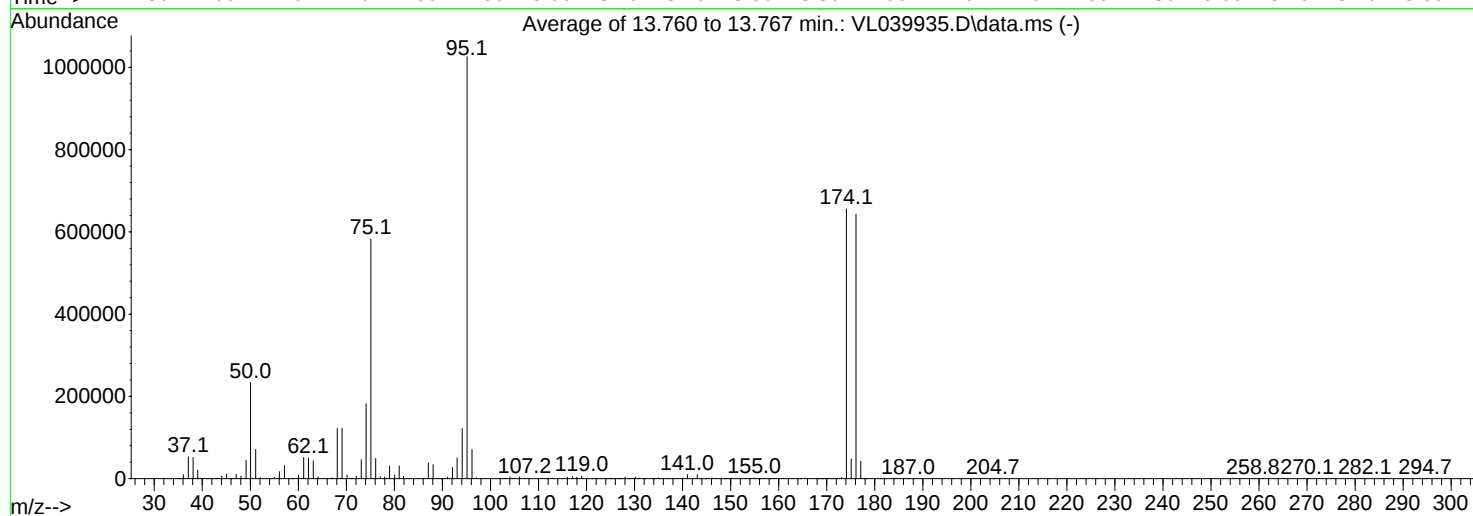


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL120122\
 Data File : VL039935.D
 Acq On : 1 Dec 2022 8:39
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111822AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Fri Dec 02 23:21:36 2022

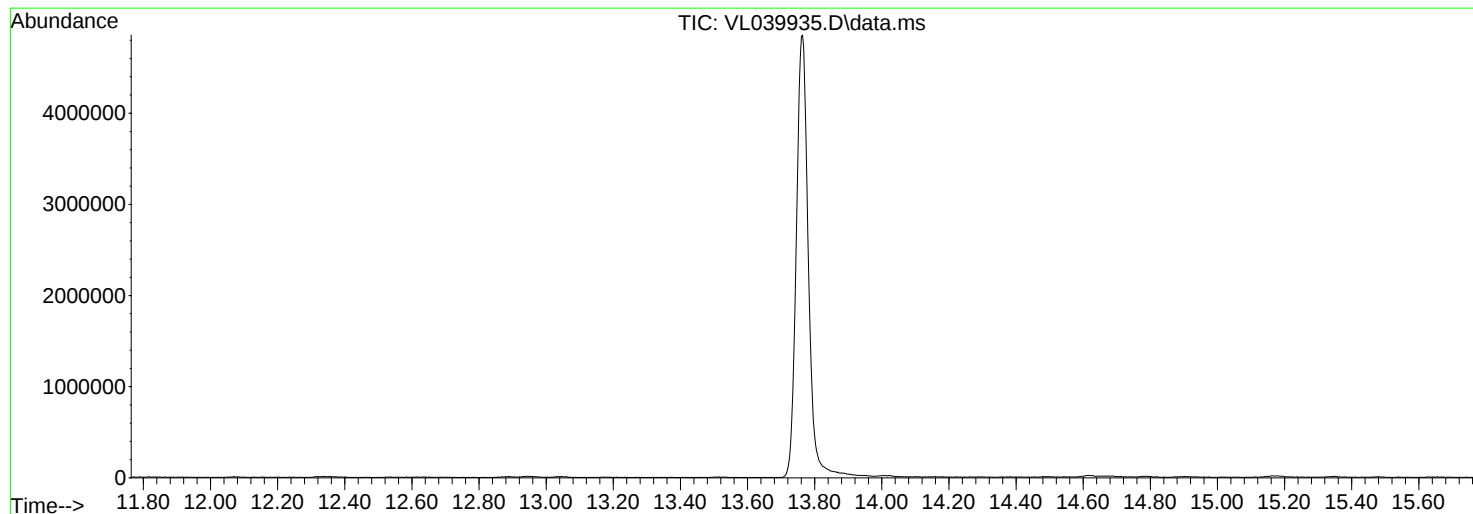

AutoFind: Scans 3470, 3471, 3472; Background Corrected with Scan 3444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.8	233771	PASS
75	95	30	66	56.8	582699	PASS
95	95	100	100	100.0	1025600	PASS
96	95	5	9	6.9	70787	PASS
173	174	0.00	2	0.4	2805	PASS
174	95	50	120	63.9	655573	PASS
175	174	4	9	7.3	47797	PASS
176	174	93	101	98.1	643029	PASS
177	176	5	9	6.6	42317	PASS

Average of 13.760 to 13.767 min.: VL039935.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.20	65	45.90	252	57.10	31877	67.00	166
36.05	9842	46.25	527	57.95	1060	67.20	81
37.10	52965	47.05	10631	58.20	455	68.10	12280
38.10	51491	48.05	6163	58.70	133	69.10	12283
39.05	20643	49.10	44448	60.05	9001	70.15	8917
39.95	745	50.05	233771	61.10	51243	71.00	89
41.10	130	51.10	70813	62.10	50118	72.05	5717
42.80	134	52.10	2904	63.10	43763	73.10	45981
43.15	530	54.10	60	64.15	4359	74.10	182336
44.05	6587	55.05	2711	65.10	553	75.10	582699
45.05	10534	56.05	17069	66.10	528	76.10	48904

Instrument :

MSVOA_L

ClientSampleId :

BFB

Average of 13.760 to 13.767 min.: VL039935.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	4671	88.05	34155	103.10	217	114.85	519
77.95	3759	89.70	87	104.05	3836	115.20	517
79.00	30277	90.00	90	104.90	535	116.05	3655
80.05	9083	91.05	3647	105.15	1078	117.05	5263
81.00	30648	92.10	26947	106.05	3841	117.95	3632
81.90	5937	93.05	50117	107.15	1235	119.00	5981
82.80	553	94.10	121933	109.85	648	120.00	208
83.10	355	95.10	1.0256e+006	110.85	868	121.10	118
84.00	65	96.15	70787	111.60	168	122.05	183
85.85	525	97.05	2515	112.10	646	123.00	567
87.05	37957	102.90	475	112.90	1197	123.75	269

Average of 13.760 to 13.767 min.: VL039935.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.10	197	130.80	353	141.00	9931	148.70	162
124.80	239	131.05	1008	141.90	649	148.90	172
125.10	80	132.10	86	142.10	541	149.25	436
125.80	415	133.80	155	143.05	9611	149.70	151
126.60	69	134.10	194	143.95	962	150.10	943
127.00	53	135.00	1511	144.80	202	151.80	94
128.05	3128	135.90	353	145.05	709	152.10	335
128.90	950	136.80	641	146.10	1526	152.45	283
129.10	605	137.15	1242	146.95	609	153.00	681
129.80	978	138.85	360	147.80	994	153.95	910
130.15	3465	140.00	721	148.15	1666	155.00	1696

Average of 13.760 to 13.767 min.: VL039935.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.70	106	169.20	214	177.10	42317	282.10	52
156.05	169	169.65	126	178.00	843	294.70	63
157.05	1241	170.30	320	178.30	216		
158.25	233	170.85	518	181.20	123		
158.90	375	171.40	533	183.90	130		
159.15	849	171.80	457	187.00	78		
160.95	834	172.25	957	204.70	118		
164.50	73	173.10	2805	207.10	93		
168.20	221	174.10	655573	258.80	122		
168.60	124	175.10	47797	260.70	70		
169.00	196	176.10	643029	270.10	56		