

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL120219\
 Data File : VL034425.D
 Acq On : 2 Dec 2019 14:20
 Operator : SY/AP
 Sample : K6068-01DL 10X
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV-1DL

Quant Time: Dec 03 02:49:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111919AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Nov 19 14:15:35 2019
 QLast Update : Tue Nov 19 14:15:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.69	49	1015292	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.21	114	2080730	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.15	117	2048190	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.48	95	1700653	9.87	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.70%


Target Compounds						Qvalue
2) Dichlorodifluoromethane	3.02	85	14674	0.080	ppbv	88
3) Chlorodifluoromethane	2.97	51	5501	0.043	ppbv	95
9) Propene	2.99	41	417870	7.430	ppbv	95
10) Heptane	8.17	43	26586	0.183	ppbv #	60
13) Ethanol	3.59	45	281194	17.949	ppbv	97
15) Acetone	3.84	43	541995	3.728	ppbv	98
16) 1,3-Butadiene	3.29	39	255976	4.042	ppbv #	34
17) tert-Butyl alcohol	4.30	59	89599	0.733	ppbv	96
19) Isopropyl Alcohol	3.96	45	1801304	19.330	ppbv #	98
20) Methylene Chloride	4.35	84	41053	0.796	ppbv	88
21) Allyl Chloride	4.40	41	3040	0.035	ppbv #	1
22) trans-1,2-Dichloroethene	4.89	96	2245	0.042	ppbv #	89
23) Vinyl Acetate	5.08	43	13262	0.070	ppbv #	10
25) Ethyl Acetate	5.71	43	56617	0.218	ppbv #	91
26) Hexane	5.71	57	70411	0.632	ppbv #	42
27) Carbon Disulfide	4.56	76	5098	0.042	ppbv #	1
29) Chloroform	5.77	83	21059	0.117	ppbv	90
30) Cyclohexane	7.16	84	2837	0.034	ppbv #	1
31) cis-1,2-Dichloroethene	5.56	61	61184	0.531	ppbv #	91
32) 1,1,1-Trichloroethane	6.54	97	50152	0.296	ppbv	99
34) 2-Butanone	5.27	43	59745	0.349	ppbv	98
36) Benzene	6.92	78	46394	0.223	ppbv #	91
38) Trichloroethene	7.88	130	1311790	15.368	ppbv	97
39) 1,2-Dichloropropane	7.21	63	597499	7.456	ppbv #	23
42) Bromodichloromethane	7.88	83	10507	0.054	ppbv	92
44) 2,2,4-Trimethylpentane	7.92	57	17737	0.047	ppbv #	1
52) Tetrachloroethene	11.28	164	37076	0.412	ppbv	87
53) Toluene	9.86	91	297287	1.258	ppbv	100
58) Ethyl Benzene	12.76	91	12597	0.040	ppbv	96
59) m/p-Xylene	13.07	91	12609	0.046	ppbv #	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL120219\
Data File : VL034425.D
Acq On : 2 Dec 2019 14:20
Operator : SY/AP
Sample : K6068-01DL 10X
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV-1DL

Quant Time: Dec 03 02:49:12 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL111919AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Nov 19 14:15:35 2019
QLast Update : Tue Nov 19 14:15:35 2019
Response via : Initial Calibration

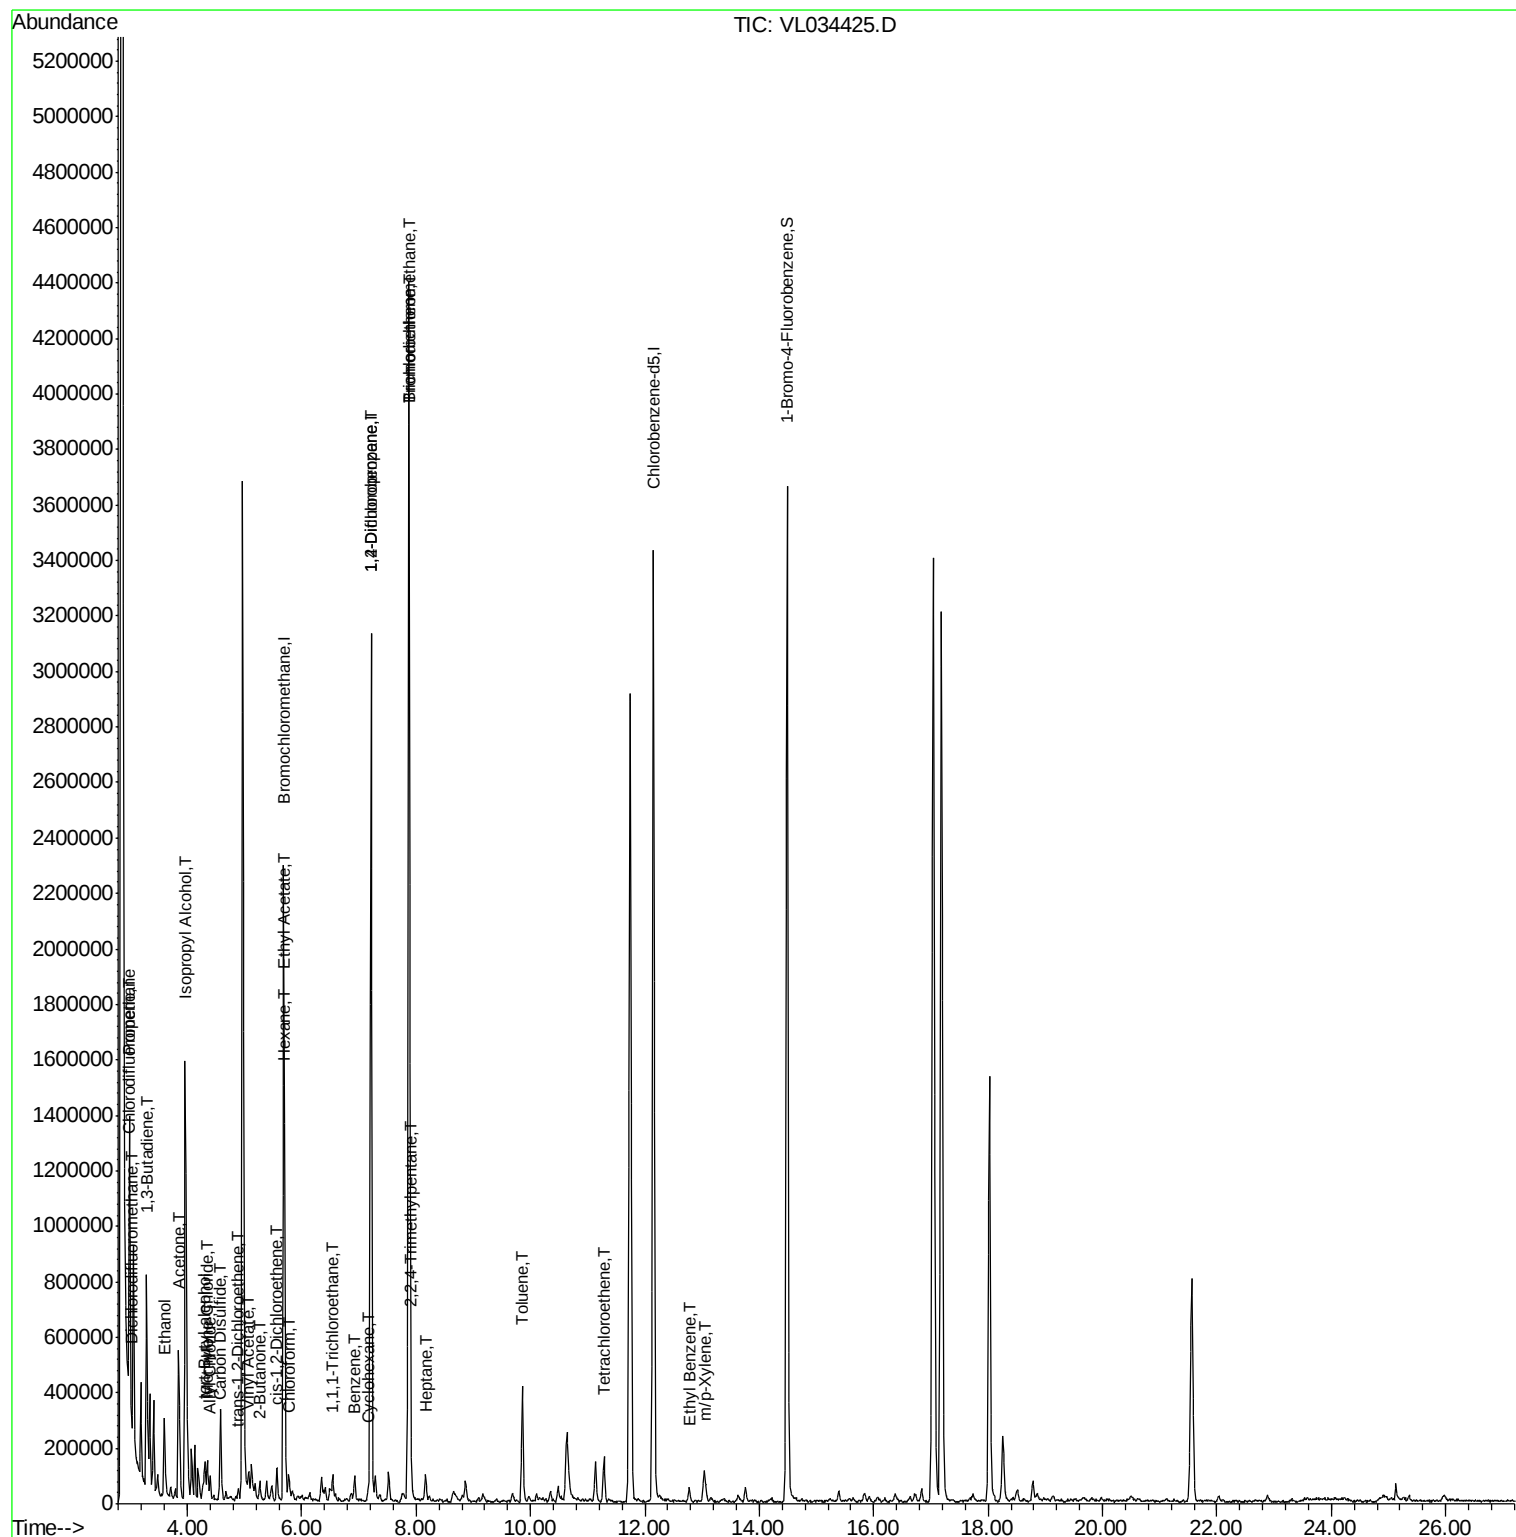

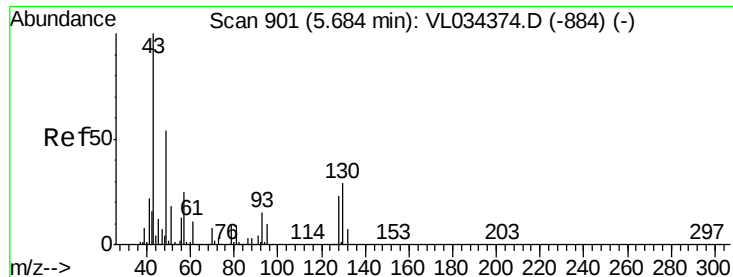

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.69 min Scan# 902

Delta R.T. 0.00 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20

Instrument :

MSVOA_L

ClientSampleId :

SV-1DL


Tgt Ion: 49 Resp: 1015292

Ion Ratio Lower Upper

49 100

128 44.7 21.8 65.3




130 57.0 28.0 84.0

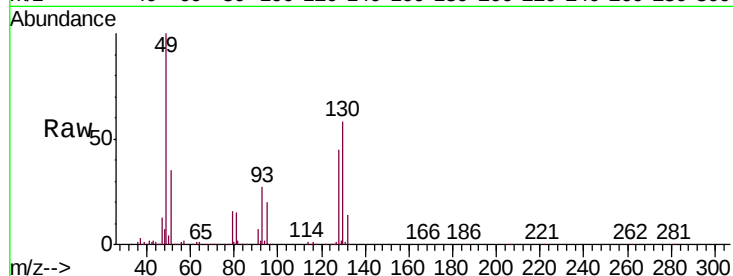

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

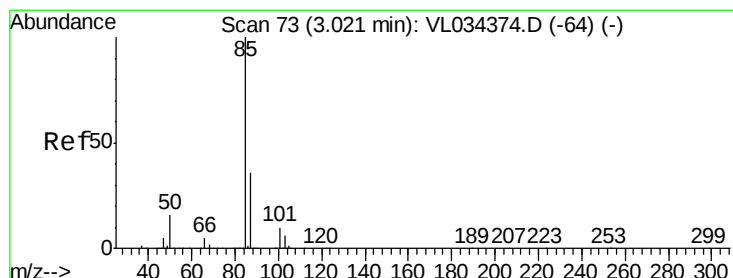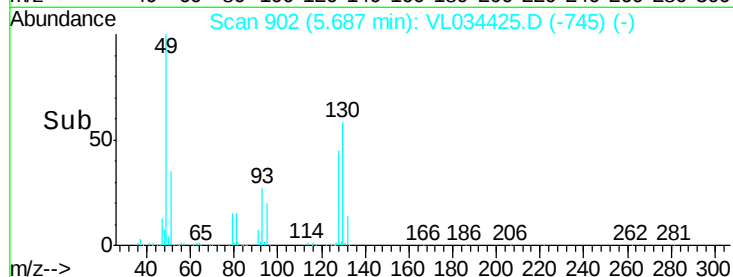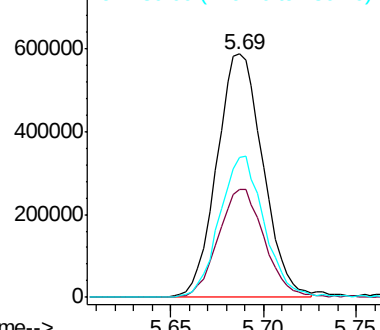

#2

Dichlorodifluoromethane

Concen: 0.080 ppbv

RT: 3.02 min Scan# 74

Delta R.T. 0.00 min

Lab File: VL034425.D


Acq: 2 Dec 2019 14:20

Tgt Ion: 85 Resp: 14674

Ion Ratio Lower Upper



85 100


87 28.5 28.5 42.7

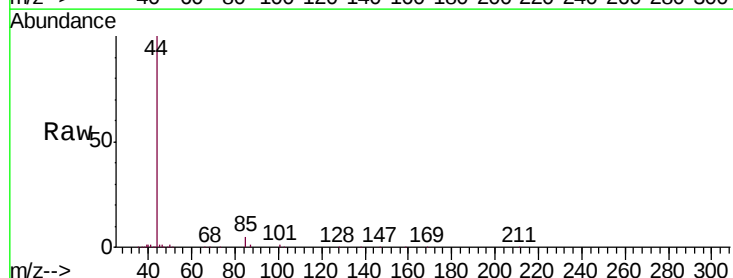

Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0

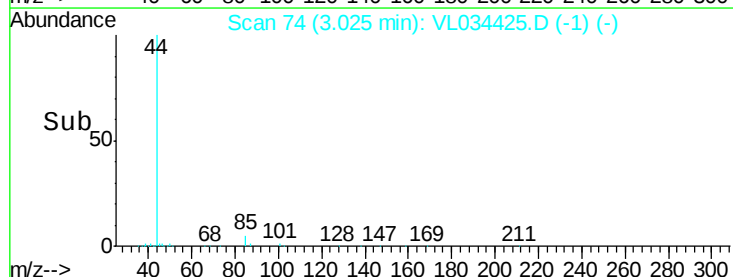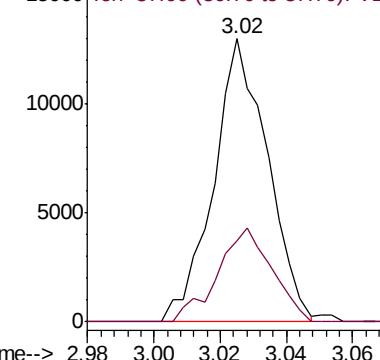

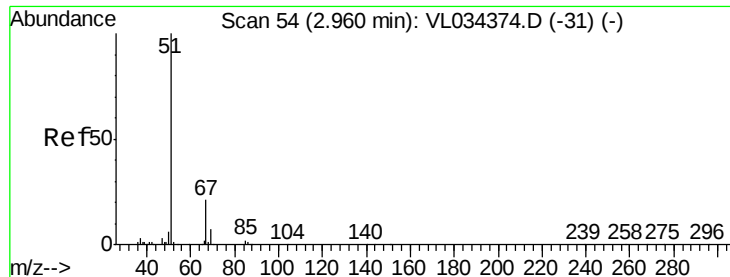

#3

Chlorodifluoromethane

Concen: 0.043 ppbv

RT: 2.97 min Scan# 57

Delta R.T. 0.01 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20

Instrument :

MSVOA_L

ClientSampleId :


SV-1DL

Tgt Ion: 51 Resp: 5501

Ion Ratio Lower Upper




51 100

67 18.1 16.2 24.2

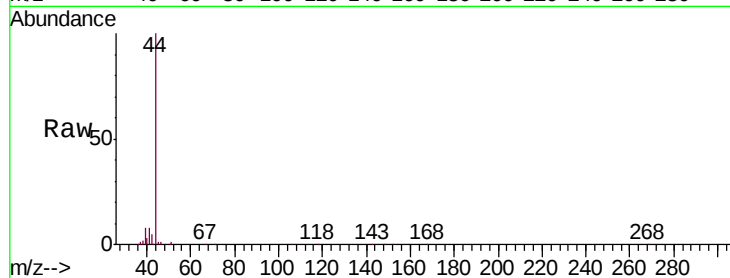

Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

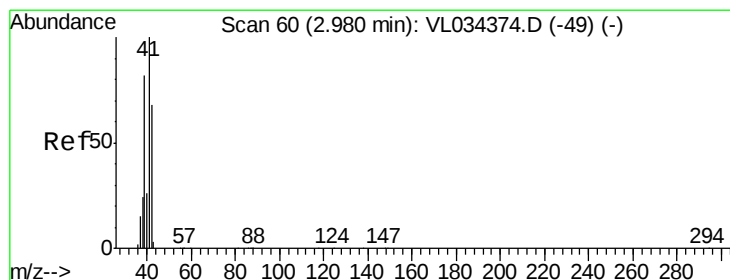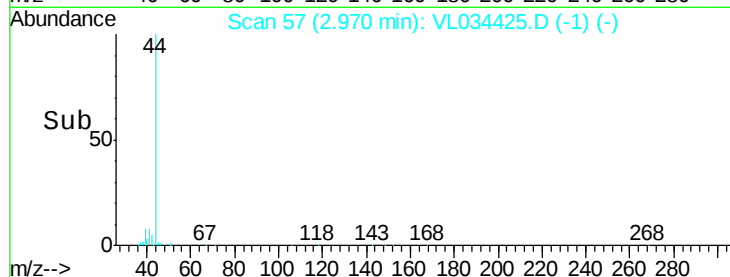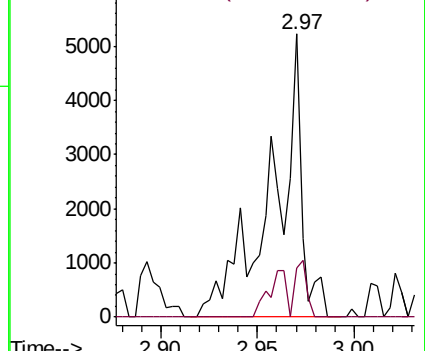

#9

Propene

Concen: 7.430 ppbv

RT: 2.99 min Scan# 62

Delta R.T. 0.01 min

Lab File: VL034425.D


Acq: 2 Dec 2019 14:20

Tgt Ion: 41 Resp: 417870

Ion Ratio Lower Upper



41 100


42 64.5 54.6 82.0

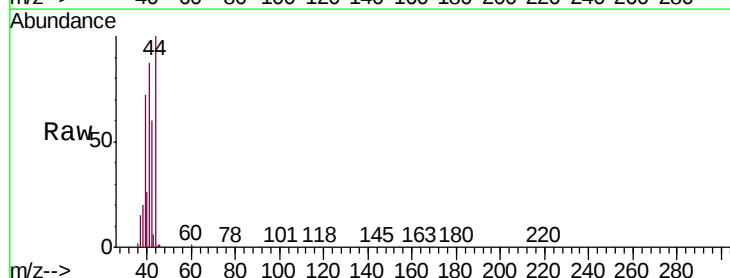

Abundance Ion 41.10 (40.80 to 41.80): VL0

Ion 42.10 (41.80 to 42.80): VL0



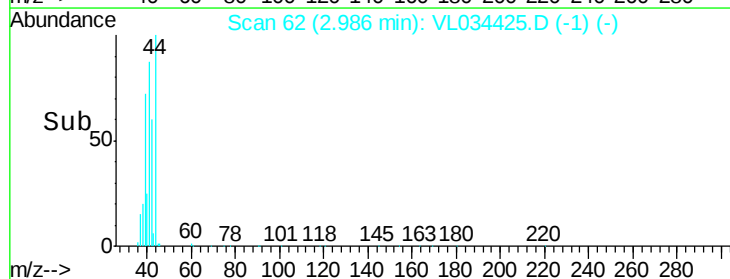
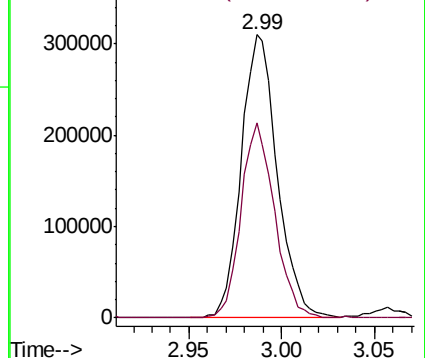


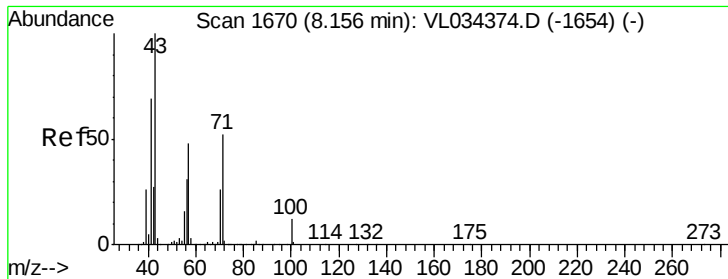

#10
Heptane
Concen: 0.183 ppbv
RT: 8.17 min Scan# 1673
Delta R.T. 0.01 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20




Instrument :
MSVOA_L
ClientSampled :
SV-1DL


Tgt Ion: 43 Resp: 26586
Ion Ratio Lower Upper
43 100
57 77.7 40.2 60.2#

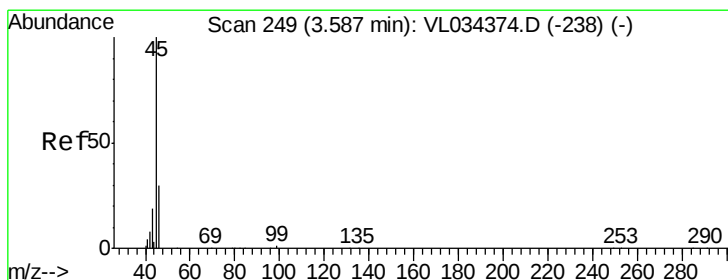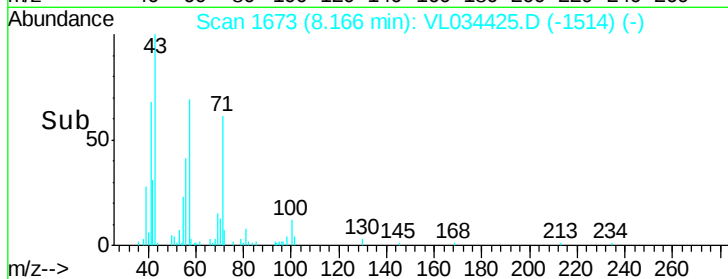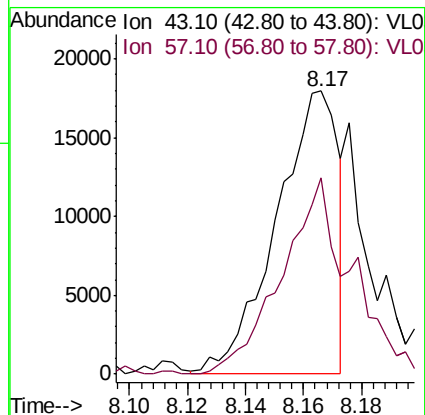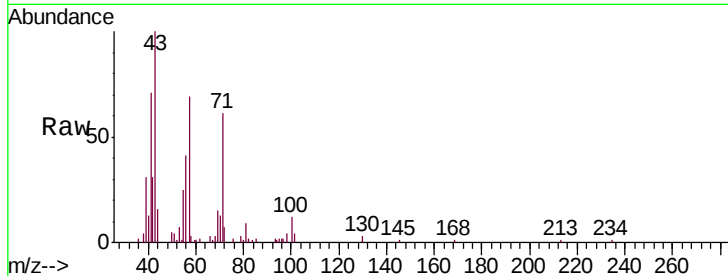

#13
Ethanol
Concen: 17.949 ppbv
RT: 3.59 min Scan# 251
Delta R.T. 0.01 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20

Tgt Ion: 45 Resp: 281194
Ion Ratio Lower Upper
45 100
46 36.1 13.8 55.4

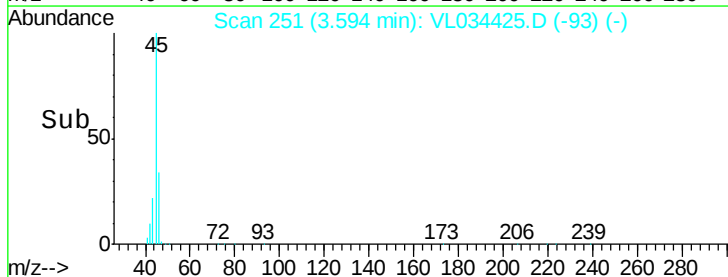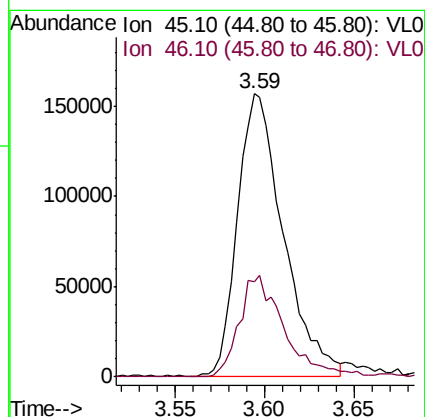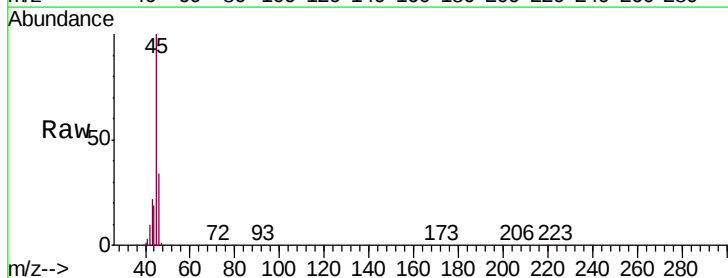



#15

Acetone

Concen: 3.728 ppbv

RT: 3.84 min Scan# 329

Delta R.T. 0.01 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20

Instrument :

MSVOA_L

ClientSampleId :





SV-1DL

Tgt Ion: 43 Resp: 541995

Ion Ratio Lower Upper

43 100

58 26.3 20.2 30.4

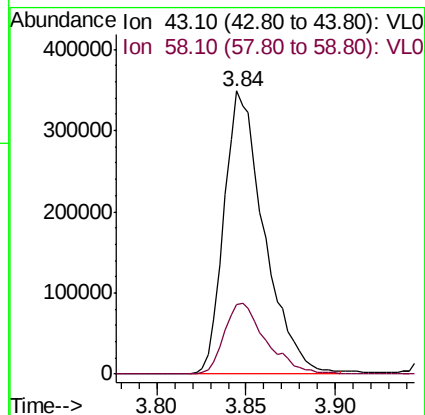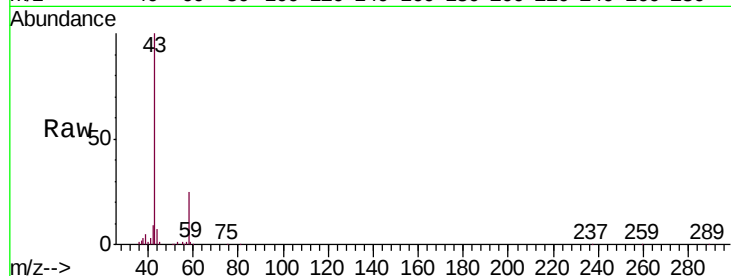

#16

1,3-Butadiene

Concen: 4.042 ppbv

RT: 3.29 min Scan# 157

Delta R.T. -0.01 min

Lab File: VL034425.D




Acq: 2 Dec 2019 14:20


Tgt Ion: 39 Resp: 255976

Ion Ratio Lower Upper

39 100

54 22.4 64.7 97.1#



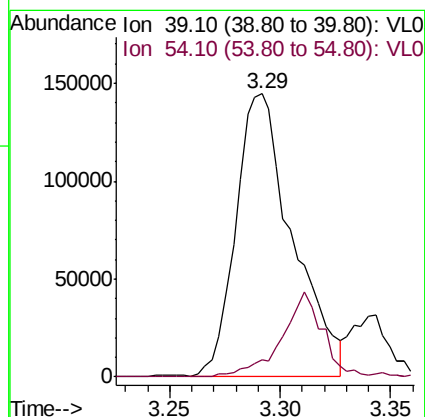



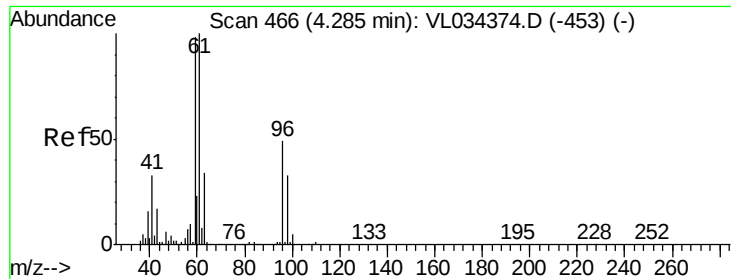

#17
 tert-Butyl alcohol
 Concen: 0.733 ppbv
 RT: 4.30 min Scan# 471
 Delta R.T. 0.02 min
 Lab File: VL034425.D
 Acq: 2 Dec 2019 14:20




Instrument :
 MSVOA_L
 ClientSampleID :
 SV-1DL


Tgt Ion: 59 Resp: 89599
 Ion Ratio Lower Upper
 59 100
 57 12.4 8.8 13.2

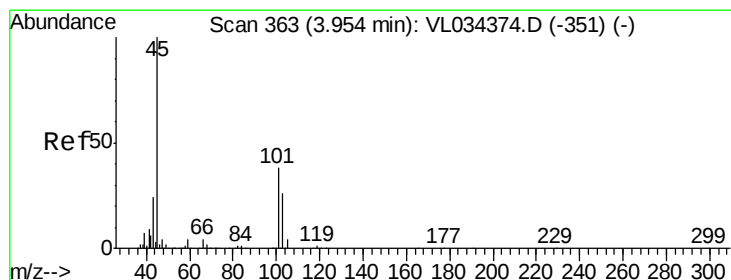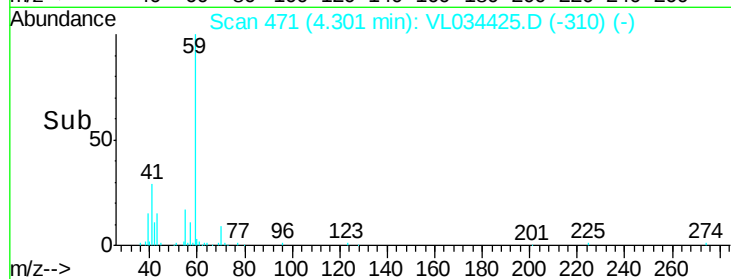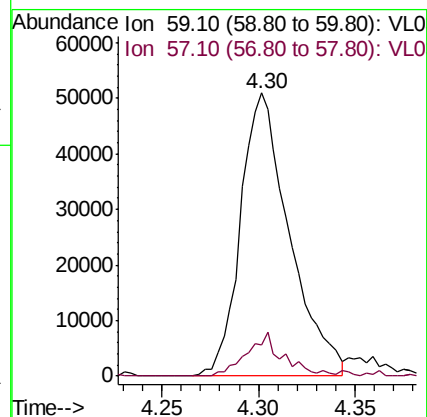

#19
 Isopropyl Alcohol
 Concen: 19.330 ppbv
 RT: 3.96 min Scan# 366
 Delta R.T. 0.01 min
 Lab File: VL034425.D
 Acq: 2 Dec 2019 14:20

Tgt Ion: 45 Resp: 1801304
 Ion Ratio Lower Upper
 45 100
 58 0.9 1.3 1.9#

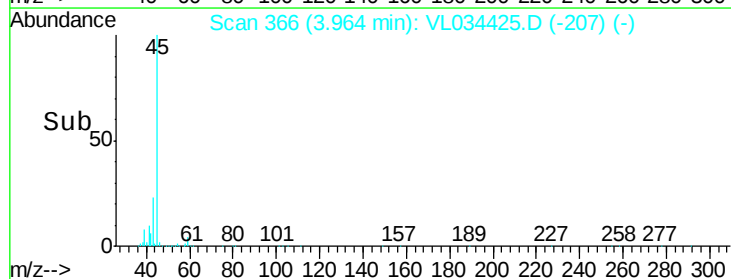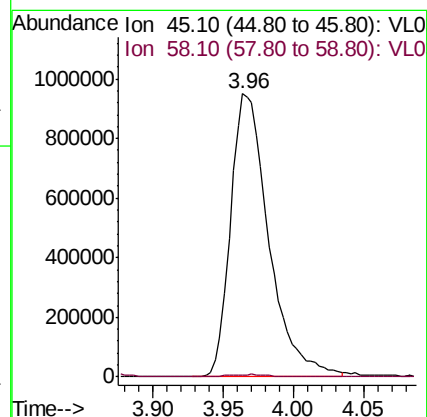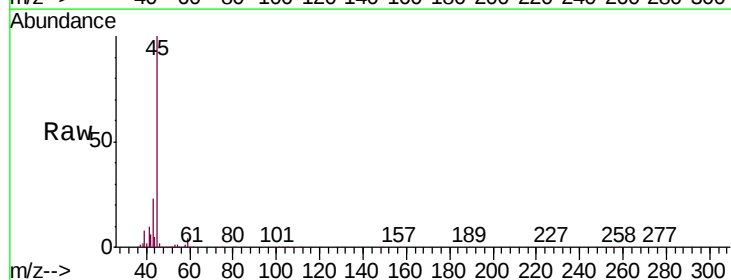







#20
Methylene Chloride
Concen: 0.796 ppbv
RT: 4.35 min Scan# 485
Delta R.T. 0.01 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20

Instrument :
MSVOA_L
ClientSampleId :
SV-1DL

Tgt Ion: 84 Resp: 41053
Ion Ratio Lower Upper
84 100
49 132.1 116.8 175.2
51 35.7 35.6 53.4
86 52.4 50.7 76.1

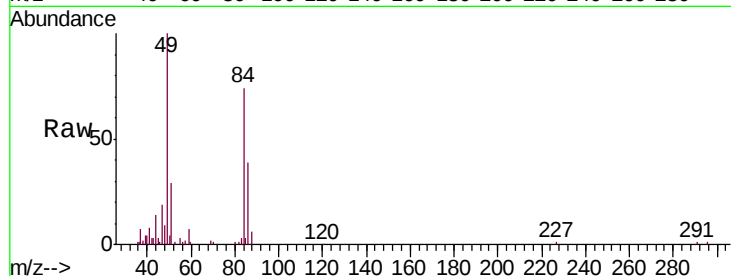


Abundance Ion 84.00 (83.70 to 84.70): VL0
Ion 49.10 (48.80 to 49.80): VL0
Ion 51.10 (50.80 to 51.80): VL0
Ion 86.00 (85.70 to 86.70): VL0


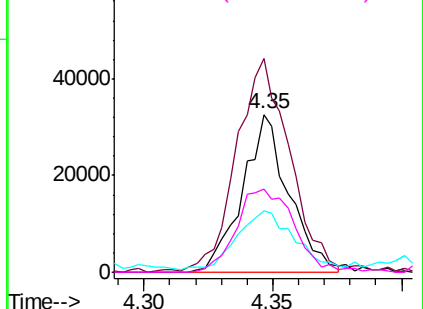



#21
Allyl Chloride
Concen: 0.035 ppbv
RT: 4.40 min Scan# 503
Delta R.T. -0.00 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20

Tgt Ion: 41 Resp: 3040
Ion Ratio Lower Upper
41 100
76 0.0 24.2 36.2#
39 992.4 66.9 100.3#



Abundance Ion 41.10 (40.80 to 41.80): VL0
Ion 76.10 (75.80 to 76.80): VL0
Ion 39.10 (38.80 to 39.80): VL0

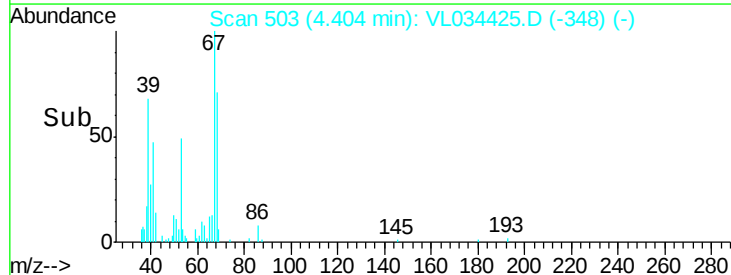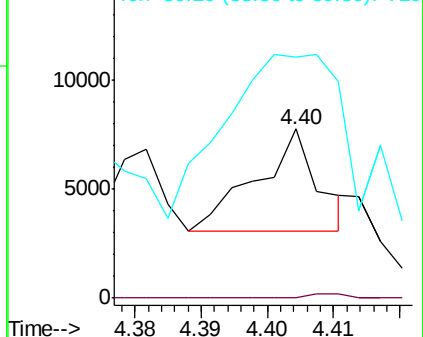

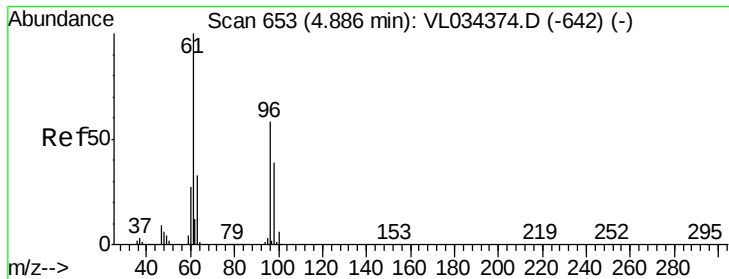

#22

trans-1,2-Dichloroethene

Concen: 0.042 ppbv

RT: 4.89 min Scan# 653

Delta R.T. 0.00 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20

Instrument :

MSVOA_L

ClientSampleId :

SV-1DL





Tgt Ion: 96 Resp: 2245

Ion Ratio Lower Upper

96 100

61 172.7 137.9 206.9

98 97.0 53.5 80.3#

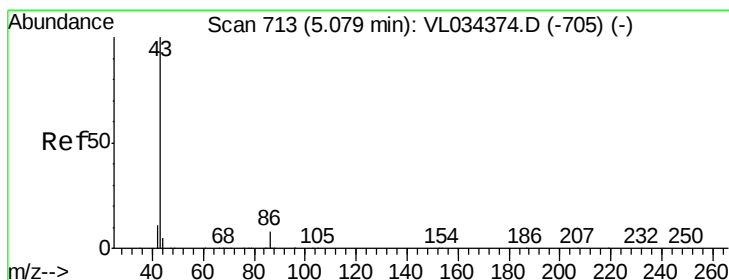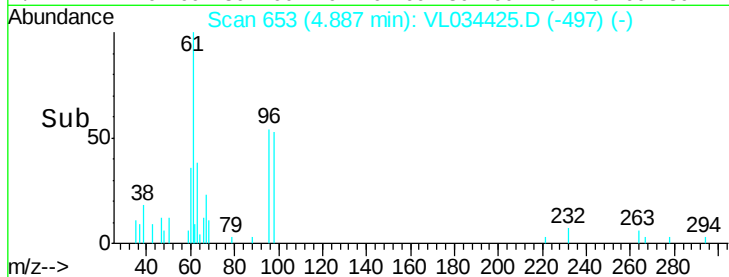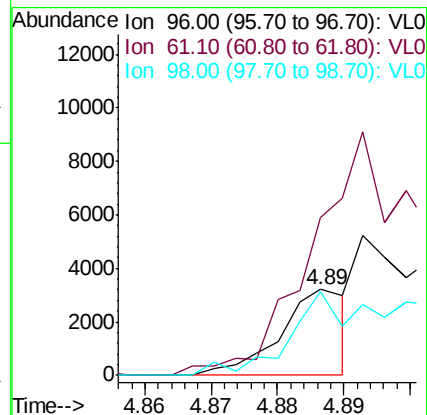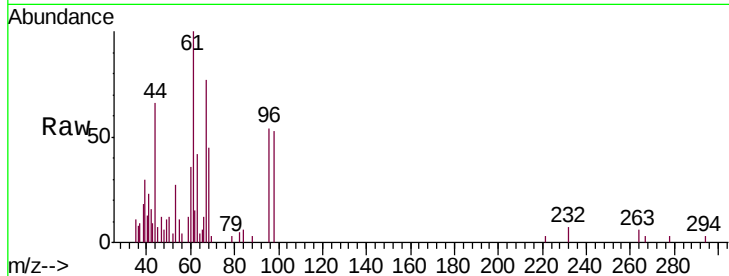

#23

Vinyl Acetate

Concen: 0.070 ppbv

RT: 5.08 min Scan# 713

Delta R.T. 0.00 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20

Tgt Ion: 43 Resp: 13262




Ion Ratio Lower Upper


43 100

86 11.3 5.8 8.6#

42 73.8 8.9 13.3#

44 16.9 4.0 6.0#


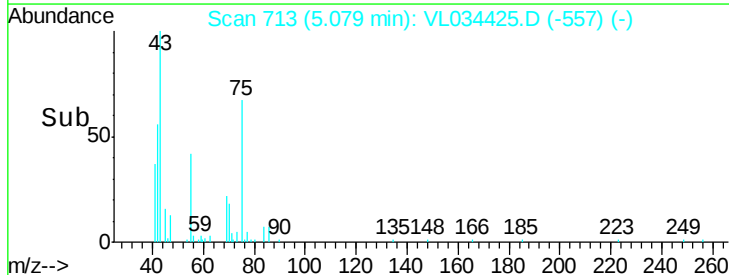
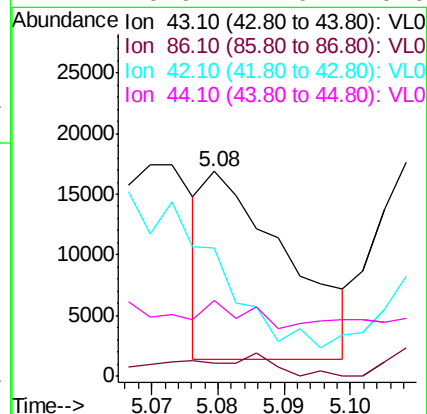
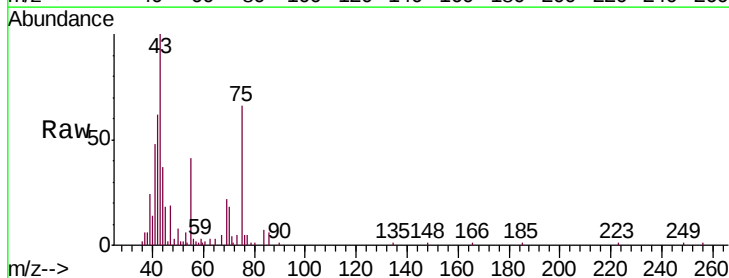




#25
Ethyl Acetate
Concen: 0.218 ppbv
RT: 5.71 min Scan# 908
Delta R.T. 0.02 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20




Instrument :
MSVOA_L
ClientSampleId :
SV-1DL


Tgt Ion:	43	Resp:	56617
Ion	Ratio	Lower	Upper
43	100		
45	8.4	8.2	12.4
61	4.1	7.5	11.3#
70	4.0	5.7	8.5#

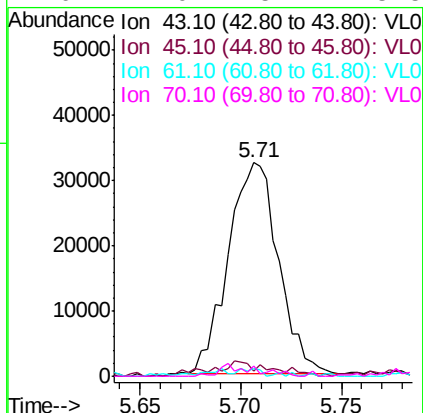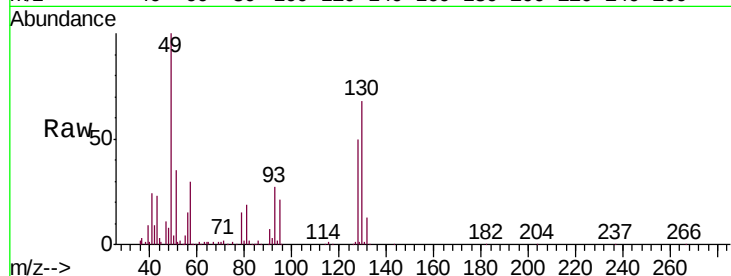

#26
Hexane
Concen: 0.632 ppbv
RT: 5.71 min Scan# 909
Delta R.T. 0.01 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20

Tgt Ion:	57	Resp:	70411
Ion	Ratio	Lower	Upper
57	100		
41	99.8	75.0	112.4
43	83.7	186.6	279.8#
56	57.5	41.5	62.3

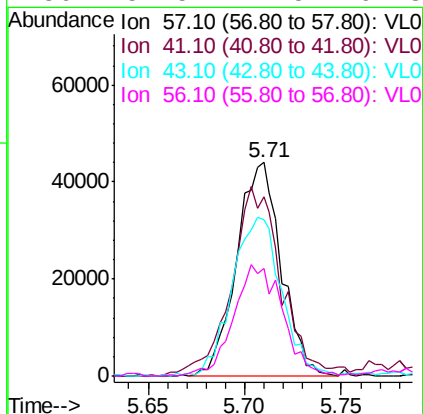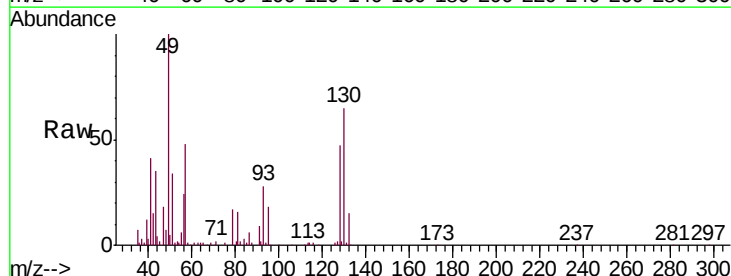

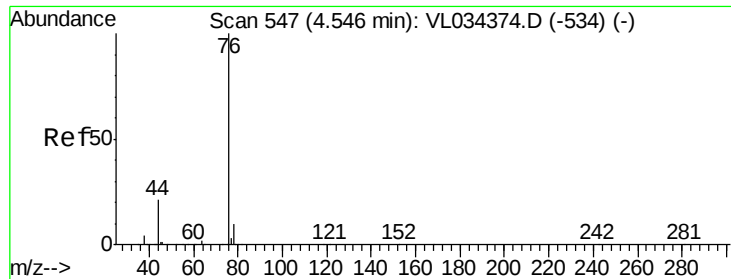

#27

Carbon Disulfide

Concen: 0.042 ppbv

RT: 4.56 min Scan# 550

Delta R.T. 0.01 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20

Instrument :

MSVOA_L

ClientSampled :

SV-1DL


Tgt Ion: 76 Resp: 5098

Ion Ratio Lower Upper

76 100

44 170.6 17.0 25.4#




78 38.0 7.6 11.4#

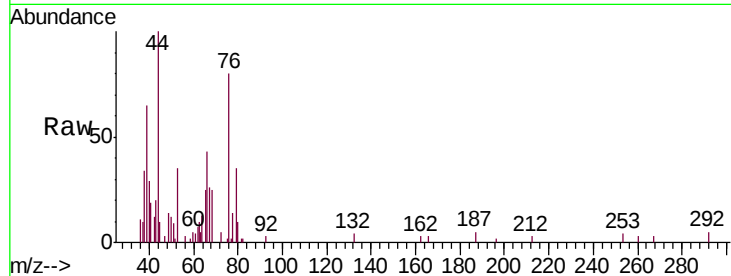

Abundance Ion 76.00 (75.70 to 76.70): VL0

Ion 44.10 (43.80 to 44.80): VL0

Ion 78.00 (77.70 to 78.70): VL0

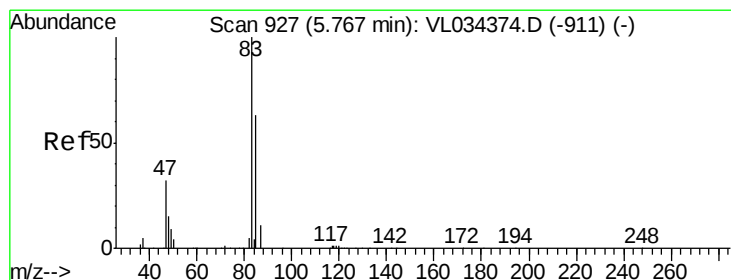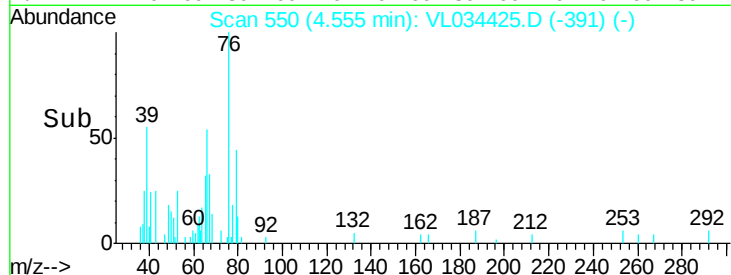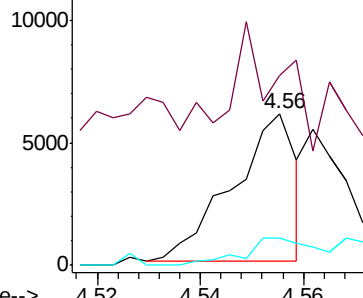

#29

Chloroform

Concen: 0.117 ppbv

RT: 5.77 min Scan# 927

Delta R.T. 0.00 min

Lab File: VL034425.D


Acq: 2 Dec 2019 14:20

Tgt Ion: 83 Resp: 21059

Ion Ratio Lower Upper



83 100


85 55.4 50.4 75.6



Abundance Ion 83.00 (82.70 to 83.70): VL0

Ion 85.00 (84.70 to 85.70): VL0




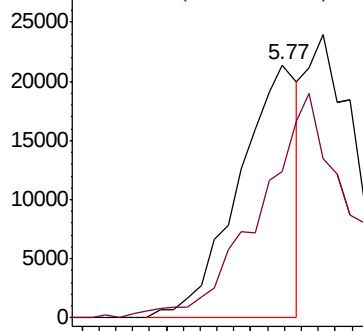


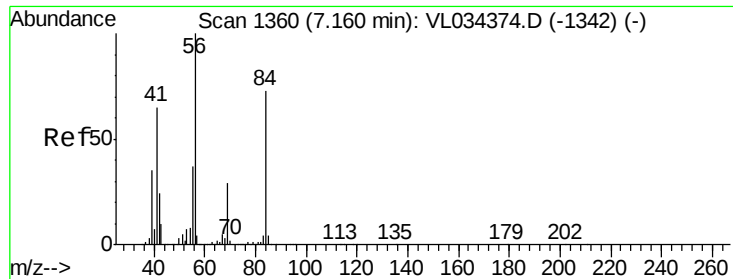

#30
Cyclohexane
Concen: 0.034 ppbv
RT: 7.16 min Scan# 1361
Delta R.T. 0.00 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20




Instrument :
MSVOA_L
ClientSampleId :
SV-1DL


Tgt Ion: 84 Resp: 2837
Ion Ratio Lower Upper
84 100
56 0.0 112.6 169.0#
41 509.1 73.4 110.2#

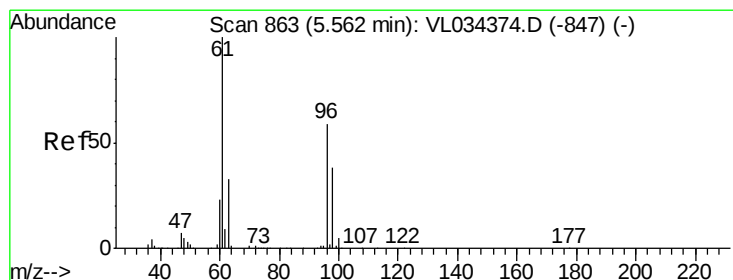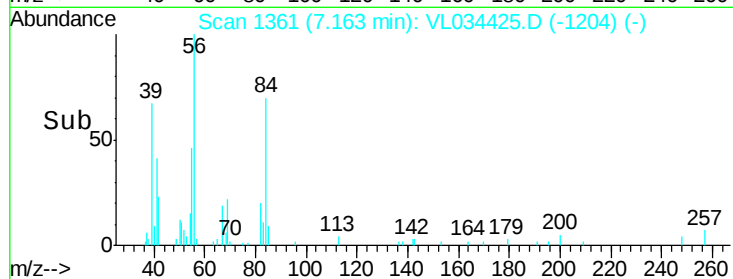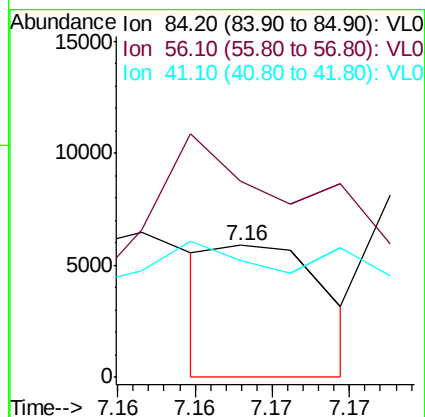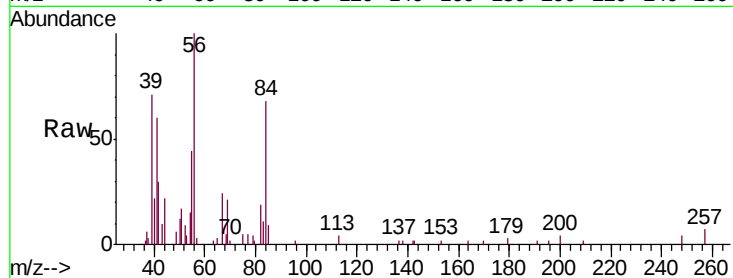

#31
cis-1,2-Dichloroethene
Concen: 0.531 ppbv
RT: 5.56 min Scan# 864
Delta R.T. 0.00 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20

Tgt Ion: 61 Resp: 61184
Ion Ratio Lower Upper
61 100
96 57.2 47.4 71.2
98 27.5 30.6 45.8#

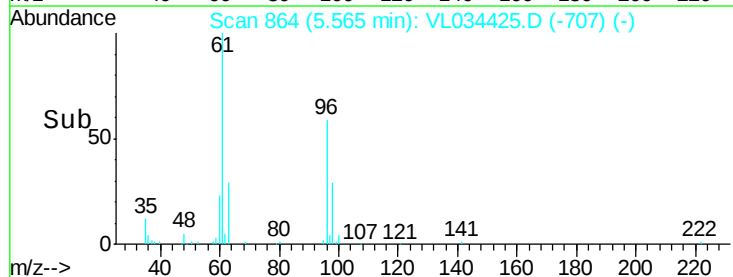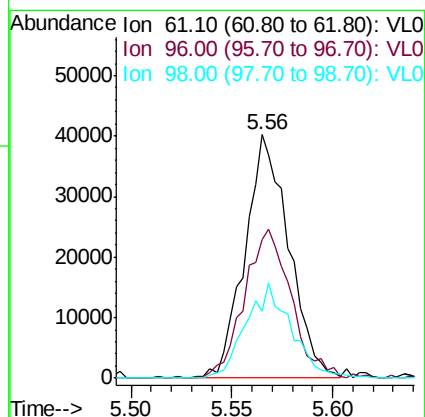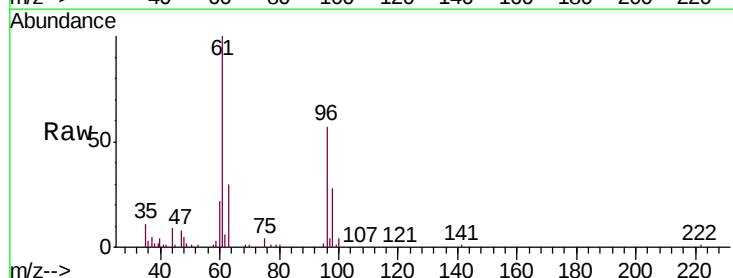



#32

1,1,1-Trichloroethane

Concen: 0.296 ppbv

RT: 6.54 min Scan# 1168

Delta R.T. 0.01 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20

Instrument :

MSVOA_L

ClientSampleId :

SV-1DL


Tgt Ion: 97 Resp: 50152

Ion Ratio Lower Upper




97 100

99 64.9 52.3 78.5

61 56.2 43.7 65.5



Abundance Ion 97.00 (96.70 to 97.70): VL0
Ion 99.00 (98.70 to 99.70): VL0
Ion 61.10 (60.80 to 61.80): VL0

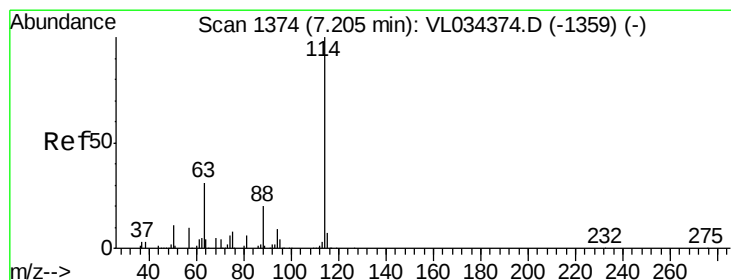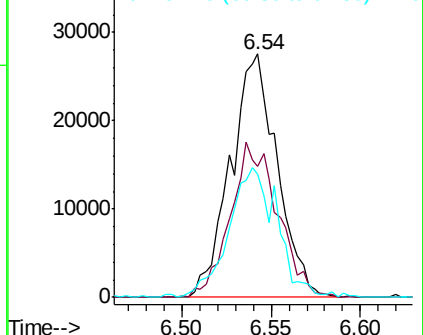

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.21 min Scan# 1376

Delta R.T. 0.01 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20


Tgt Ion: 114 Resp: 2080730

Ion Ratio Lower Upper



114 100


63 28.9 24.2 36.4

88 20.0 15.9 23.9



Abundance Ion 114.10 (113.80 to 114.80): V
Ion 63.10 (62.80 to 63.80): VL0
Ion 88.10 (87.80 to 88.80): VL0




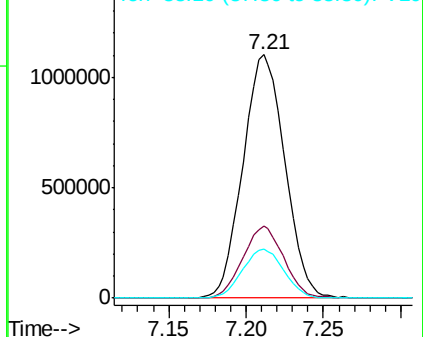


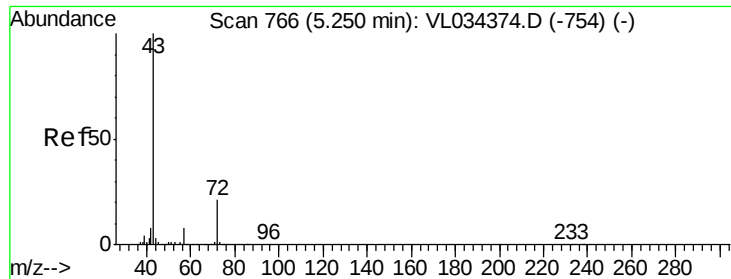

#34
2-Butanone
Concen: 0.349 ppbv
RT: 5.27 min Scan# 771
Delta R.T. 0.02 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20




Instrument :
MSVOA_L
ClientSampleId :
SV-1DL


Tgt Ion: 43 Resp: 59745
Ion Ratio Lower Upper
43 100
72 20.3 17.0 25.6

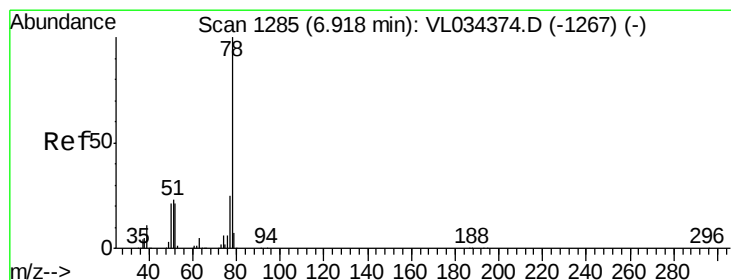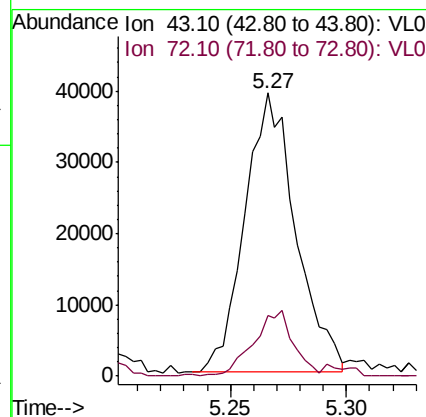

#36
Benzene
Concen: 0.223 ppbv
RT: 6.92 min Scan# 1286
Delta R.T. 0.00 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20

Tgt Ion: 78 Resp: 46394
Ion Ratio Lower Upper
78 100
77 19.5 20.2 30.4#
50 18.7 17.1 25.7

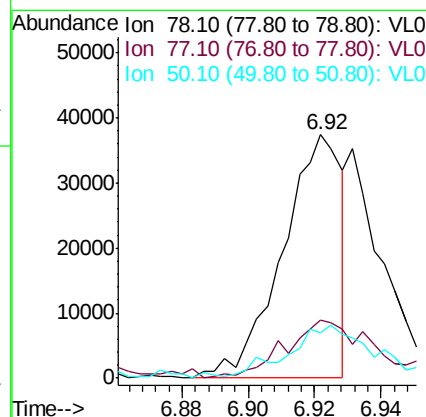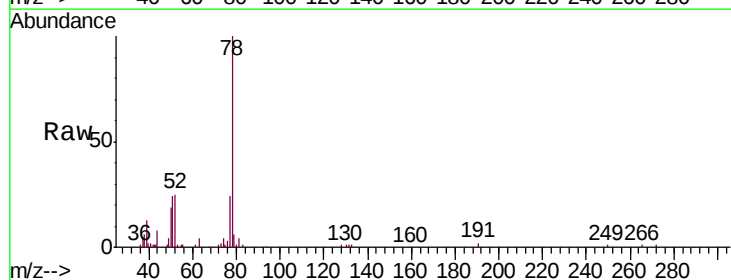



#38

Trichloroethene

Concen: 15.368 ppbv

RT: 7.88 min Scan# 1584

Delta R.T. 0.01 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20

Instrument :

MSVOA_L

ClientSampleId :

SV-1DL

Tgt Ion:130 Resp: 1311790


Ion Ratio Lower Upper

130 100

95 113.9 93.4 140.0

132 93.8 76.4 114.6

97 73.0 61.1 91.7



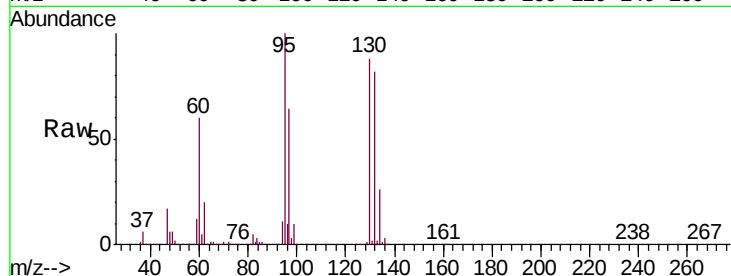


Abundance Ion 130.00 (129.70 to 130.70): V

Ion 95.00 (94.70 to 95.70): VL0

Ion 132.00 (131.70 to 132.70): V

Ion 97.00 (96.70 to 97.70): VL0

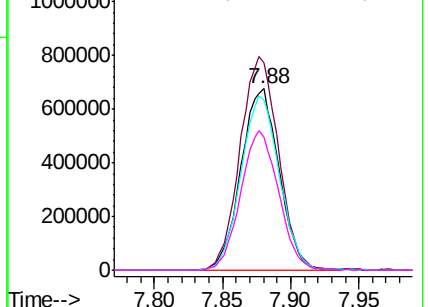

#39

1,2-Dichloropropane

Concen: 7.456 ppbv

RT: 7.21 min Scan# 1376

Delta R.T. -0.44 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20


Tgt Ion: 63 Resp: 597499

Ion Ratio Lower Upper

63 100

41 0.0 63.1 94.7#



62 17.4 52.3 78.5#




Abundance Ion 63.10 (62.80 to 63.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 62.10 (61.80 to 62.80): VL0

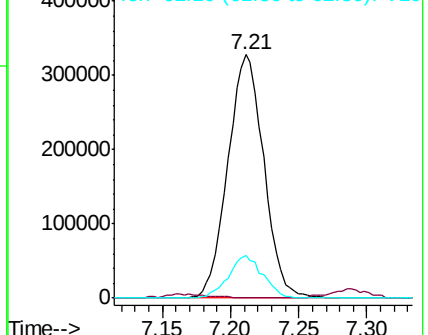

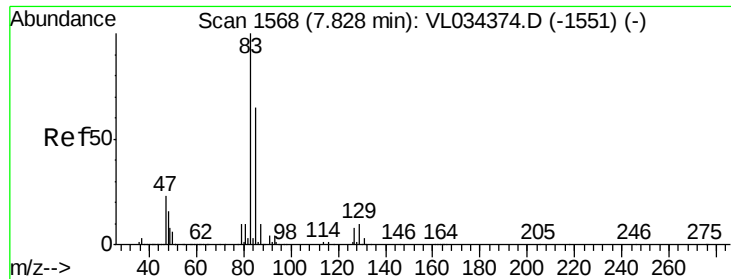

#42

Bromodichloromethane

Concen: 0.054 ppbv

RT: 7.88 min Scan# 1584

Delta R.T. 0.05 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20

Instrument :

MSVOA_L

ClientSampleId :

SV-1DL





Tgt Ion: 83 Resp: 10507

Ion Ratio Lower Upper

83 100

85 58.7 52.3 78.5

127 7.8 6.1 9.1

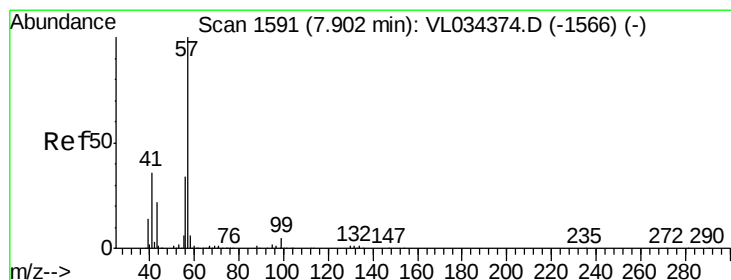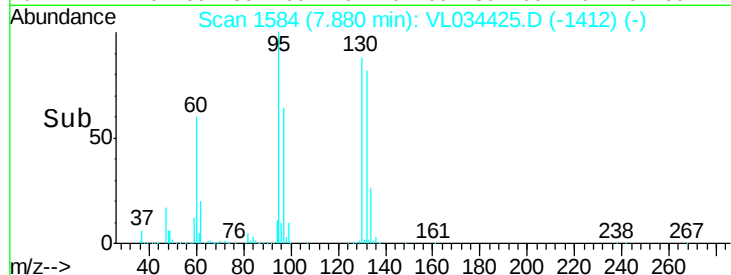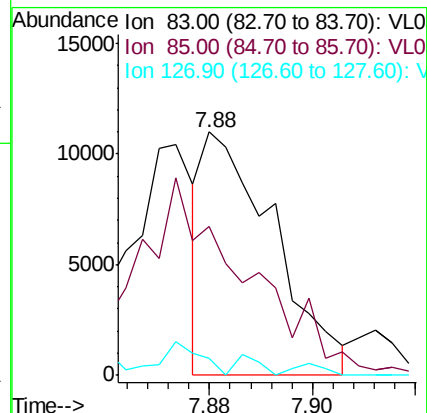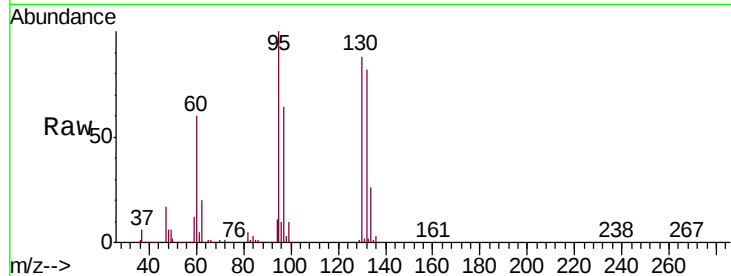

#44

2,2,4-Trimethylpentane

Concen: 0.047 ppbv

RT: 7.92 min Scan# 1595

Delta R.T. 0.01 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20




Tgt Ion: 57 Resp: 17737


Ion Ratio Lower Upper

57 100

41 160.2 28.6 42.8#

56 143.0 25.3 37.9#

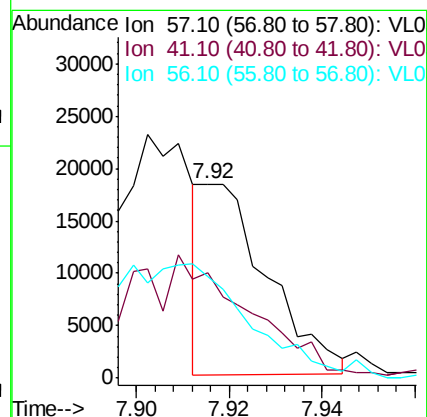

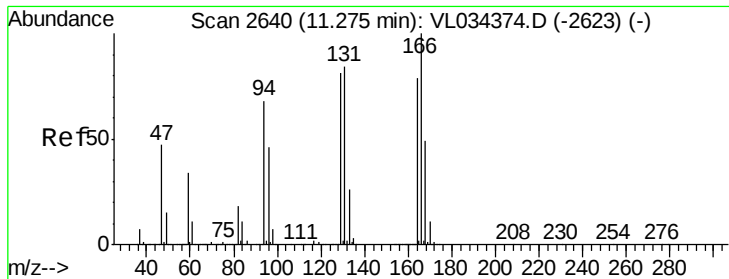

#52

Tetrachloroethene

Concen: 0.412 ppbv

RT: 11.28 min Scan# 2643

Delta R.T. 0.01 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20

Instrument :

MSVOA_L

ClientSampleId :

SV-1DL

Tgt Ion:164 Resp: 37076


Ion Ratio Lower Upper

164 100

166 110.3 101.7 152.5

129 98.1 82.6 123.8

131 87.7 85.2 127.8



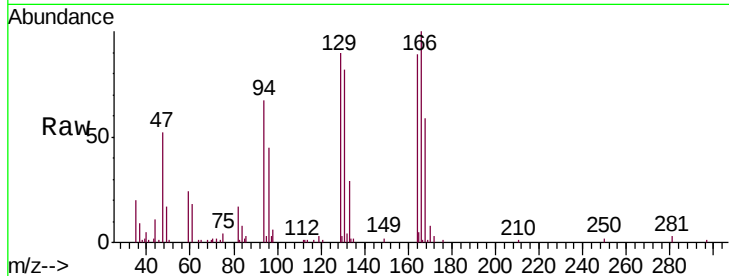


Abundance Ion 163.90 (163.60 to 164.60): V

Ion 165.90 (165.60 to 166.60): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

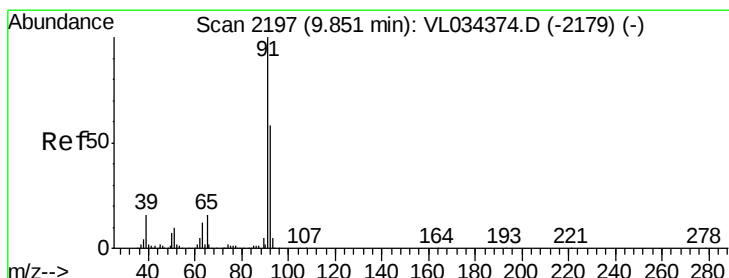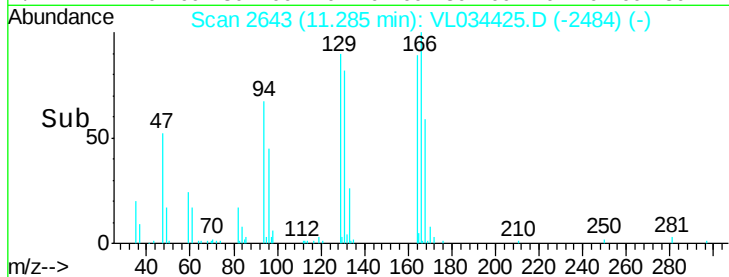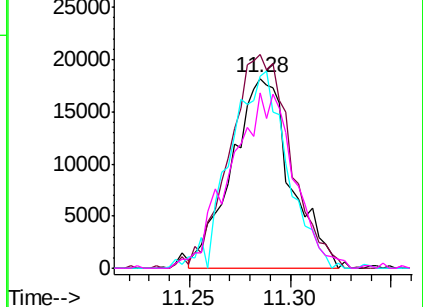

#53

Toluene

Concen: 1.258 ppbv

RT: 9.86 min Scan# 2200

Delta R.T. 0.01 min

Lab File: VL034425.D


Acq: 2 Dec 2019 14:20

Tgt Ion: 91 Resp: 297287

Ion Ratio Lower Upper



91 100


92 59.7 47.9 71.9

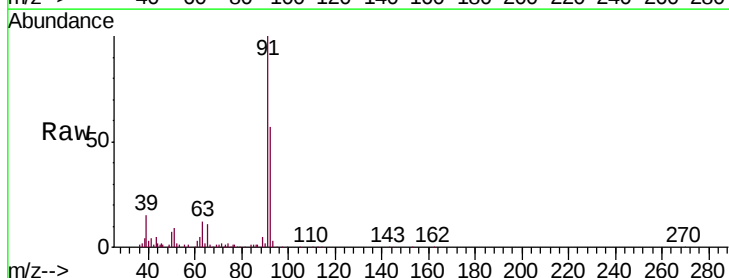

Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 92.10 (91.80 to 92.80): VL0

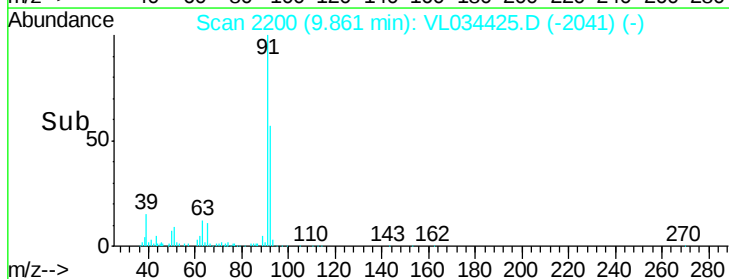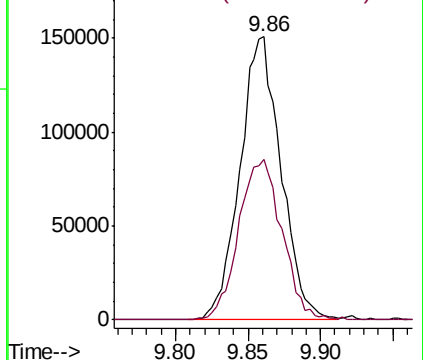

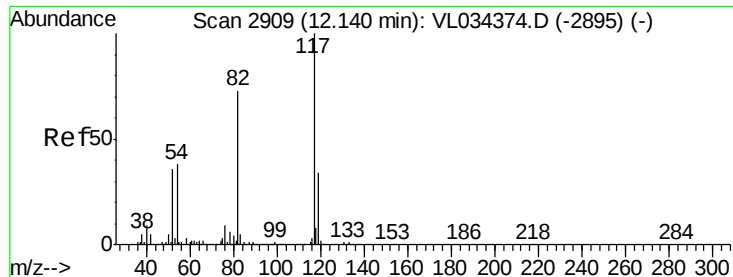

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.15 min Scan# 2912

Delta R.T. 0.01 min

Lab File: VL034425.D

Acq: 2 Dec 2019 14:20

Instrument :

MSVOA_L

ClientSampleId :

SV-1DL


Tgt Ion:117 Resp: 2048190

Ion Ratio Lower Upper

117 100

82 70.7 57.5 86.3




119 32.6 25.4 38.2

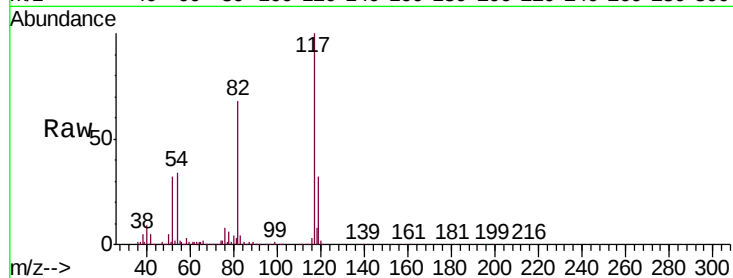

Abundance Ion 117.10 (116.80 to 117.80): V

Ion 82.10 (81.80 to 82.80): VL0

Ion 119.10 (118.80 to 119.80): V

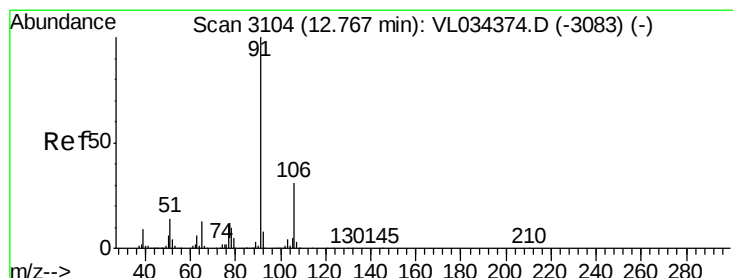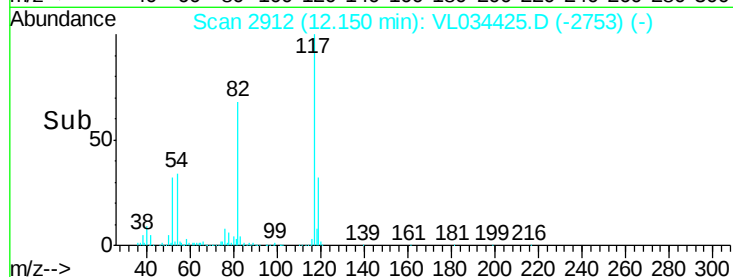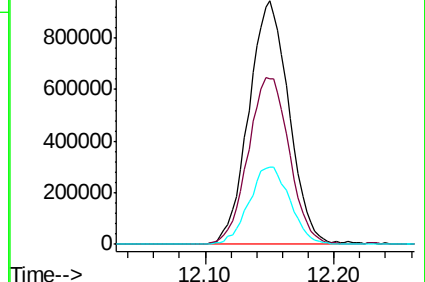

#58

Ethyl Benzene

Concen: 0.040 ppbv

RT: 12.76 min Scan# 3103

Delta R.T. -0.00 min

Lab File: VL034425.D


Acq: 2 Dec 2019 14:20

Tgt Ion: 91 Resp: 12597

Ion Ratio Lower Upper



91 100


106 28.9 24.8 37.2

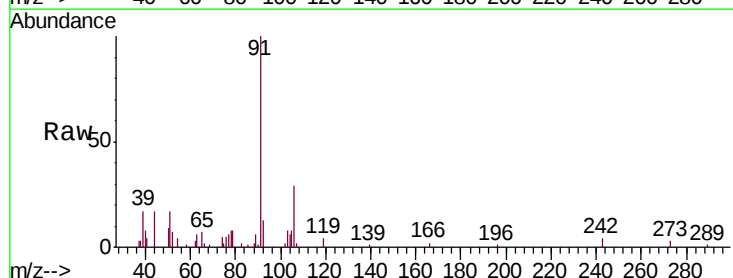

Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 106.10 (105.80 to 106.80): V



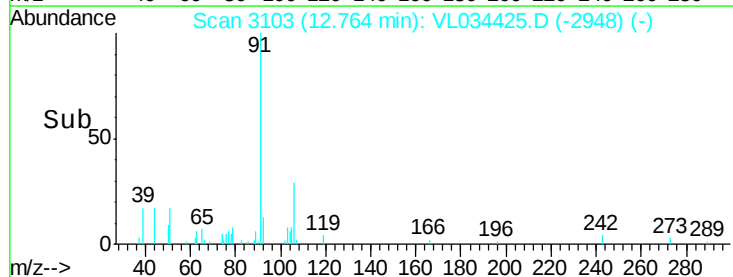
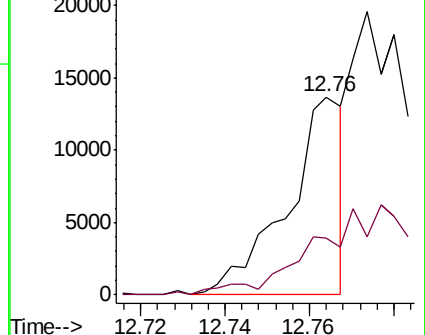


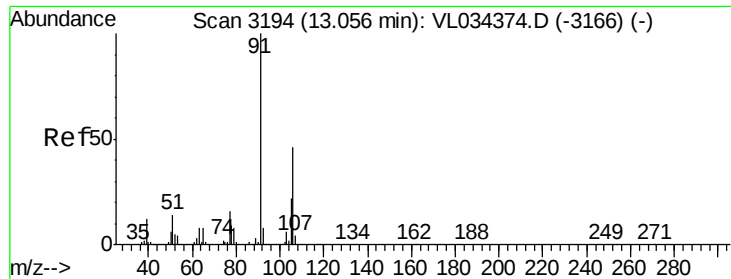

#59
m/p-Xylene
Concen: 0.046 ppbv
RT: 13.07 min Scan# 3197
Delta R.T. 0.01 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20

Instrument :
MSVOA_L
ClientSampleID :
SV-1DL

Tgt Ion: 91 Resp: 12609
Ion Ratio Lower Upper
91 100
106 0.0 34.6 51.8#

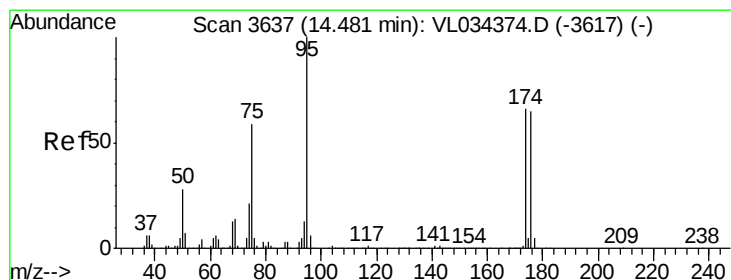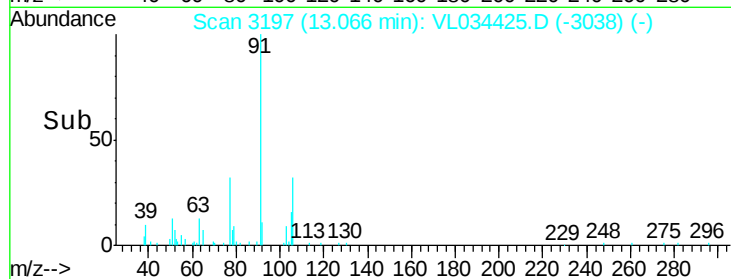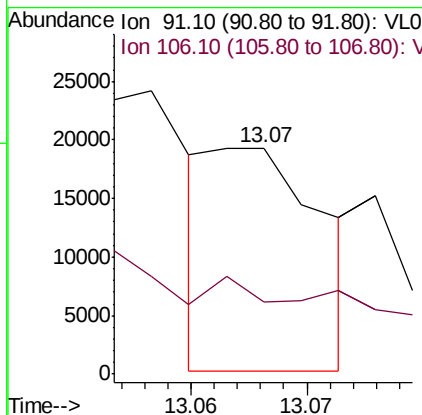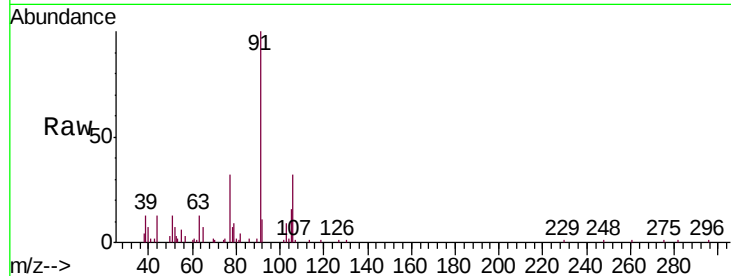

#68
1-Bromo-4-Fluorobenzene
Concen: 9.870 ppbv
RT: 14.48 min Scan# 3638
Delta R.T. 0.00 min
Lab File: VL034425.D
Acq: 2 Dec 2019 14:20

Tgt Ion: 95 Resp: 1700653
Ion Ratio Lower Upper
95 100
174 66.2 52.2 78.2
175 4.9 3.8 5.8

