


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL120219\
 Data File : VL034420.D
 Acq On : 2 Dec 2019 8:46
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111919AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Nov 19 14:15:35 2019
 Last Update : Tue Nov 19 14:15:35 2019

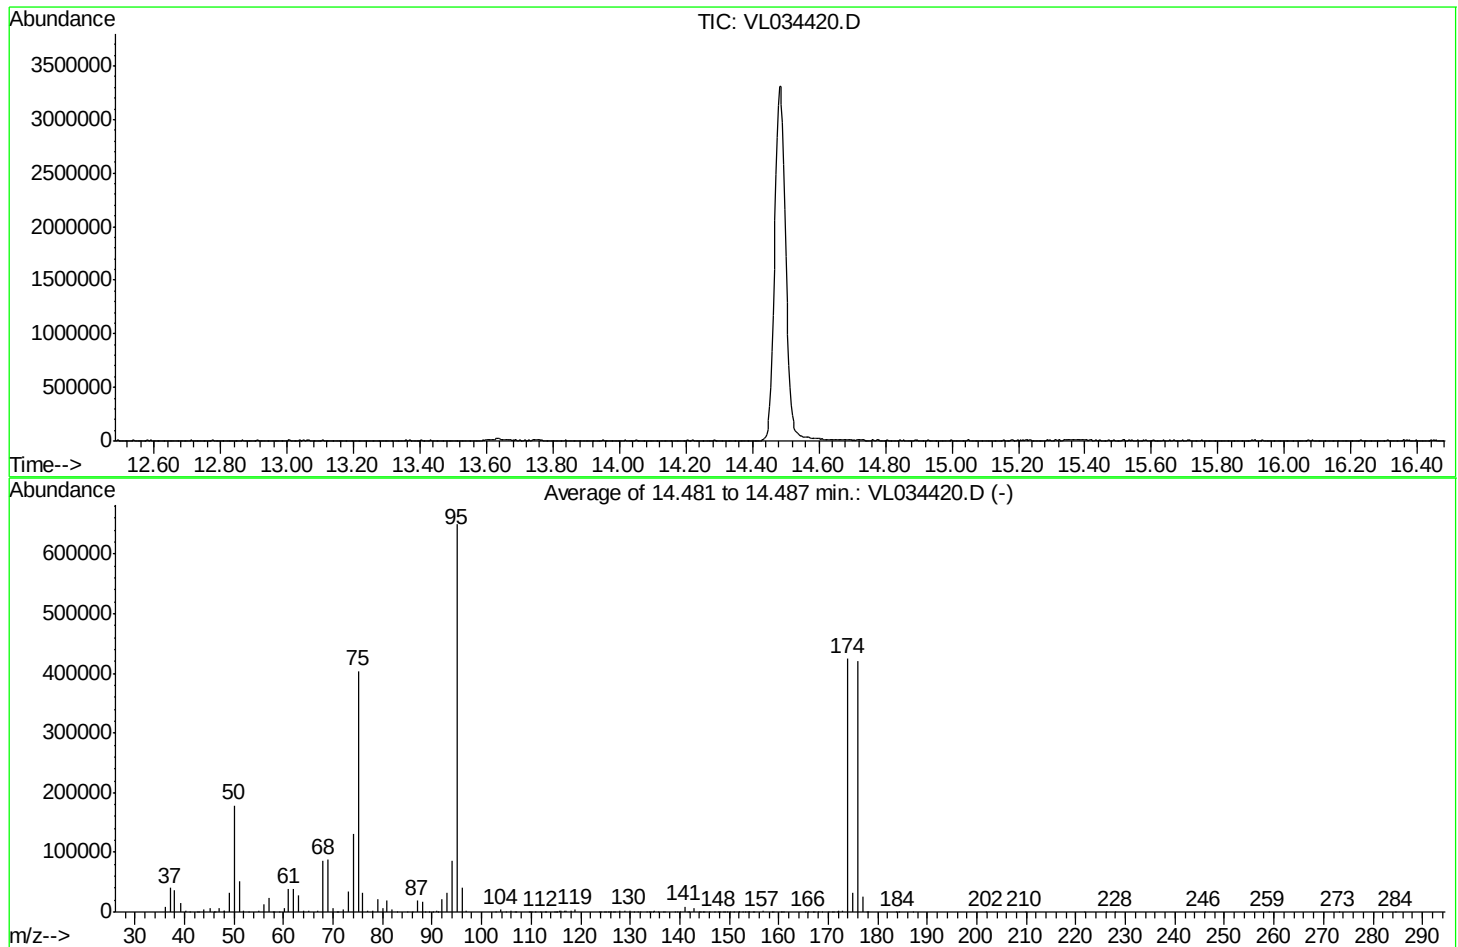

AutoFind: Scans 3637, 3638, 3639; Background Corrected with Scan 3615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.5	179029	PASS
75	95	30	66	62.2	404522	PASS
95	95	100	100	100.0	649877	PASS
96	95	5	9	6.4	41389	PASS
173	174	0.00	2	0.6	2696	PASS
174	95	50	120	65.3	424490	PASS
175	174	4	9	7.6	32317	PASS
176	174	93	101	99.2	421013	PASS
177	176	5	9	6.2	26304	PASS