


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL120222\
Data File : VL039963.D
Acq On : 2 Dec 2022 9:52
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111822AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Dec 02 23:21:36 2022

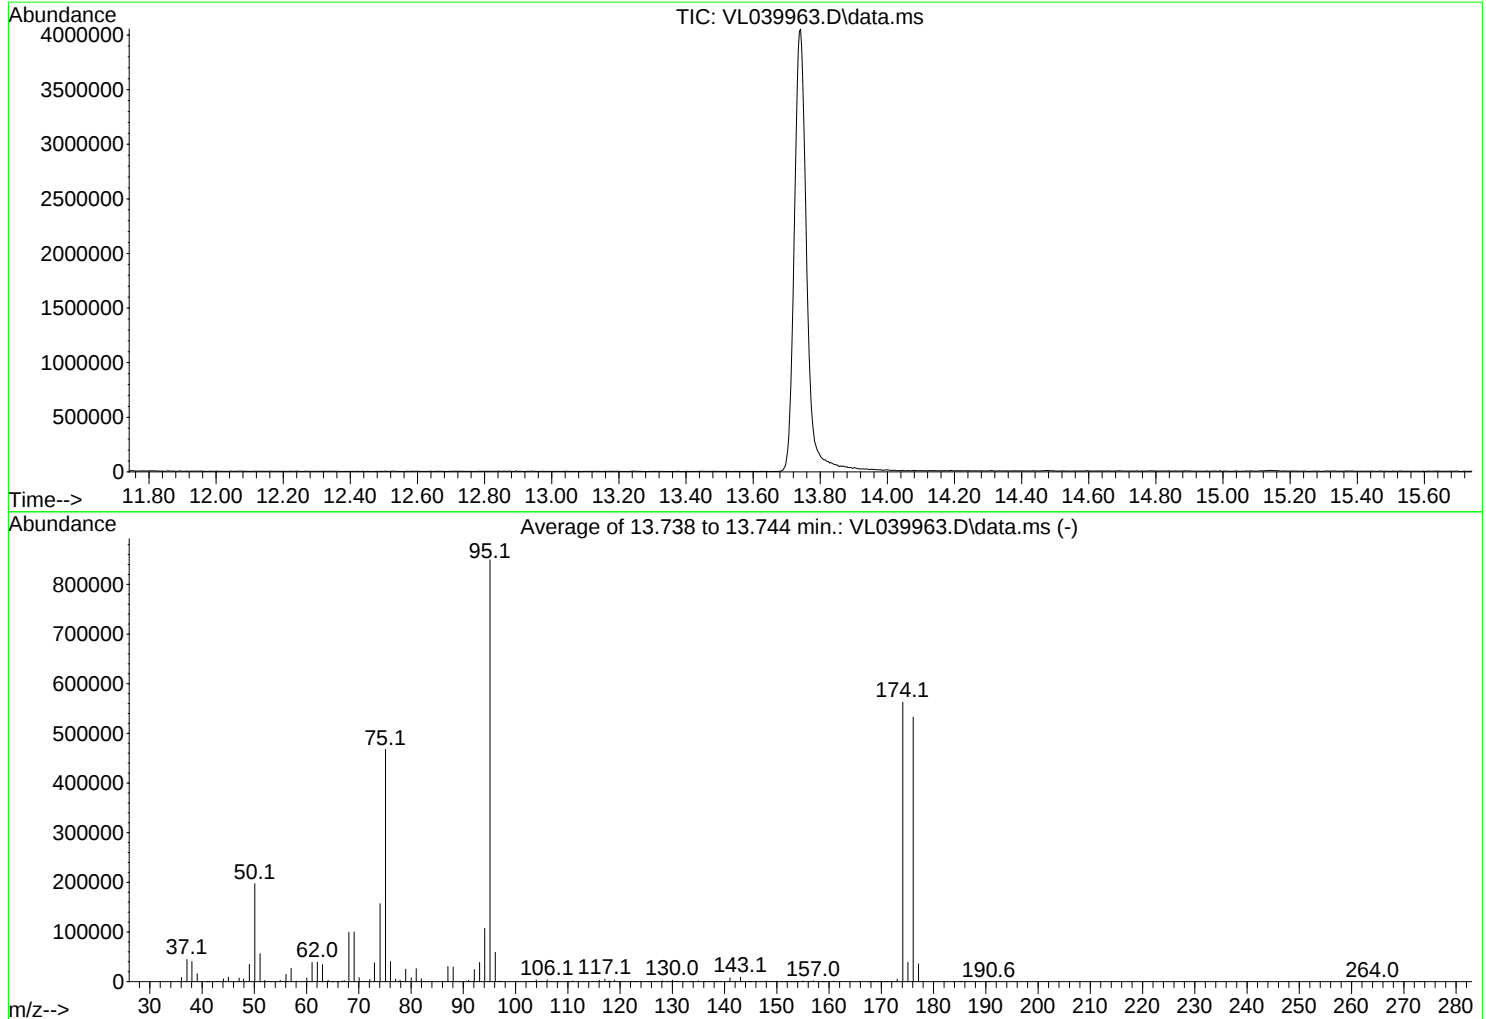

AutoFind: Scans 3463, 3464, 3465; Background Corrected with Scan 3438

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.2	197141	PASS
75	95	30	66	55.0	467541	PASS
95	95	100	100	100.0	849408	PASS
96	95	5	9	6.9	58819	PASS
173	174	0.00	2	0.9	5338	PASS
174	95	50	120	66.3	562923	PASS
175	174	4	9	6.9	38981	PASS
176	174	93	101	94.6	532672	PASS
177	176	5	9	6.7	35621	PASS

Average of 13.738 to 13.744 min.: VL039963.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8261	47.10	7517	58.05	1206	68.10	9965
37.10	44925	47.95	5435	59.05	247	69.10	10009
38.05	40747	49.05	34979	60.05	7448	70.05	795
39.05	16287	50.10	197141	61.05	38843	70.85	29
40.90	88	51.10	56531	62.05	39355	72.10	4461
41.30	72	52.00	2372	63.05	34560	73.00	37671
42.85	305	53.10	146	64.10	2801	74.05	157075
43.30	387	54.00	108	64.90	124	75.10	467541
44.10	5577	54.95	2648	65.90	75	76.05	40202
45.05	8977	56.05	14868	66.85	1339	77.05	4991
46.05	733	57.05	26624	67.20	1827	77.90	3017

Instrument :
MSVOA_L
ClientSampleId :
BFB

Average of 13.738 to 13.744 min.: VL039963.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	25173	93.10	38664	106.05	3597	117.10	5039
80.05	7729	94.10	107403	106.90	795	117.80	935
81.00	26141	95.10	849408	108.10	78	118.05	1394
81.95	5724	96.10	58819	109.85	415	118.95	3600
83.10	831	97.00	1424	110.10	100	120.10	67
86.00	968	97.30	549	110.95	1344	122.10	64
87.05	30512	102.65	272	111.90	533	122.80	101
88.05	29288	103.10	419	112.95	620	123.25	276
89.45	202	103.95	3591	114.70	345	123.90	161
91.00	2580	104.80	230	114.95	393	124.15	233
92.10	24352	105.00	1019	116.05	2721	124.95	324

Average of 13.738 to 13.744 min.: VL039963.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.50	51	136.95	719	146.00	1098	153.10	590
125.95	309	137.20	479	146.95	610	153.30	71
128.00	1026	138.30	51	147.80	521	153.80	239
128.15	1720	139.10	100	148.05	1463	154.10	228
129.10	1120	140.00	539	148.80	240	155.00	1669
130.00	2857	141.05	7749	149.30	202	156.30	373
130.90	877	142.10	955	150.00	903	157.00	1869
131.10	401	143.05	8953	150.90	69	157.90	88
133.60	158	144.00	734	151.65	191	158.70	189
135.00	1580	144.70	103	152.10	212	159.00	503
136.00	122	145.10	554	152.70	65	159.20	163

Average of 13.738 to 13.744 min.: VL039963.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.85	848	171.20	221	183.80	134		
161.90	65	171.75	802	185.20	55		
165.80	95	172.00	397	190.60	59		
167.60	65	172.60	801	264.00	111		
168.50	64	173.05	5338	273.00	90		
168.80	297	174.10	562923				
169.30	142	175.10	38981				
169.80	68	176.10	532672				
170.10	110	177.10	35621				
170.60	279	177.90	480				
170.90	142	178.10	426				