


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL120721\
 Data File : VL038142.D
 Acq On : 7 Dec 2021 9:28
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111821AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Nov 18 13:16:09 2021
 Last Update : Thu Nov 18 13:16:09 2021

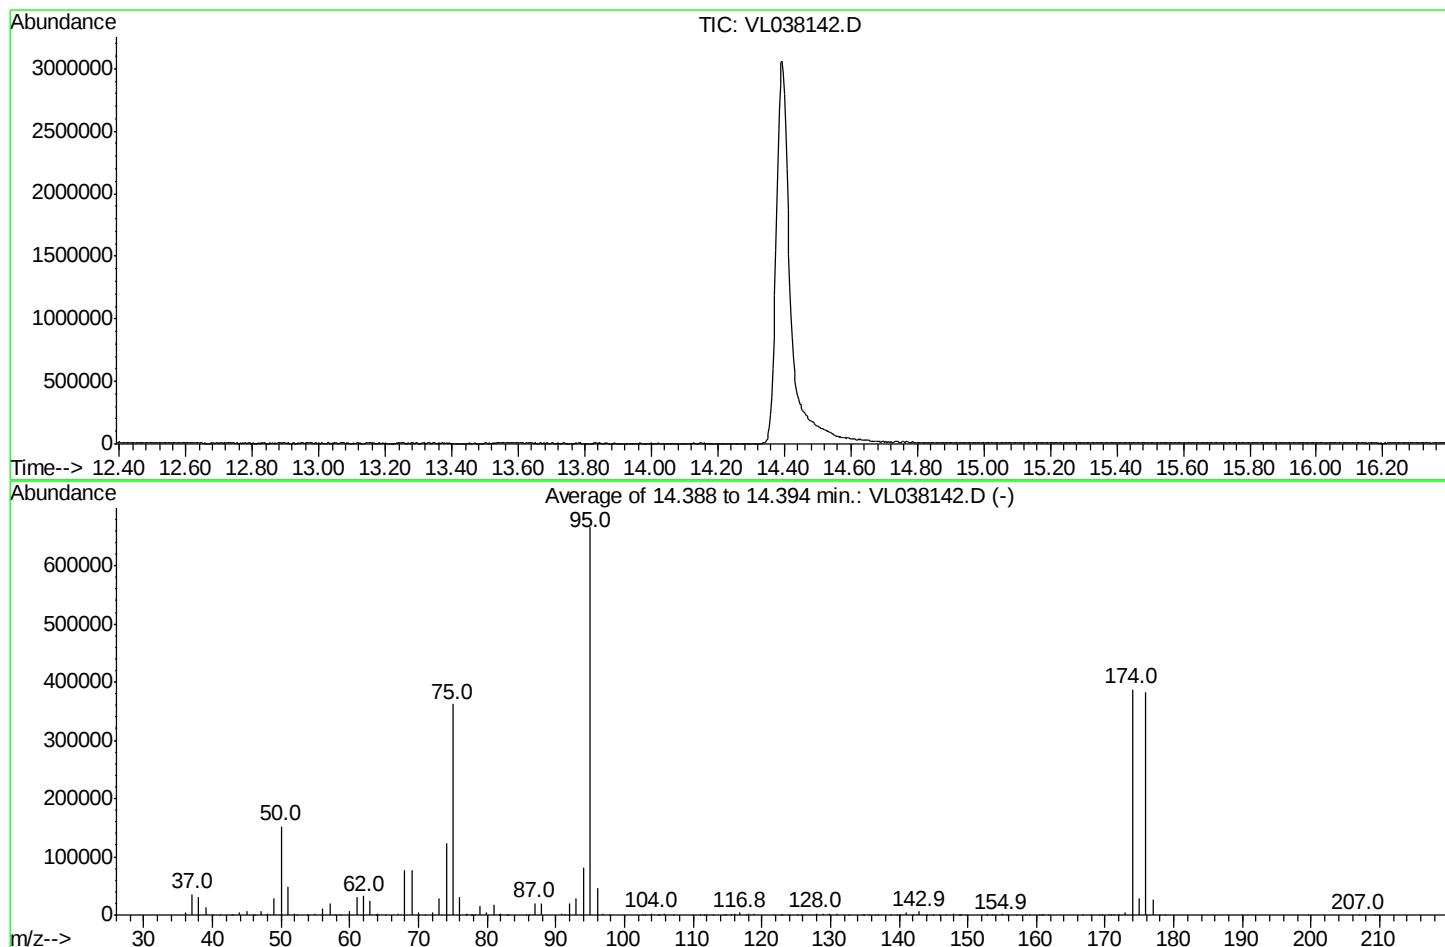

AutoFind: Scans 3608, 3609, 3610; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.9	152746	PASS
75	95	30	66	54.4	361941	PASS
95	95	100	100	100.0	665920	PASS
96	95	5	9	6.8	45248	PASS
173	174	0.00	2	1.0	3974	PASS
174	95	50	120	58.2	387605	PASS
175	174	4	9	7.4	28829	PASS
176	174	93	101	98.8	383125	PASS
177	176	5	9	6.8	25962	PASS