


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL120820\
 Data File : VL036096.D
 Acq On : 8 Dec 2020 14:28
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL120720AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Dec 07 16:56:49 2020
 Last Update : Mon Dec 07 16:56:49 2020

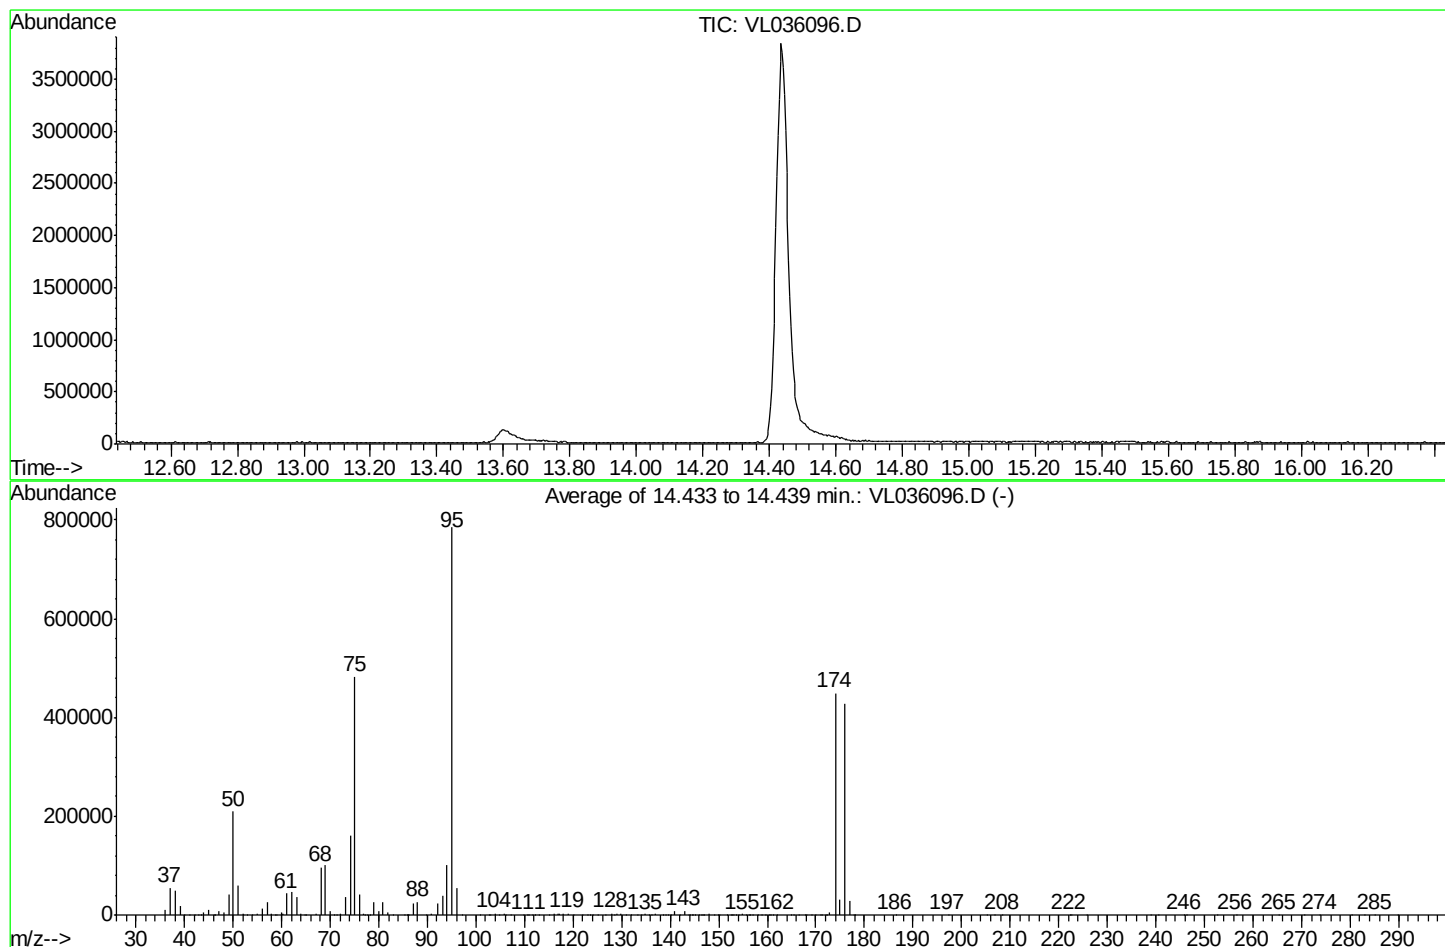

AutoFind: Scans 3622, 3623, 3624; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.7	209664	PASS
75	95	30	66	61.5	482922	PASS
95	95	100	100	100.0	785045	PASS
96	95	5	9	6.9	54530	PASS
173	174	0.00	2	1.2	5545	PASS
174	95	50	120	57.2	449045	PASS
175	174	4	9	7.2	32402	PASS
176	174	93	101	95.3	427882	PASS
177	176	5	9	6.4	27373	PASS