

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL121020\
Quantitation Report (Not Reviewed)

Data File : VL036151.D
Acq On : 11 Dec 2020 6:02
Operator : SY/AP
Sample : VIBLK
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Quant Time: Dec 11 07:13:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL120720AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Dec 07 16:56:49 2020
QLast Update : Mon Dec 07 16:56:49 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.65	49	1234654	10.00	ppbv	-0.03
33) 1,4-Difluorobenzene	7.16	114	2498341	10.00	ppbv	-0.04
55) Chlorobenzene-d5	12.07	117	2293700	10.00	ppbv	-0.04

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.40	95	1934196	10.62	ppbv	-0.04
Spiked Amount	10.000	Range	65 - 135	Recovery	=	106.20%


Target Compounds					Qvalue	
13) Ethanol	3.63	45	694	0.071	ppbv #	1
15) Acetone	3.87	43	15401	0.104	ppbv #	1
39) 1,2-Dichloropropane	7.16	63	830227	9.929	ppbv #	23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VL036151.D
Acq On : 11 Dec 2020 6:02
Operator : SY/AP
Sample : VIBLK
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Quant Time: Dec 11 07:13:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL120720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Dec 07 16:56:49 2020
QLast Update : Mon Dec 07 16:56:49 2020
Response via : Initial Calibration

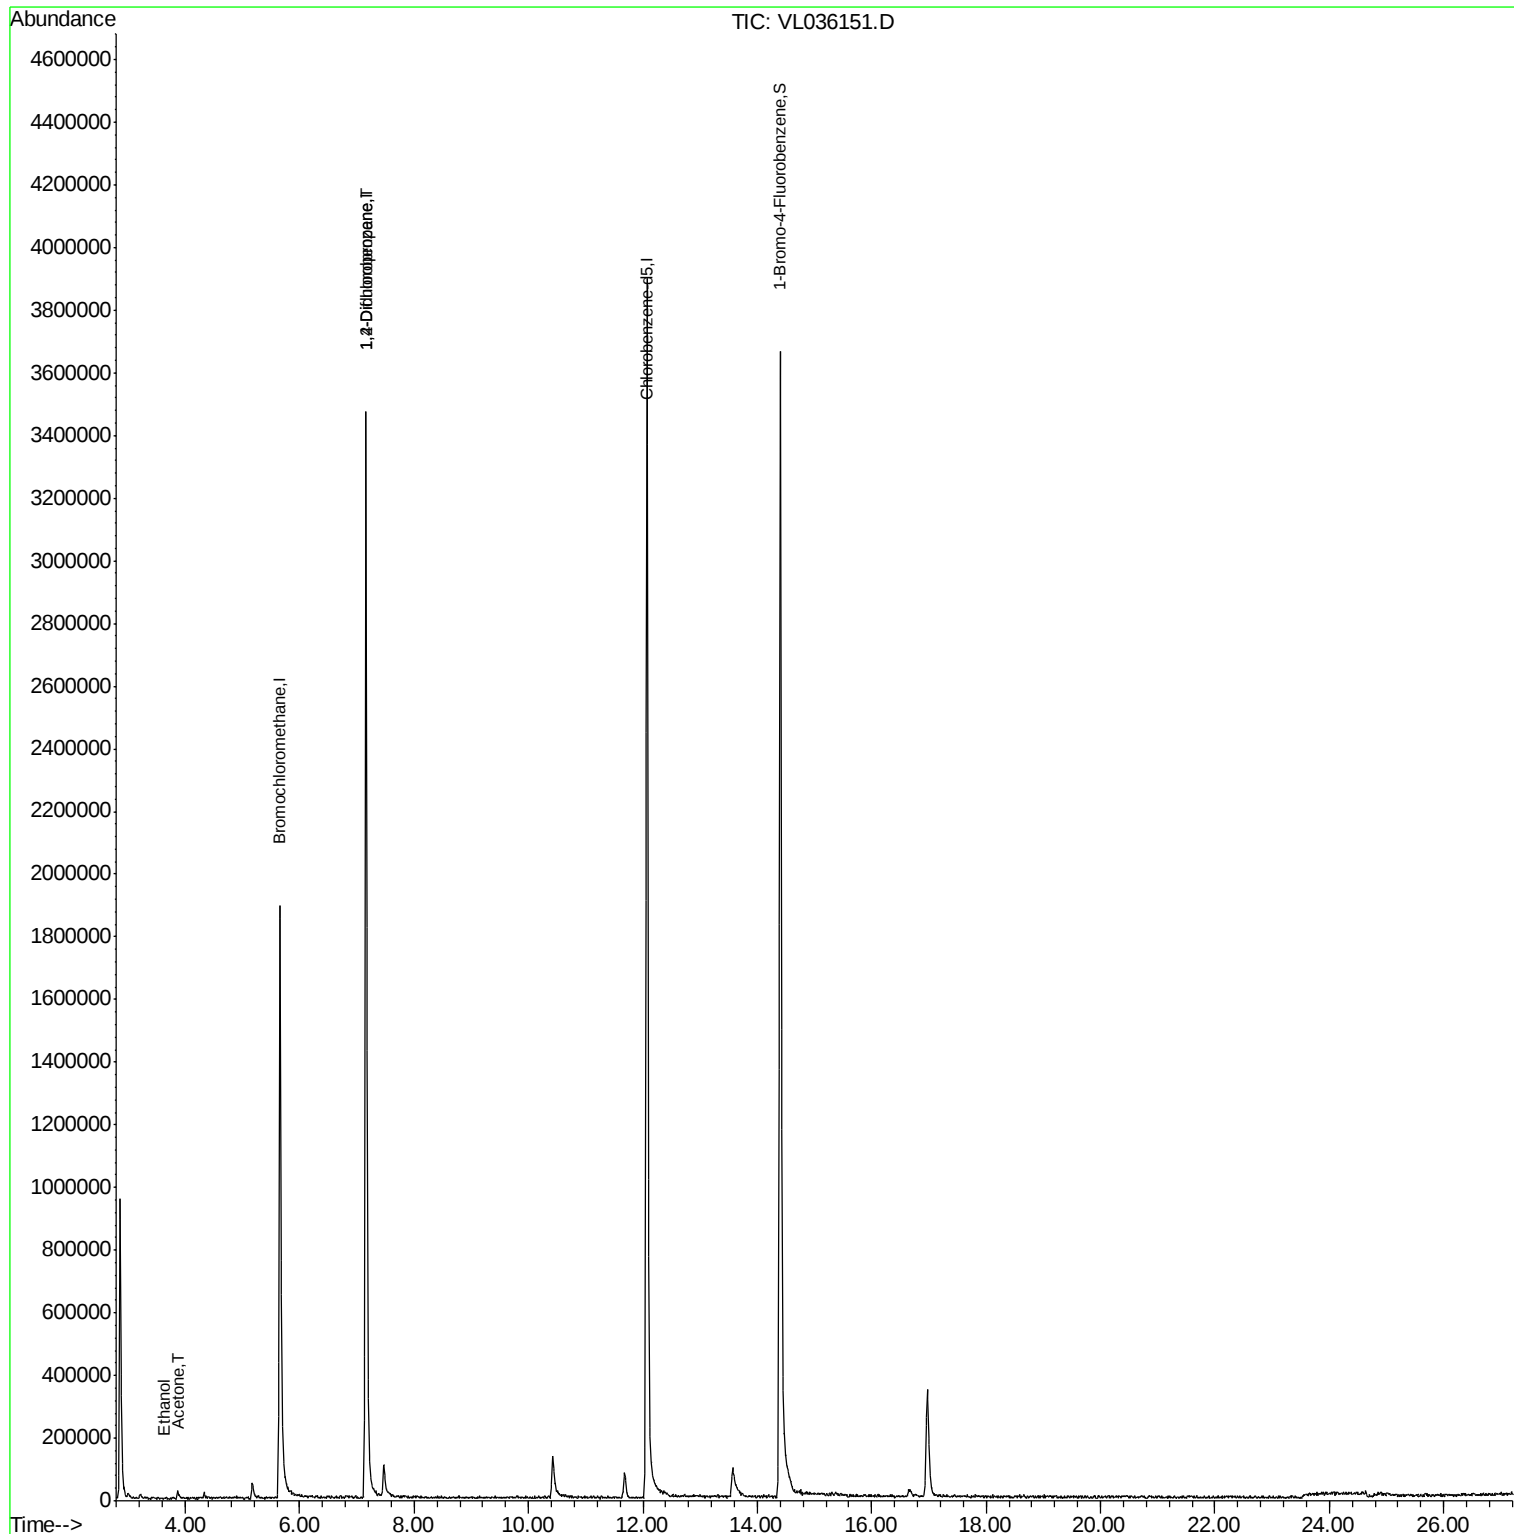

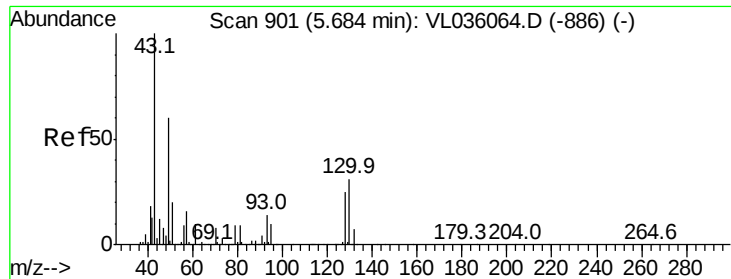

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.65 min Scan# 891

Delta R.T. -0.03 min

Lab File: VL036151.D

Acq: 11 Dec 2020 6:02

Instrument :

MSVOA_L

ClientSampleId :

VIBLK


Tgt Ion: 49 Resp: 1234654

Ion Ratio Lower Upper

49 100

128 37.1 21.1 63.1




130 48.9 27.1 81.3

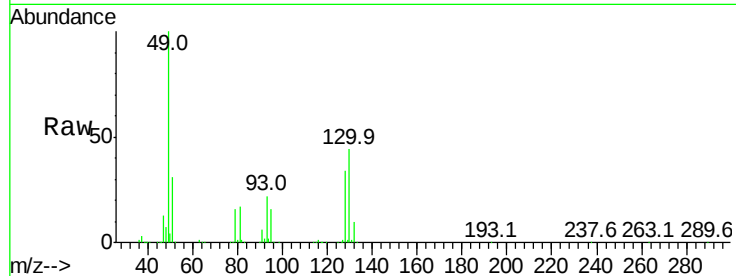

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

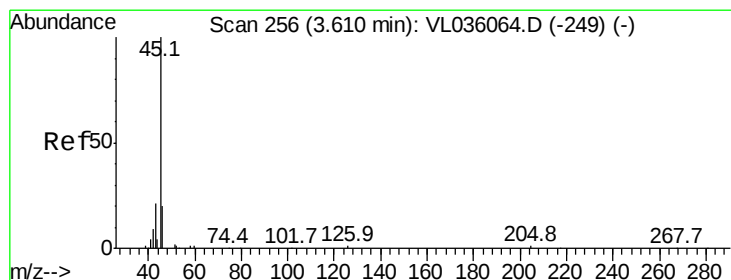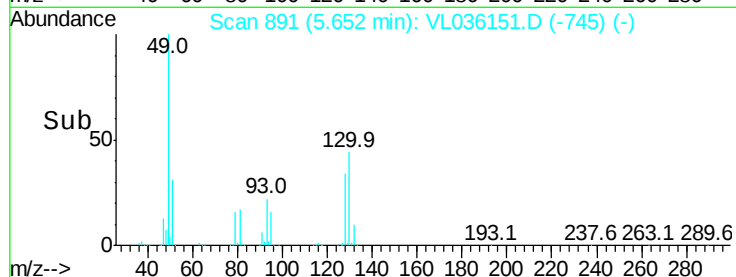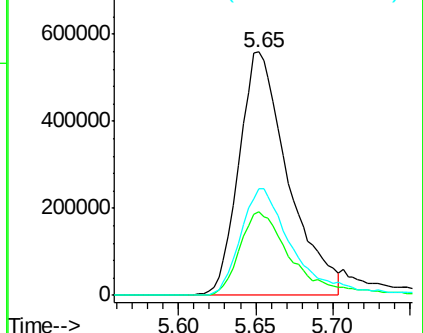

#13

Ethanol

Concen: 0.071 ppbv

RT: 3.63 min Scan# 261

Delta R.T. 0.02 min

Lab File: VL036151.D


Acq: 11 Dec 2020 6:02

Tgt Ion: 45 Resp: 694

Ion Ratio Lower Upper



45 100


46 171.8 19.0 75.8#

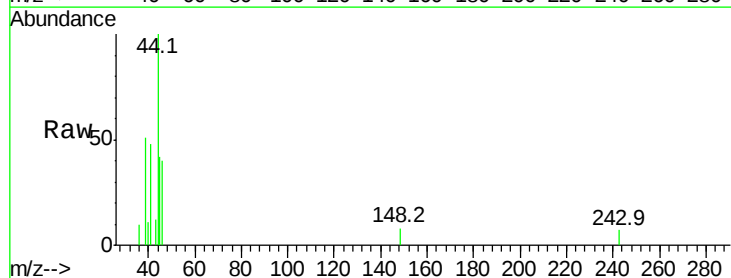

Abundance Ion 45.10 (44.80 to 45.80): VL0

Ion 46.10 (45.80 to 46.80): VL0

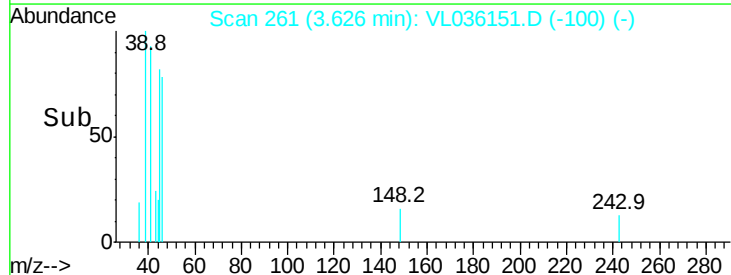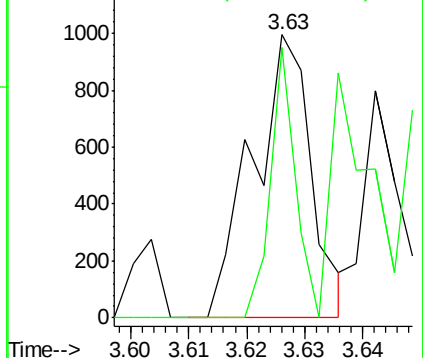

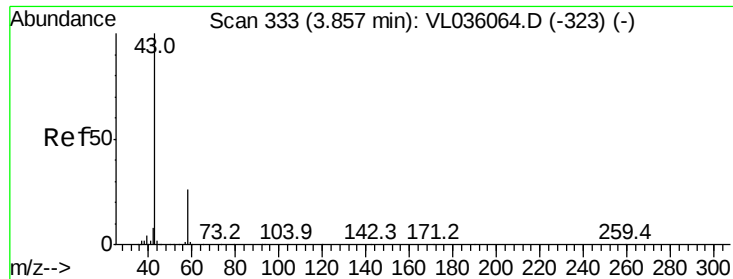

#15

Acetone

Concen: 0.104 ppbv

RT: 3.87 min Scan# 336

Delta R.T. 0.01 min

Lab File: VL036151.D

Acq: 11 Dec 2020 6:02

Instrument :

MSVOA_L

ClientSampleId :





VIBLK

Tgt Ion: 43 Resp: 15401

Ion Ratio Lower Upper

43 100

58 99.4 20.9 31.3#

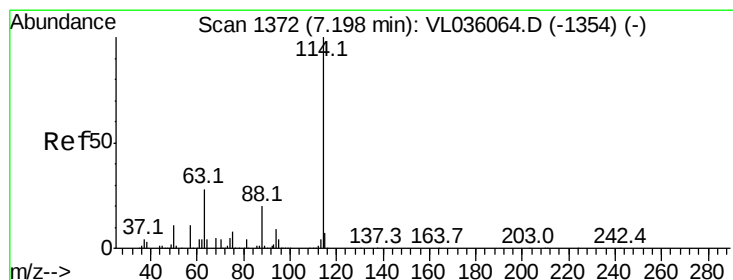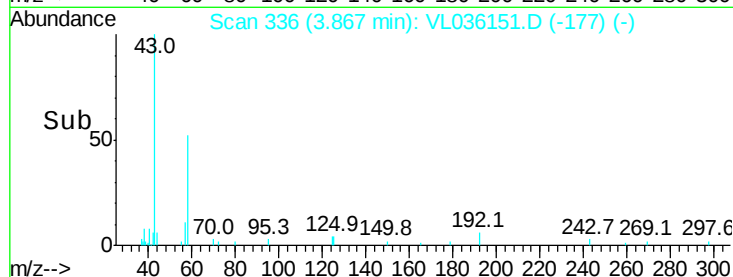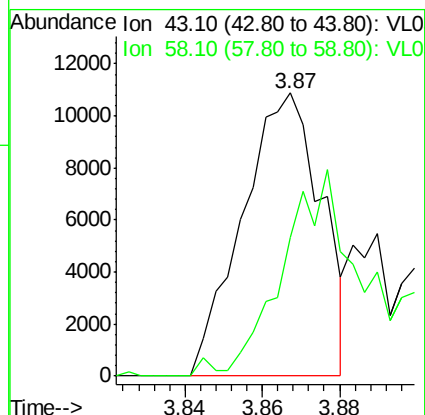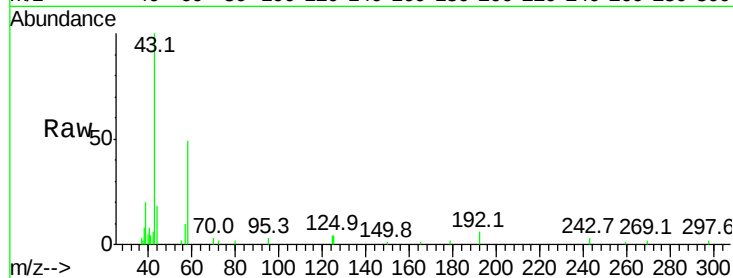

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.16 min Scan# 1360

Delta R.T. -0.04 min

Lab File: VL036151.D

Acq: 11 Dec 2020 6:02




Tgt Ion: 114 Resp: 2498341


Ion Ratio Lower Upper

114 100

63 34.1 23.6 35.4

88 21.7 15.8 23.6

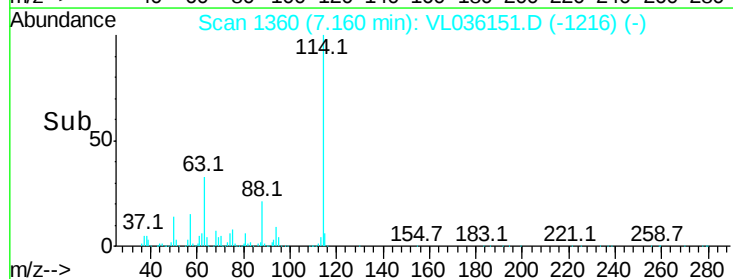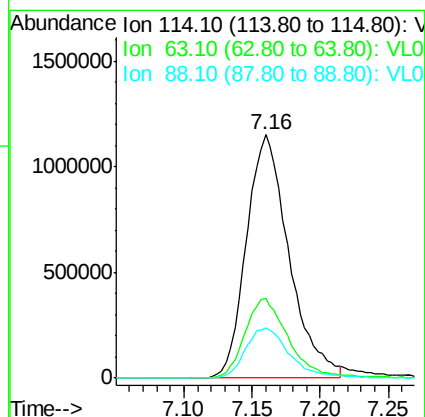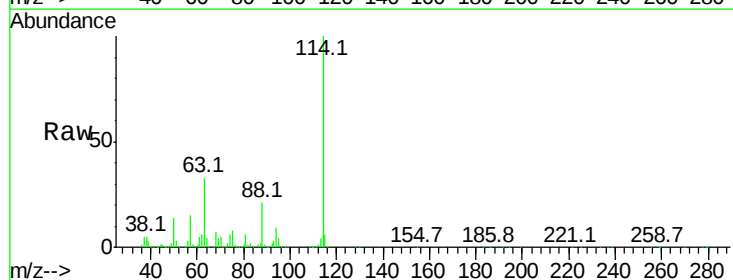

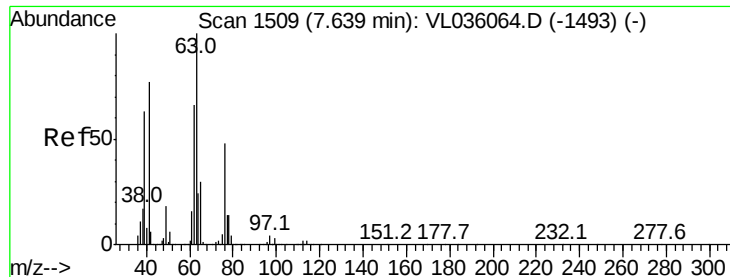

#39

1,2-Dichloropropane

Concen: 9.929 ppbv

RT: 7.16 min Scan# 1360

Delta R.T. -0.48 min

Lab File: VL036151.D

Acq: 11 Dec 2020 6:02

Instrument :

MSVOA_L

ClientSampleId :

VIBLK


Tgt Ion: 63 Resp: 830227

Ion Ratio Lower Upper

63 100

41 0.1 61.9 92.9#




62 16.8 52.5 78.7#

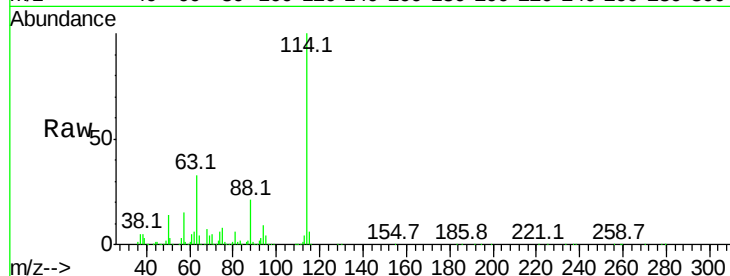

Abundance Ion 63.10 (62.80 to 63.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 62.10 (61.80 to 62.80): VL0

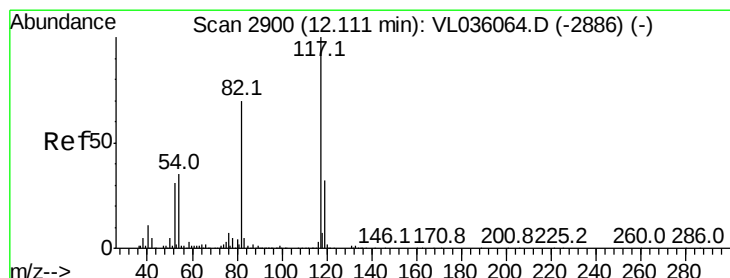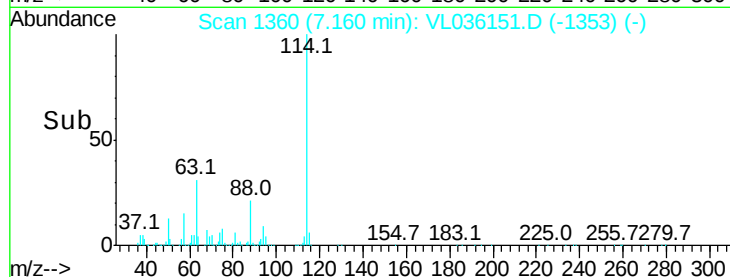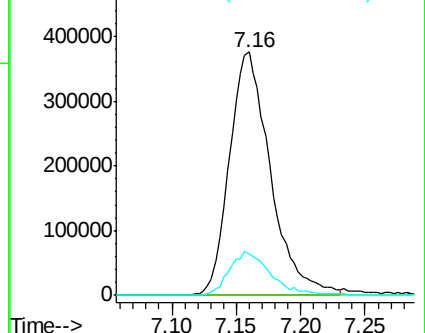

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.07 min Scan# 2888

Delta R.T. -0.04 min

Lab File: VL036151.D

Acq: 11 Dec 2020 6:02


Tgt Ion: 117 Resp: 2293700

Ion Ratio Lower Upper

117 100

82 81.3 0.0 0.0#



119 33.5 0.0 0.0#

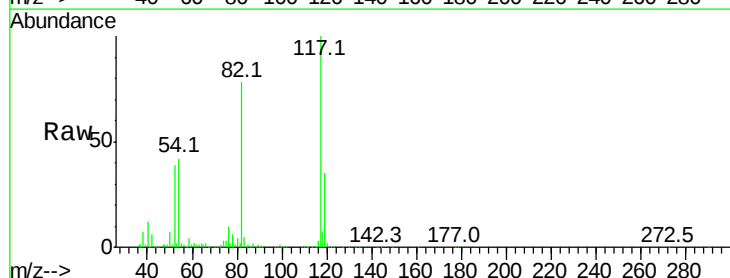


Abundance Ion 117.10 (116.80 to 117.80): V

Ion 82.10 (81.80 to 82.80): VL0

Ion 119.10 (118.80 to 119.80): V

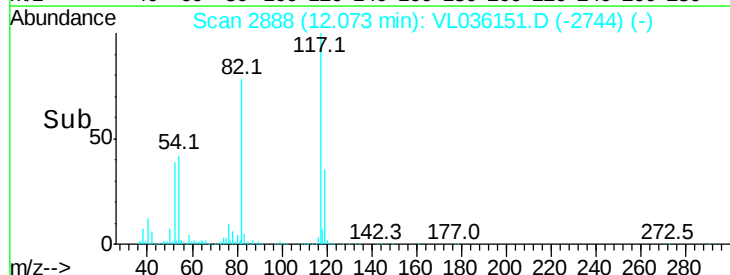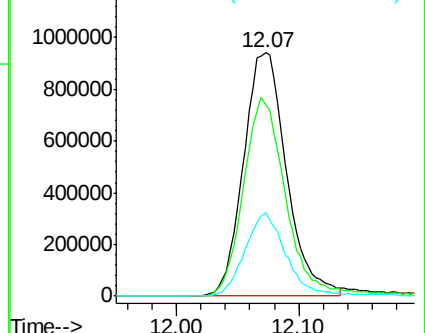

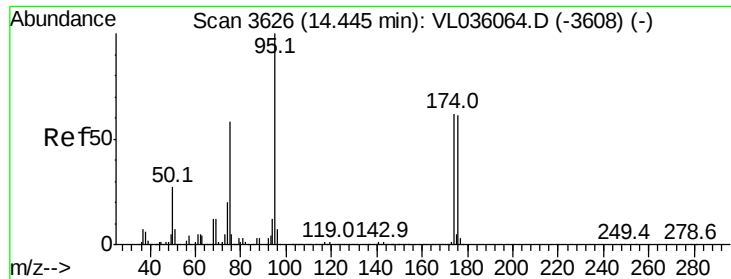

#68

1-Bromo-4-Fluorobenzene

Concen: 10.620 ppbv

RT: 14.40 min Scan# 3613

Delta R.T. -0.04 min

Lab File: VL036151.D

Acq: 11 Dec 2020 6:02

Instrument :

MSVOA_L

ClientSampleId :

VIBLK


Tgt Ion: 95 Resp: 1934196

Ion Ratio Lower Upper

95 100

174 56.9 50.7 76.1

175 4.1 4.0 6.0

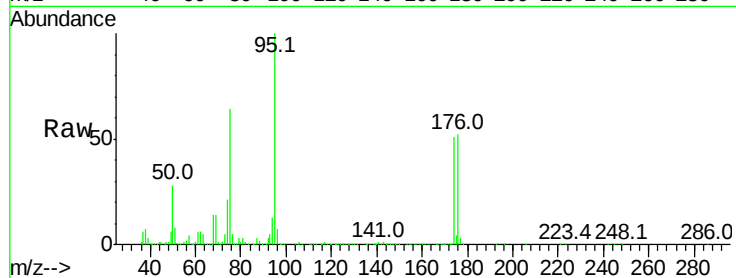

Abundance Ion 95.10 (94.80 to 95.80): VL0

Ion 174.00 (173.70 to 174.70): V

Ion 175.00 (174.70 to 175.70): V

