


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121220\
 Data File : VY003742.D
 Acq On : 12 Dec 2020 09:32
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/10ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB90

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM121220S.M
 Title : VOC Analysis
 Last Update : Fri Dec 11 10:03:37 2020

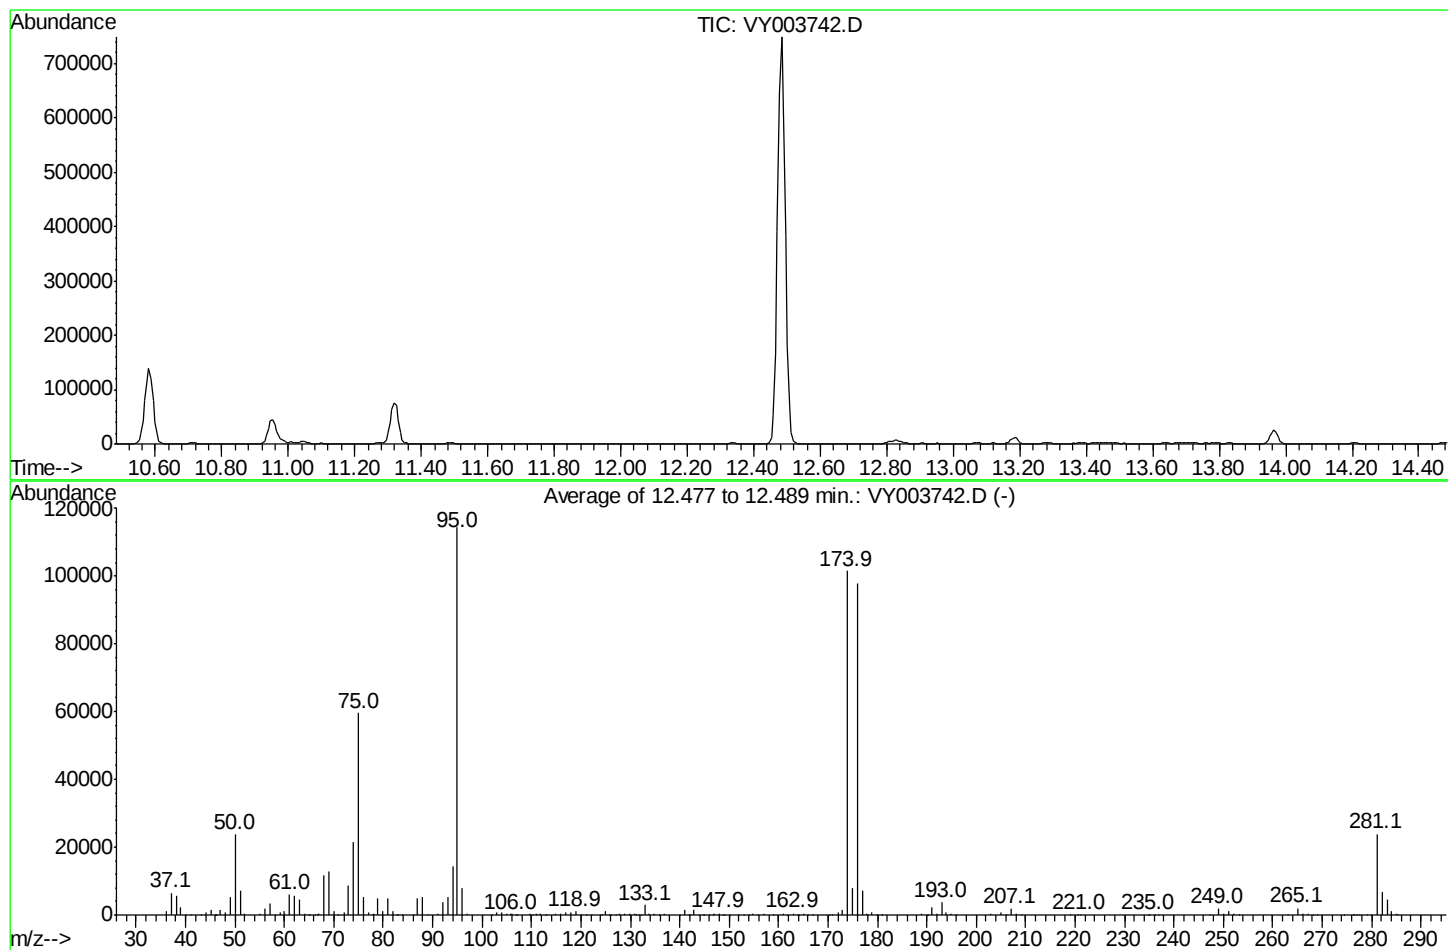

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	23733	PASS
75	95	30	80	52.1	59594	PASS
95	95	100	100	100.0	114328	PASS
96	95	5	9	7.0	7979	PASS
173	174	0.00	2	1.4	1419	PASS
174	95	50	120	88.8	101509	PASS
175	174	5	9	7.9	8000	PASS
176	174	95	101	96.2	97610	PASS
177	176	5	9	7.4	7216	PASS