


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL121020\
 Data File : VL036130.D
 Acq On : 10 Dec 2020 13:15
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL120720AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Dec 07 16:56:49 2020
 Last Update : Mon Dec 07 16:56:49 2020

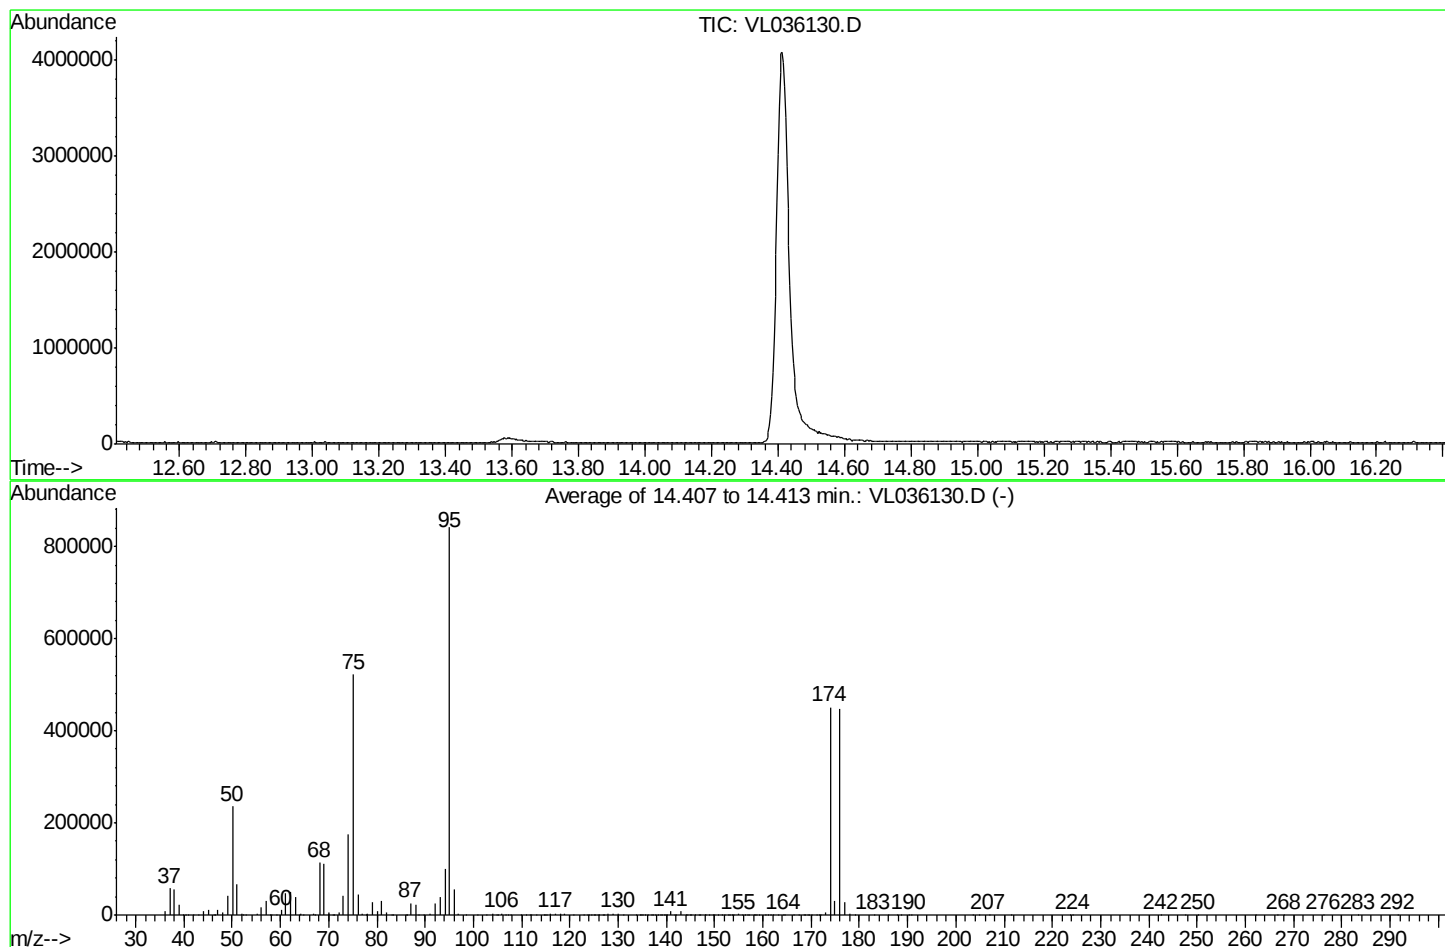

AutoFind: Scans 3614, 3615, 3616; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	28.0	235925	PASS
75	95	30	66	61.9	521322	PASS
95	95	100	100	100.0	841557	PASS
96	95	5	9	6.6	55325	PASS
173	174	0.00	2	1.2	5497	PASS
174	95	50	120	53.6	450922	PASS
175	174	4	9	6.9	31058	PASS
176	174	93	101	99.2	447530	PASS
177	176	5	9	6.1	27485	PASS