


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL121118\
 Data File : VL032952.D
 Acq On : 11 Dec 2018 12:12
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL120718AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Dec 07 09:35:17 2018
 Last Update : Fri Dec 07 09:35:17 2018

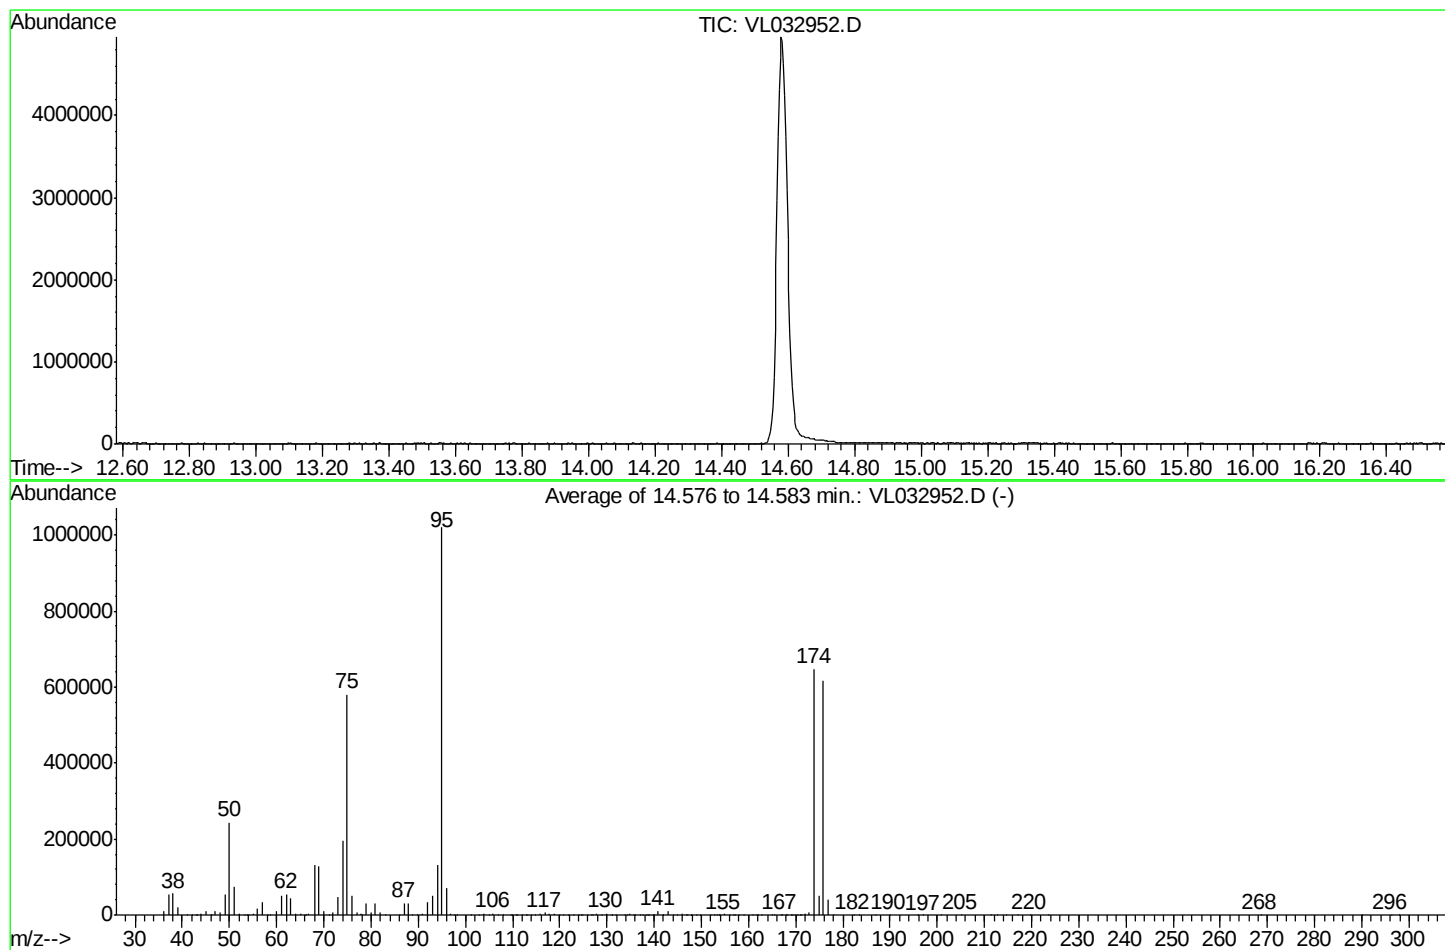

AutoFind: Scans 3620, 3621, 3622; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	242666	PASS
75	95	30	66	56.9	580309	PASS
95	95	100	100	100.0	1020224	PASS
96	95	5	9	6.8	69392	PASS
173	174	0.00	2	1.0	6658	PASS
174	95	50	120	63.5	647573	PASS
175	174	4	9	7.7	50109	PASS
176	174	93	101	95.3	617066	PASS
177	176	5	9	6.3	39032	PASS