


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121124\
Data File : VL041718.D
Acq On : 11 Dec 2024 13:38
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121124AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Dec 12 13:35:39 2024

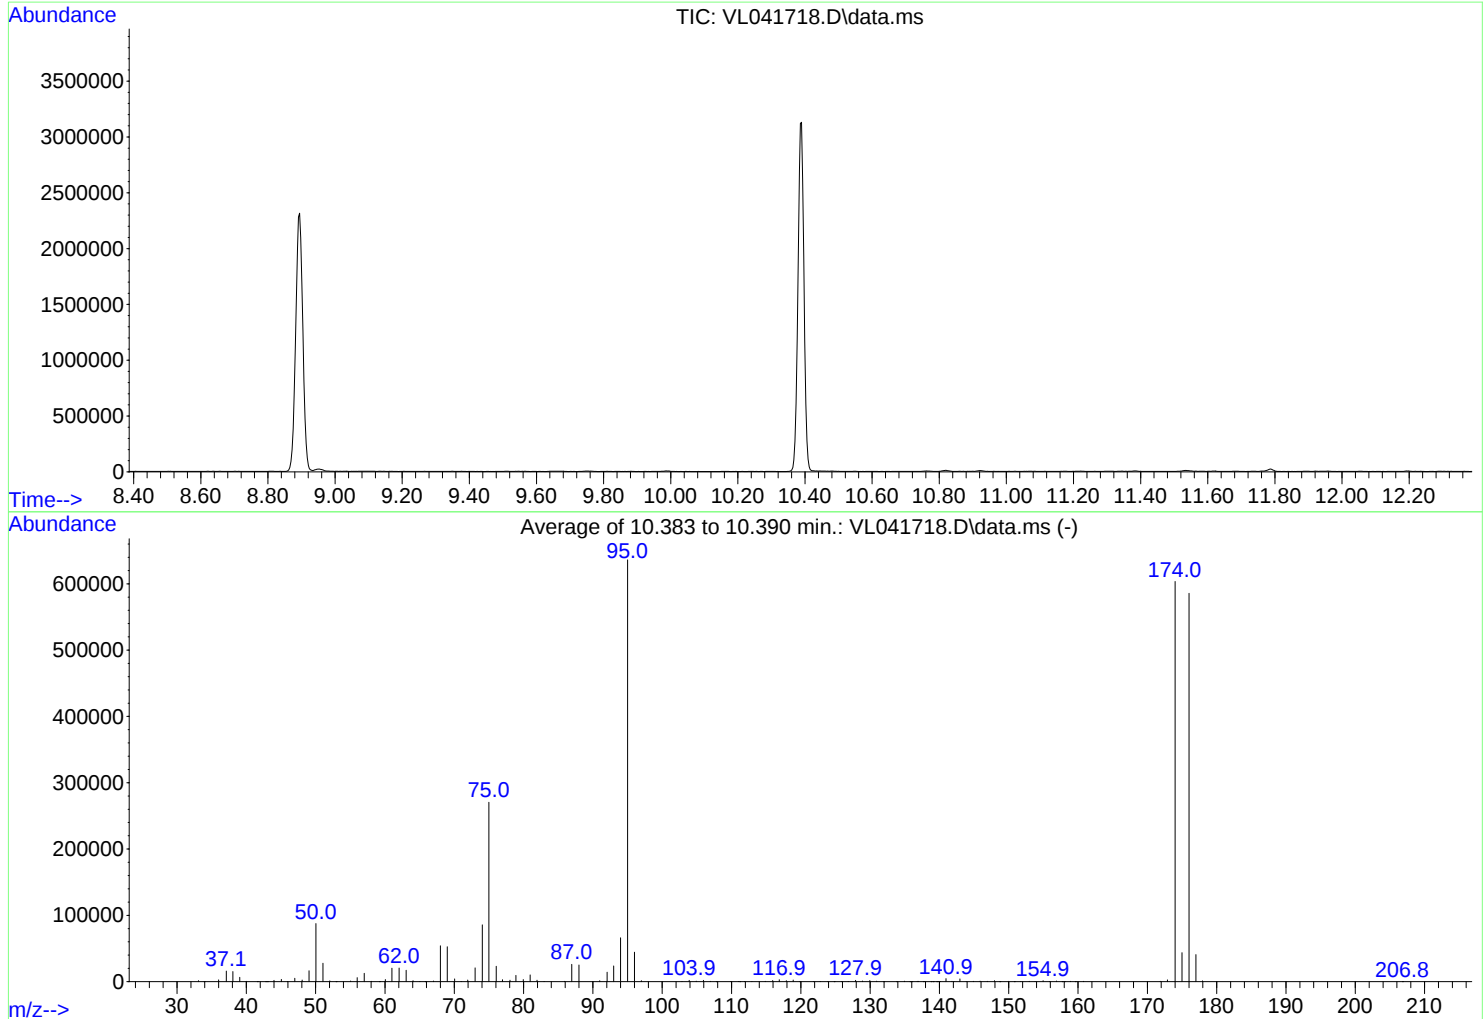

AutoFind: Scans 3181, 3182, 3183; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	13.8	87664	PASS
75	95	30	66	42.5	270592	PASS
95	95	100	100	100.0	636160	PASS
96	95	5	9	7.0	44440	PASS
173	174	0.00	2	0.4	2686	PASS
174	95	50	120	94.9	603648	PASS
175	174	4	9	7.2	43747	PASS
176	174	93	101	97.0	585707	PASS
177	176	5	9	7.0	40776	PASS

Average of 10.383 to 10.390 min.: VL041718.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1423	45.05	3397	57.00	12648	68.00	5397
33.90	32	45.95	244	58.05	566	69.00	5258
36.00	2576	47.00	5050	59.20	21	70.05	423
37.10	15917	48.05	2310	60.05	3209	71.00	22
38.05	15349	49.05	16344	61.00	20373	71.95	2401
39.05	6452	50.05	87664	62.05	20424	73.00	20824
40.00	412	51.05	27664	63.05	17141	74.05	85584
41.60	38	52.05	1330	64.05	1524	75.00	270592
42.80	20	52.95	128	65.05	308	76.05	23181
43.05	138	55.05	950	65.80	67	76.95	2866
44.00	1905	56.00	6042	67.00	1114	78.05	2279

Instrument :

MSVOA_L

ClientSampleId :

BFB

Average of 10.383 to 10.390 min.: VL041718.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.90	9527	94.00	66224	111.00	216	122.80	209
79.95	3069	95.00	636160	111.20	132	123.90	369
80.95	10172	96.00	44440	111.85	243	124.80	145
81.95	2244	97.00	1441	112.95	325	125.90	265
82.95	330	102.85	206	114.85	445	126.85	222
85.90	507	103.90	1978	115.95	1665	127.90	1959
86.95	26117	104.90	661	116.90	3011	128.90	880
88.00	25200	105.95	1869	117.90	1543	129.95	1773
91.00	1465	106.95	527	118.90	2440	130.95	753
92.05	14325	107.80	22	119.85	109	131.95	146
93.00	23792	109.90	168	121.85	181	133.80	118

Average of 10.383 to 10.390 min.: VL041718.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
134.95	780	140.95	4487	149.95	541	159.60	41
135.75	92	141.80	426	150.80	24	160.80	553
136.00	42	142.10	242	151.75	300	171.85	385
136.80	558	142.95	4194	152.95	567	172.90	2686
137.00	390	143.85	316	153.80	383	174.00	603648
137.70	38	144.90	528	154.95	1452	175.00	43747
138.80	50	145.85	858	155.90	278	176.00	585707
139.10	121	146.90	422	156.90	1045	177.00	40776
139.60	76	147.95	1479	157.70	67	177.95	1190
139.85	213	148.70	125	158.00	30	206.80	17
140.15	261	148.85	362	158.90	586		