

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121222\
 Data File : VL039994.D
 Acq On : 13 Dec 2022 2:58
 Operator : SY/MD
 Sample : N5969-01 10X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SG-1

Quant Time: Dec 13 07:13:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111822AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Dec 02 23:21:36 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.169	49	950552	10.000	ppbv	0.01
33) 1,4-Difluorobenzene	6.632	114	2778922	10.000	ppbv	0.01
55) Chlorobenzene-d5	11.465	117	2484307	10.000	ppbv	0.03
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.773	95	2162394	11.396	ppbv	0.03
Spiked Amount	10.000	Range	65 - 135	Recovery	=	114.000%
Target Compounds						
					Qvalue	
3) Chlorodifluoromethane	2.851	51	361976	2.760	ppbv #	60
4) Chloromethane	2.851	50	424767	5.068	ppbv #	68
9) Propene	2.851	41	11166329	180.724	ppbv	91
10) Heptane	7.581	43	10848423	72.764	ppbv	93
11) Trichlorofluoromethane	3.542	101	4453	0.027	ppbv #	75
13) Ethanol	3.224	45	42125	8.930	ppbv	83
15) Acetone	3.472	43	5445729	43.193	ppbv #	57
16) 1,3-Butadiene	2.989	39	2376811	37.825	ppbv #	10
19) Isopropyl Alcohol	3.571	45	37478	0.549	ppbv #	29
20) Methylene Chloride	3.912	84	72655	1.189	ppbv	93
21) Allyl Chloride	4.147	41	1221669	13.969	ppbv #	52
23) Vinyl Acetate	4.587	43	3295522	63.624	ppbv #	1
24) 1,1-Dichloroethane	4.581	63	6993	0.056	ppbv #	89
25) Ethyl Acetate	5.192	43	1707515	7.376	ppbv #	75
26) Hexane	5.195	57	2520006	24.920	ppbv #	37
29) Chloroform	5.253	83	4056	0.030	ppbv #	63
30) Cyclohexane	6.587	84	584449	5.889	ppbv #	80
34) 2-Butanone	4.780	43	56181	0.423	ppbv #	89
36) Benzene	6.346	78	58546	0.248	ppbv #	76
39) 1,2-Dichloropropane	6.954	63	67017	0.728	ppbv #	1
41) Tetrahydrofuran	5.407	42	33677	0.367	ppbv #	36
42) Bromodichloromethane	7.250	83	1139585	6.492	ppbv #	27
43) Methyl Methacrylate	7.439	69	1066332	11.514	ppbv #	54
44) 2,2,4-Trimethylpentane	7.340	57	6634380	16.825	ppbv #	1
47) 1,1,2-Trichloroethane	8.883	97	9349	0.099	ppbv #	55
50) 4-Methyl-2-Pentanone	8.205	43	1775183	7.454	ppbv #	84
51) 2-Hexanone	9.552	43	15017926	81.234	ppbv #	27
52) Tetrachloroethene	10.616	164	27842	0.315	ppbv	87
53) Toluene	9.108	91	19192	0.071	ppbv	90
57) Chlorobenzene	11.571	112	150283	0.791	ppbv #	29
59) m/p-Xylene	12.343	91	91962	0.326	ppbv #	48
62) Isopropylbenzene	14.024	105	47024	0.121	ppbv	92
63) 1,1,2,2-Tetrachloroethane	13.040	83	83853	0.934	ppbv #	1
80) Naphthalene,2-methyl-	24.400	142	1205	0.024	ppbv	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Dec 13 07:13:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111822AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 26 06:05:16 2022
QLast Update : Fri Dec 02 23:21:36 2022
Response via : Initial Calibration





#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.169 min Scan# 79

Delta R.T. 0.013 min

Lab File: VL039994.D

Acq: 13 Dec 2022 2:58

Instrument :

MSVOA_L

ClientSampleId :

SG-1





Tgt Ion: 49 Resp: 950552

Ion Ratio Lower Upper

49 100

128 43.7 22.1 66.3

130 56.7 27.7 83.1

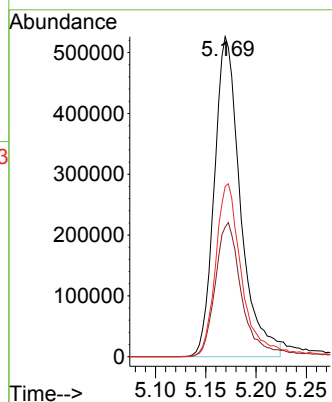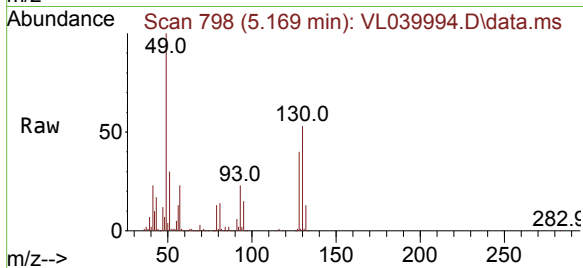

#3

Chlorodifluoromethane

Concen: 2.760 ppbv

RT: 2.851 min Scan# 77

Delta R.T. 0.209 min

Lab File: VL039994.D




Acq: 13 Dec 2022 2:58


Tgt Ion: 51 Resp: 361976

Ion Ratio Lower Upper

51 100

67 0.1 14.2 21.4#


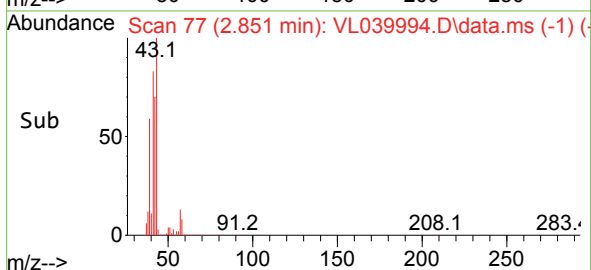

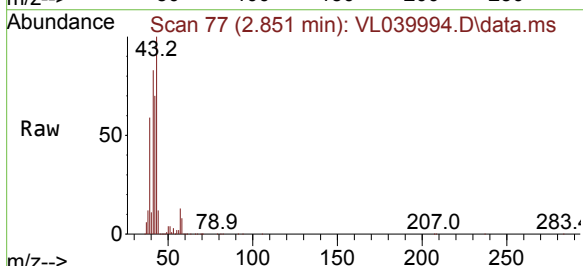


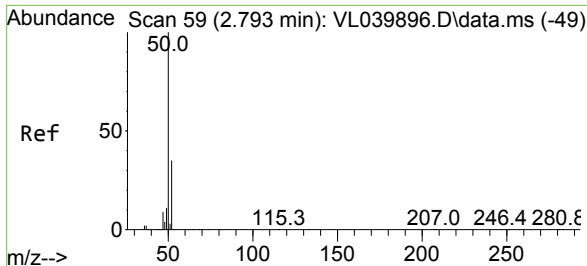

#4
Chloromethane
Concen: 5.068 ppbv
RT: 2.851 min Scan# 77
Delta R.T. 0.071 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58




Instrument : MSVOA_L
ClientSampleId : SG-1


Tgt Ion: 50 Resp: 424767
Ion Ratio Lower Upper
50 100
52 16.4 27.8 41.8#

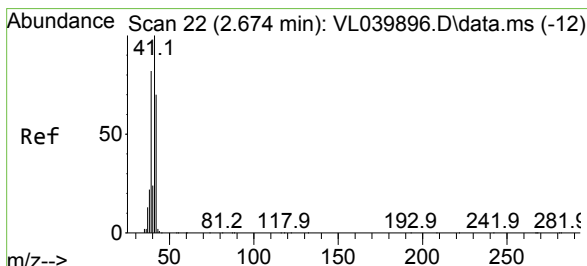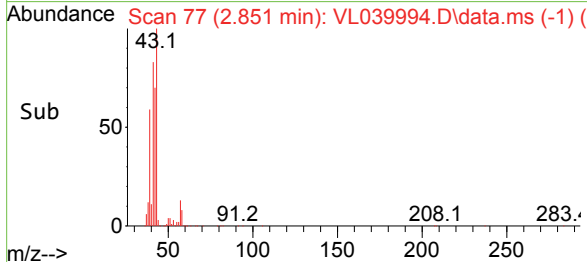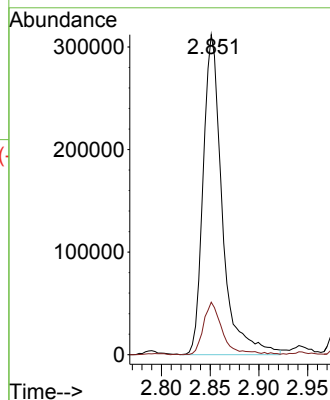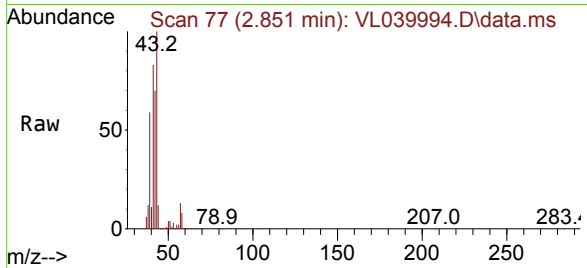

#9
Propene
Concen: 180.724 ppbv
RT: 2.851 min Scan# 77
Delta R.T. 0.190 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion: 41 Resp: 11166329
Ion Ratio Lower Upper
41 100
42 77.3 55.8 83.6


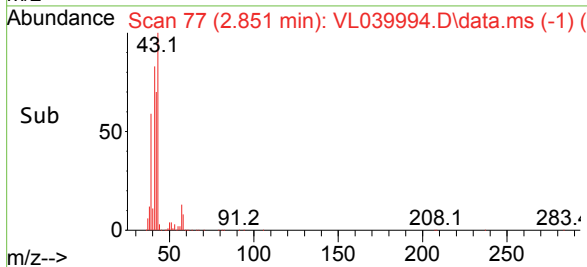
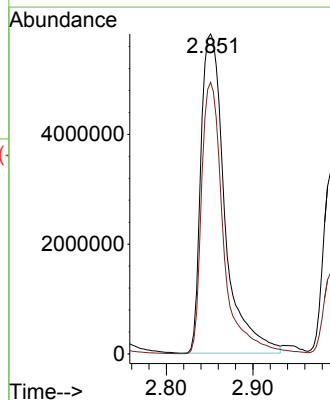
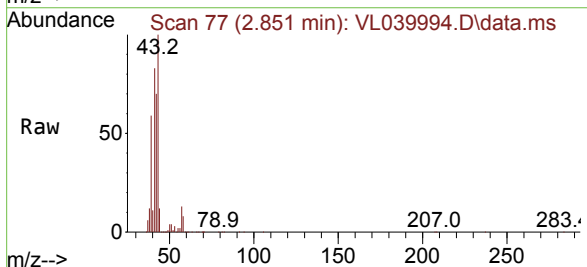




#10
Heptane
Concen: 72.764 ppbv
RT: 7.581 min Scan# 11
Delta R.T. 0.035 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58




Instrument :
MSVOA_L
ClientSampleId :
SG-1


Tgt Ion: 43 Resp:10848423
Ion Ratio Lower Upper
43 100
57 55.7 40.7 61.1

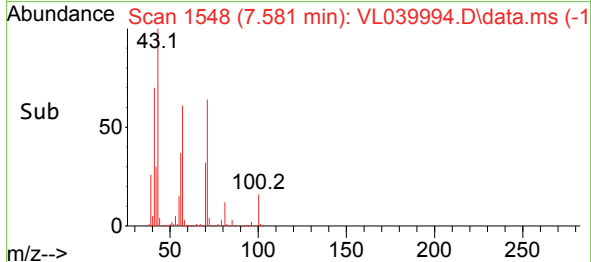

#11
Trichlorofluoromethane
Concen: 0.027 ppbv
RT: 3.542 min Scan# 292
Delta R.T. 0.013 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion:101 Resp: 4453
Ion Ratio Lower Upper
101 100
103 85.7 52.6 78.8#


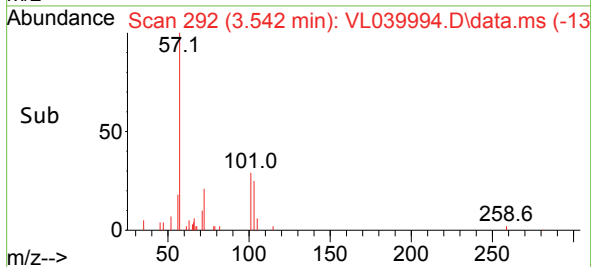

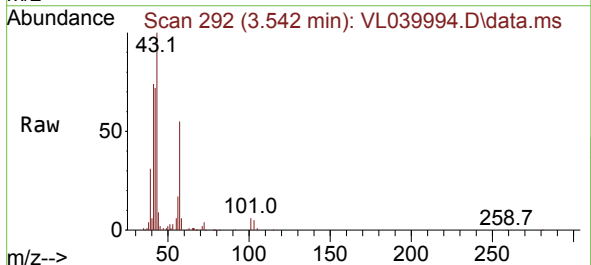




#13
Ethanol
Concen: 8.930 ppbv
RT: 3.224 min Scan# 19
Delta R.T. 0.010 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58




Instrument :
MSVOA_L
ClientSampleId :
SG-1


Tgt Ion: 45 Resp: 42125
Ion Ratio Lower Upper
45 100
46 46.6 14.6 58.2

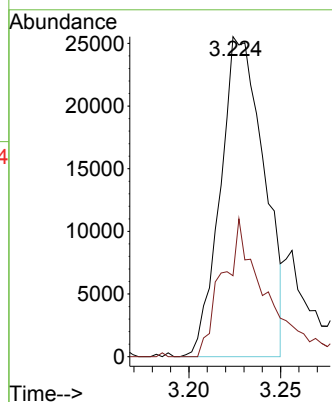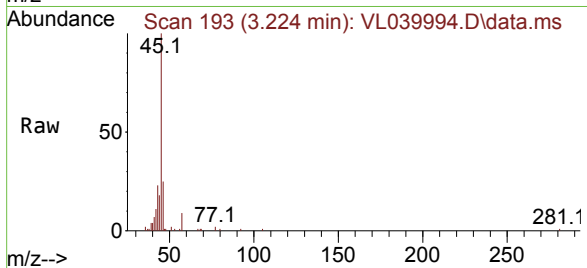

#15
Acetone
Concen: 43.193 ppbv
RT: 3.472 min Scan# 270
Delta R.T. 0.039 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion: 43 Resp: 5445729
Ion Ratio Lower Upper
43 100
58 5.7 22.9 34.3#


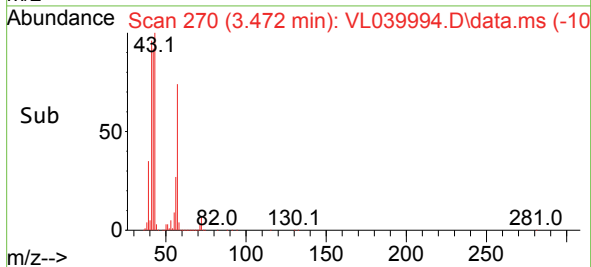
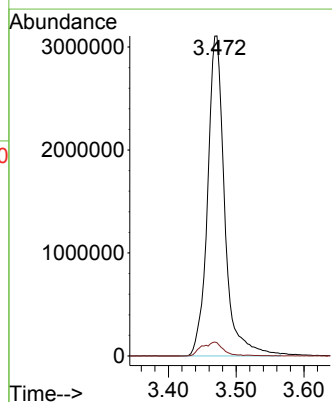
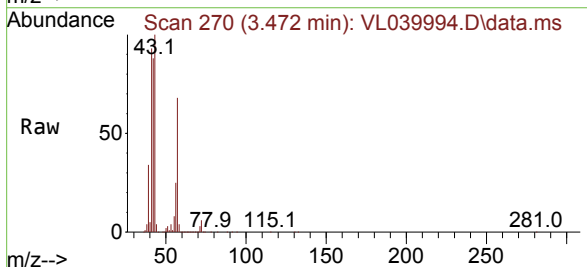




#16
1,3-Butadiene
Concen: 37.825 ppbv
RT: 2.989 min Scan# 11
Delta R.T. 0.039 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58




Instrument :
MSVOA_L
ClientSampleId :
SG-1


Tgt Ion: 39 Resp: 2376811
Ion Ratio Lower Upper
39 100
54 1.8 66.6 99.8#

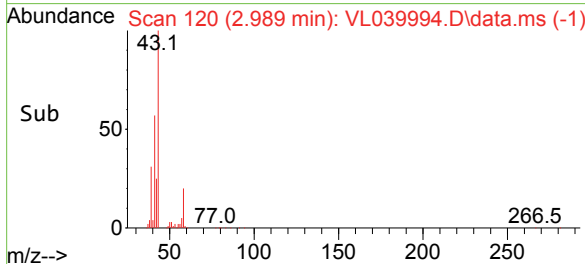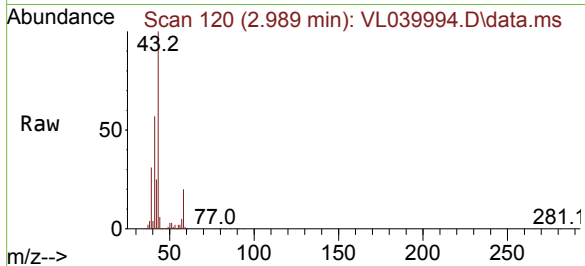

#19
Isopropyl Alcohol
Concen: 0.549 ppbv
RT: 3.571 min Scan# 301
Delta R.T. 0.029 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion: 45 Resp: 37478
Ion Ratio Lower Upper
45 100
58 0.0 38.7 58.1#


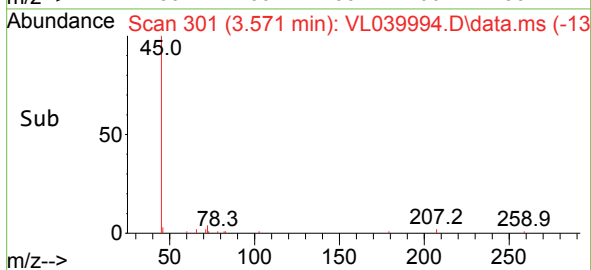

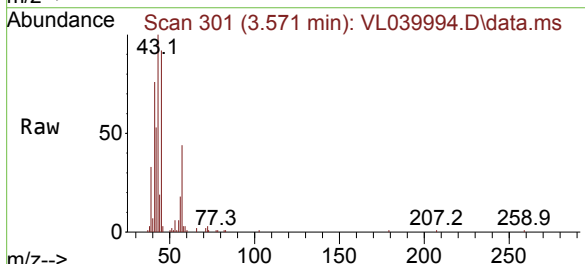




#20
Methylene Chloride
Concen: 1.189 ppbv
RT: 3.912 min Scan# 407
Delta R.T. 0.016 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58




Instrument :
MSVOA_L
ClientSampleId :
SG-1


Tgt Ion: 84	Resp: 72655
Ion Ratio	Lower Upper
84 100	
49 167.0	122.2 183.4
51 45.5	36.3 54.5
86 58.4	47.2 70.8

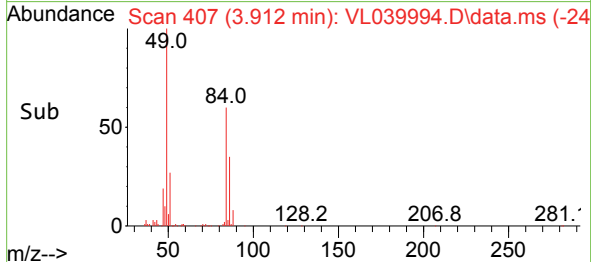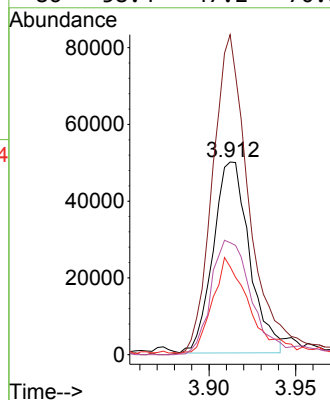

#21
Allyl Chloride
Concen: 13.969 ppbv
RT: 4.147 min Scan# 480
Delta R.T. 0.187 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion: 41		Resp: 1221669	
Ion	Ratio	Lower	Upper
41	100		
76	0.1	25.6	38.4#
39	41.6	65.2	97.8#

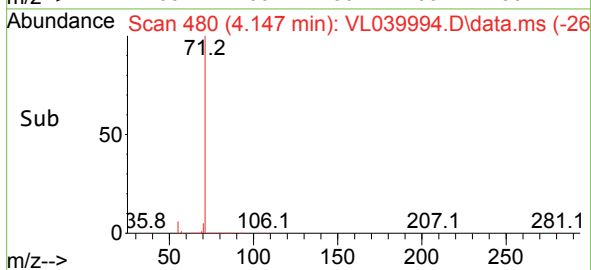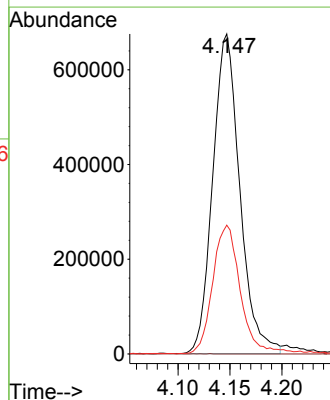







#23
 Vinyl Acetate
 Concen: 63.624 ppbv
 RT: 4.587 min Scan# 615
 Delta R.T. -0.006 min
 Lab File: VL039994.D
 Acq: 13 Dec 2022 2:58

Instrument :
 MSVOA_L
 ClientSampleId :
 SG-1

Tgt Ion: 43 Resp: 3295522




Ion	Ratio	Lower	Upper
43	100		
86	3.1	5.0	7.4#
42	88.7	7.6	11.4#
44	3.4	3.8	5.6#

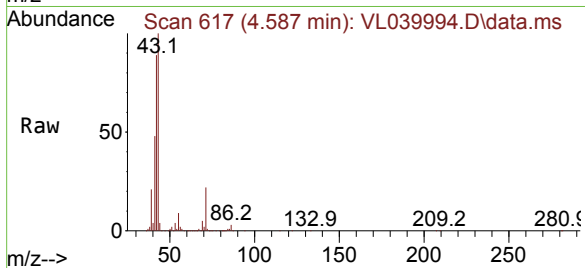


#24
 1,1-Dichloroethane
 Concen: 0.056 ppbv
 RT: 4.581 min Scan# 615
 Delta R.T. 0.052 min
 Lab File: VL039994.D
 Acq: 13 Dec 2022 2:58

Tgt Ion: 63 Resp: 6993

Ion	Ratio	Lower	Upper
63	100		
98	0.0	2.1	6.5#
100	0.0	1.1	3.5#


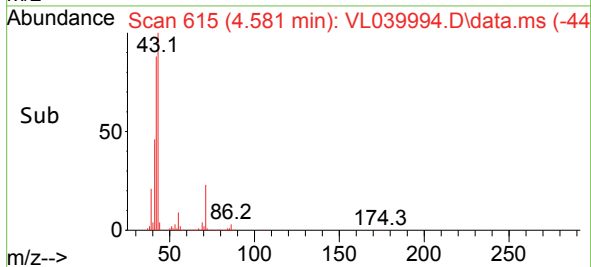

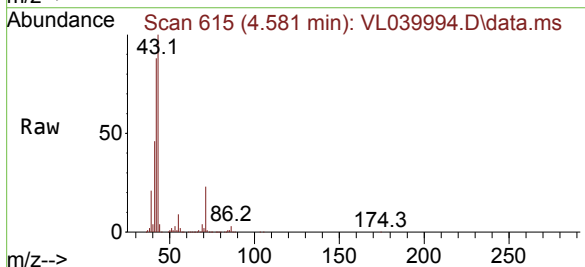




#25
Ethyl Acetate
Concen: 7.376 ppbv
RT: 5.192 min Scan# 805
Delta R.T. 0.023 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58




Instrument :
MSVOA_L
ClientSampleId :
SG-1


Tgt Ion: 43 Resp: 1707515
Ion Ratio Lower Upper
43 100
45 0.2 8.4 12.6#
61 0.2 8.5 12.7#
70 1.5 5.9 8.9#

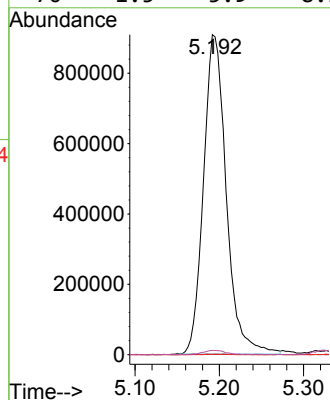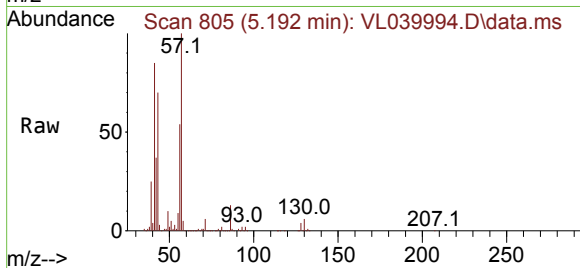

#26
Hexane
Concen: 24.920 ppbv
RT: 5.195 min Scan# 806
Delta R.T. 0.019 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion: 57 Resp: 2520006
Ion Ratio Lower Upper
57 100
41 86.2 72.3 108.5
43 68.6 188.7 283.1#
56 53.3 42.4 63.6

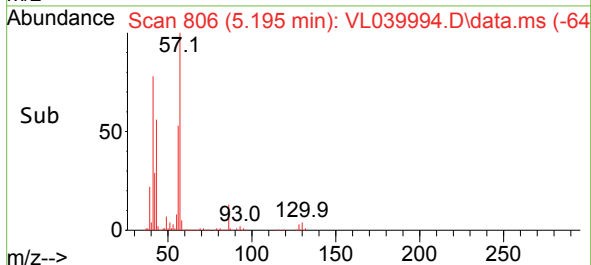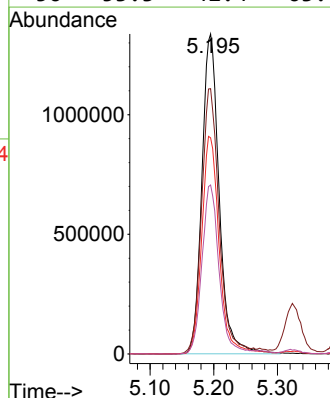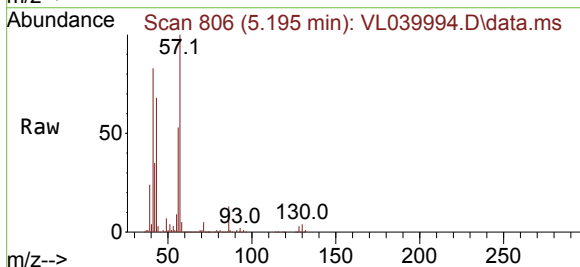



#29

Chloroform

Concen: 0.030 ppbv

RT: 5.253 min Scan# 81

Delta R.T. 0.016 min

Lab File: VL039994.D

Acq: 13 Dec 2022 2:58

Instrument :

MSVOA_L

ClientSampleId :





SG-1

Tgt Ion: 83 Resp: 4056

Ion Ratio Lower Upper

83 100

85 35.9 52.4 78.6#

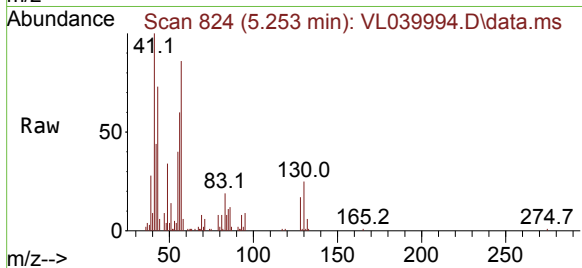

#30

Cyclohexane

Concen: 5.889 ppbv

RT: 6.587 min Scan# 1239

Delta R.T. 0.023 min

Lab File: VL039994.D

Acq: 13 Dec 2022 2:58




Tgt Ion: 84 Resp: 584449


Ion Ratio Lower Upper

84 100

56 137.0 112.5 168.7

41 128.2 67.8 101.8#

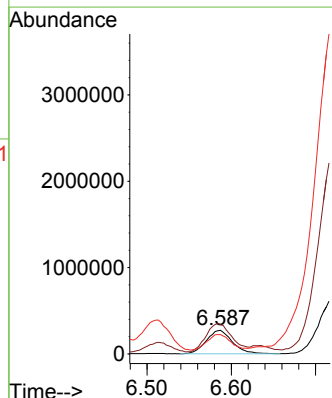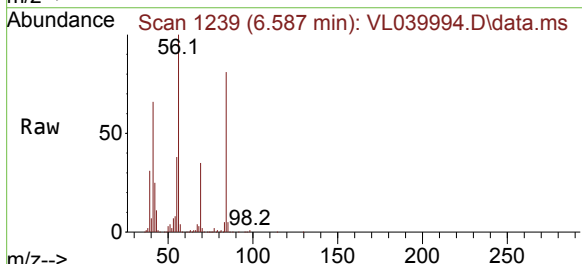



#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 6.632 min Scan# 11

Delta R.T. 0.013 min

Lab File: VL039994.D

Acq: 13 Dec 2022 2:58

Instrument :

MSVOA_L

ClientSampleId :

SG-1





Tgt Ion:114 Resp: 2778922

Ion Ratio Lower Upper

114 100

63 26.0 21.4 32.0

88 18.6 15.3 22.9

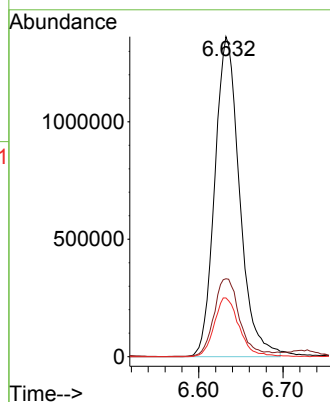

#34

2-Butanone

Concen: 0.423 ppbv

RT: 4.780 min Scan# 677

Delta R.T. 0.029 min

Lab File: VL039994.D




Acq: 13 Dec 2022 2:58


Tgt Ion: 43 Resp: 56181

Ion Ratio Lower Upper

43 100

72 27.1 17.4 26.2#


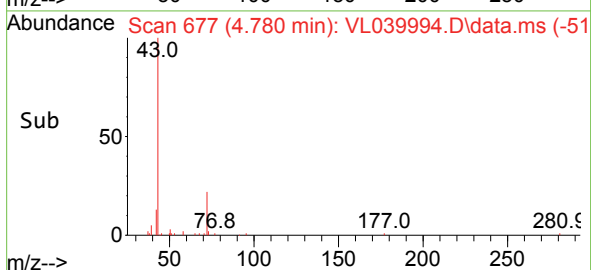
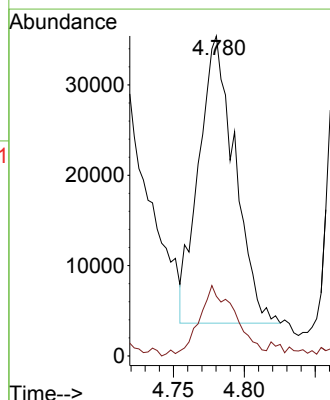



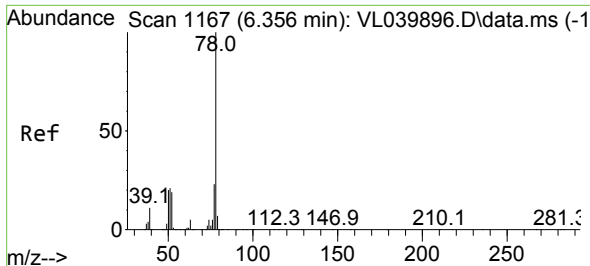

#36
Benzene
Concen: 0.248 ppbv
RT: 6.346 min Scan# 1167
Delta R.T. 0.013 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58




Instrument :
MSVOA_L
ClientSampleId :
SG-1


Tgt Ion: 78 Resp: 58546
Ion Ratio Lower Upper
78 100
77 6.6 18.2 27.2#
50 13.5 15.8 23.8#

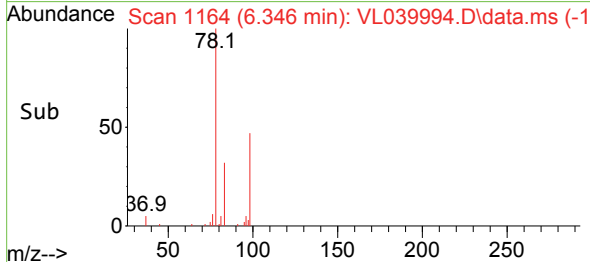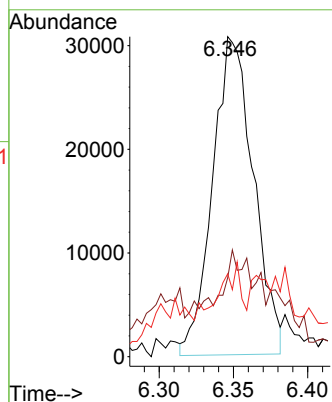

#39
1,2-Dichloropropane
Concen: 0.728 ppbv
RT: 6.954 min Scan# 1353
Delta R.T. -0.080 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion: 63 Resp: 67017
Ion Ratio Lower Upper
63 100
41 11805.9 54.7 82.1#
62 45.6 55.0 82.6#

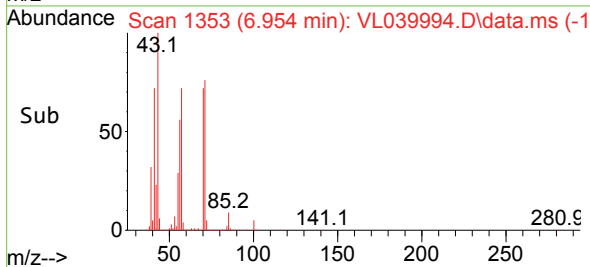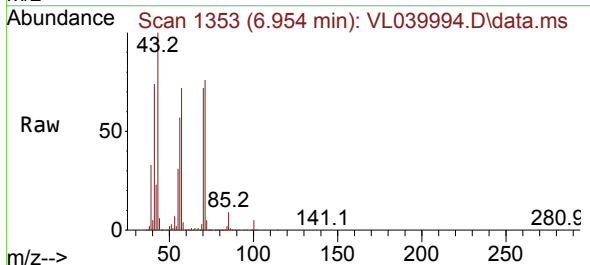



#41

Tetrahydrofuran

Concen: 0.367 ppbv

RT: 5.407 min Scan# 81

Delta R.T. -0.112 min

Lab File: VL039994.D

Acq: 13 Dec 2022 2:58

Instrument :

MSVOA_L

ClientSampleId :

SG-1





Tgt Ion: 42 Resp: 33677

Ion Ratio Lower Upper

42 100

72 0.0 31.6 47.4#

71 0.0 31.2 46.8#

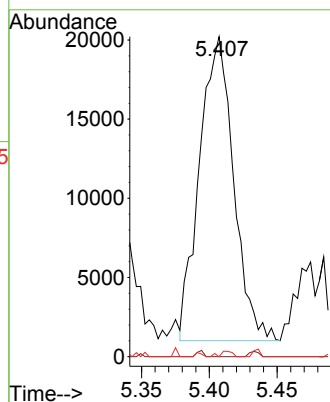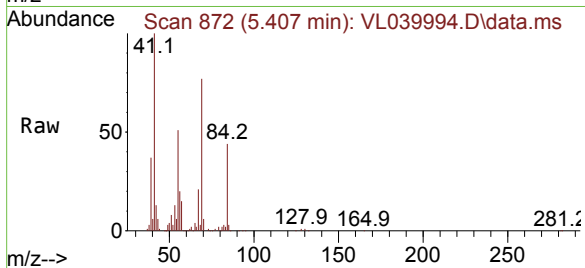

#42

Bromodichloromethane

Concen: 6.492 ppbv

RT: 7.250 min Scan# 1445

Delta R.T. 0.039 min

Lab File: VL039994.D

Acq: 13 Dec 2022 2:58




Tgt Ion: 83 Resp: 1139585


Ion Ratio Lower Upper

83 100

85 2.1 52.0 78.0#

127 0.0 6.5 9.7#


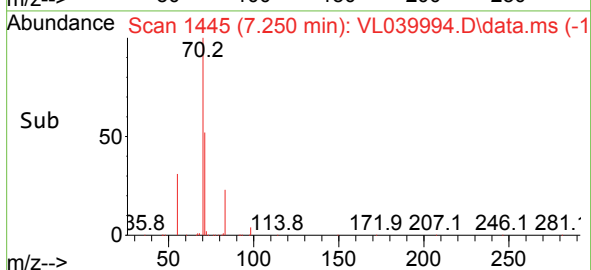
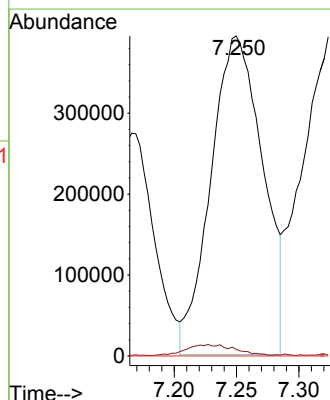
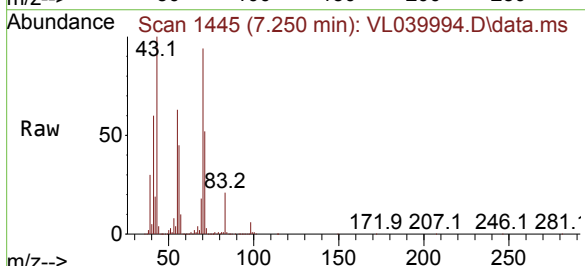




#43
Methyl Methacrylate
Concen: 11.514 ppbv
RT: 7.439 min Scan# 11
Delta R.T. 0.000 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58




Instrument :
MSVOA_L
ClientSampleId :
SG-1


Tgt Ion: 69 Resp: 1066332
Ion Ratio Lower Upper
69 100
41 91.2 116.4 174.6#
100 0.0 26.8 40.2#

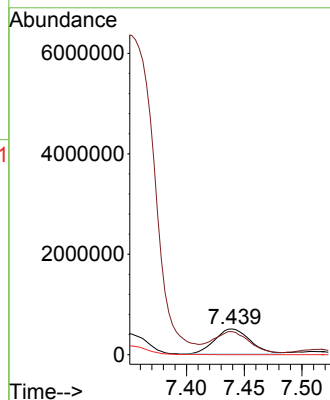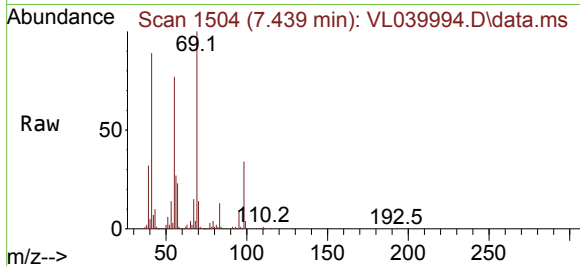

#44
2,2,4-Trimethylpentane
Concen: 16.825 ppbv
RT: 7.340 min Scan# 1473
Delta R.T. 0.048 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion: 57 Resp: 6634380
Ion Ratio Lower Upper
57 100
41 421.7 26.2 39.2#
56 431.0 25.5 38.3#

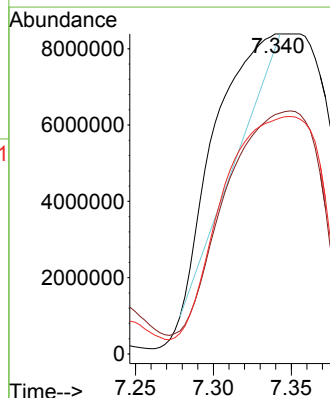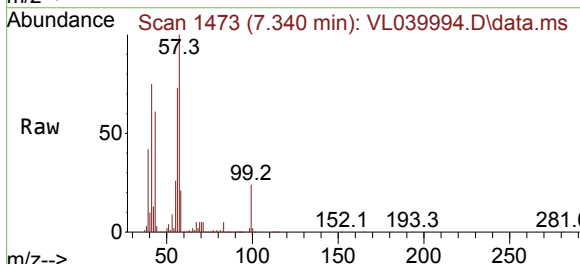

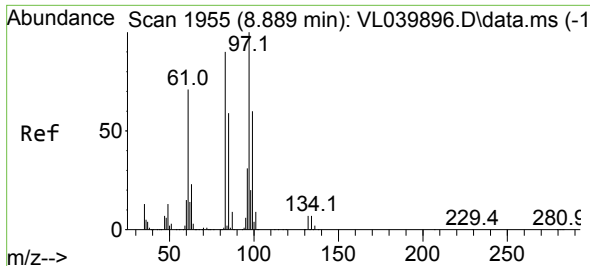

#47

1,1,2-Trichloroethane

Concen: 0.099 ppbv

RT: 8.883 min Scan# 1955

Delta R.T. 0.019 min

Lab File: VL039994.D

Acq: 13 Dec 2022 2:58

Instrument :

MSVOA_L

ClientSampleId :

SG-1

Tgt Ion: 97 Resp: 9349





Ion Ratio Lower Upper

97 100

83 93.7 72.1 108.1

85 0.0 47.2 70.8#

99 3.3 48.2 72.2#

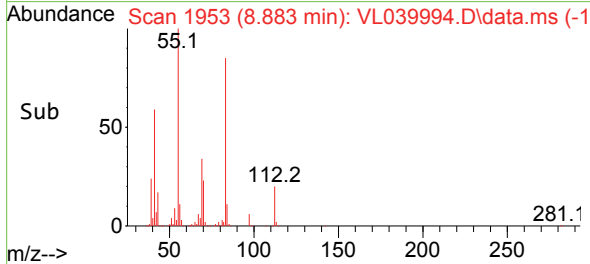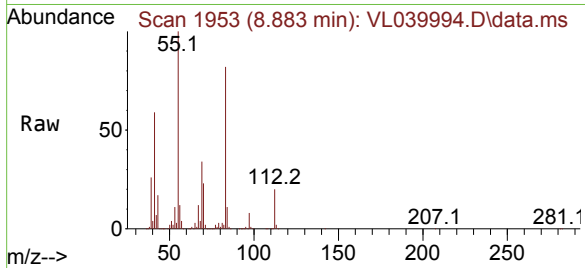

#50

4-Methyl-2-Pentanone

Concen: 7.454 ppbv

RT: 8.205 min Scan# 1742

Delta R.T. 0.058 min

Lab File: VL039994.D




Acq: 13 Dec 2022 2:58


Tgt Ion: 43 Resp: 1775183

Ion Ratio Lower Upper

43 100

58 27.4 29.8 44.6#


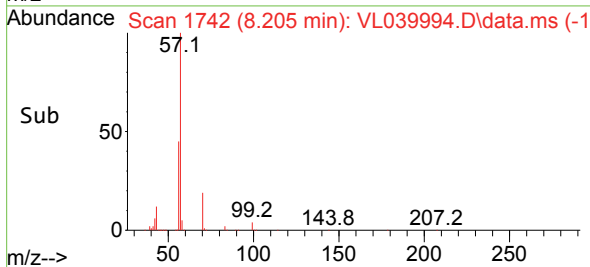

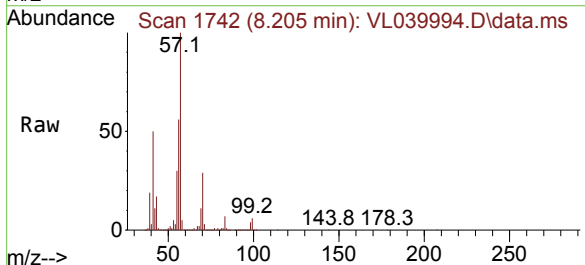




#51
2-Hexanone
Concen: 81.234 ppbv
RT: 9.552 min Scan# 2158
Delta R.T. 0.035 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58




Instrument :
MSVOA_L
ClientSampleId :
SG-1


Tgt Ion: 43 Resp:15017926
Ion Ratio Lower Upper
43 100
58 0.0 40.2 60.4#
98 0.0 0.1 0.1#

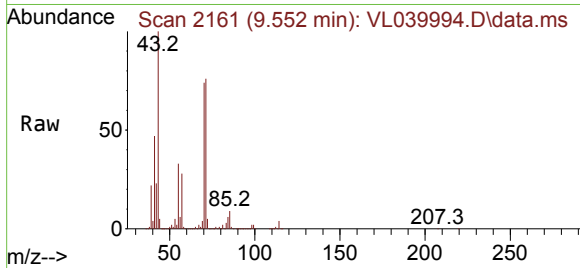

#52
Tetrachloroethene
Concen: 0.315 ppbv
RT: 10.616 min Scan# 2492
Delta R.T. 0.035 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion:164 Resp: 27842
Ion Ratio Lower Upper
164 100
166 102.5 98.3 147.5
129 102.1 79.7 119.5
131 83.3 80.2 120.4


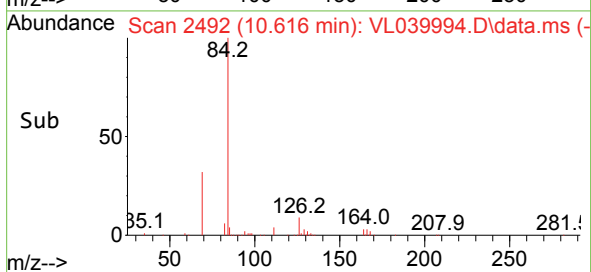

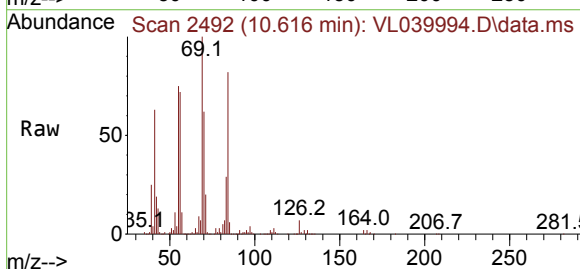




#53
Toluene
Concen: 0.071 ppbv
RT: 9.108 min Scan# 2056
Delta R.T. -0.077 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58




Instrument :
MSVOA_L
ClientSampleId :
SG-1


Tgt Ion: 91 Resp: 19192
Ion Ratio Lower Upper
91 100
92 54.5 49.8 74.6

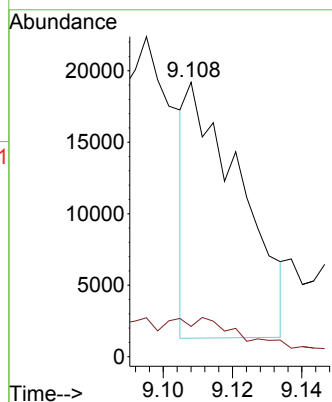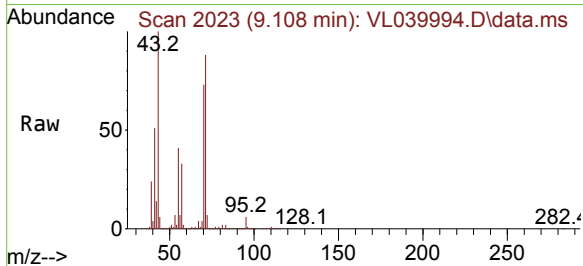

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.465 min Scan# 2756
Delta R.T. 0.032 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion: 117 Resp: 2484307
Ion Ratio Lower Upper
117 100
82 77.0 52.3 78.5
119 32.8 25.7 38.5


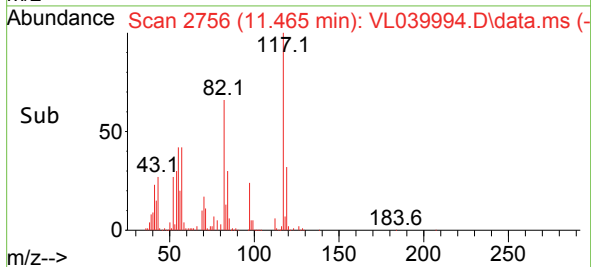

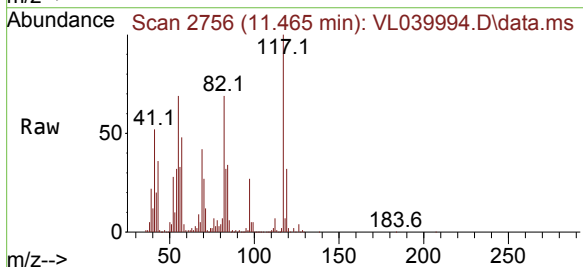




#57
Chlorobenzene
Concen: 0.791 ppbv
RT: 11.571 min Scan# 21
Delta R.T. 0.080 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58




Instrument :
MSVOA_L
ClientSampleId :
SG-1


Tgt Ion:112 Resp: 150283
Ion Ratio Lower Upper
112 100
77 6.1 54.6 81.8#
114 0.4 30.1 36.7#

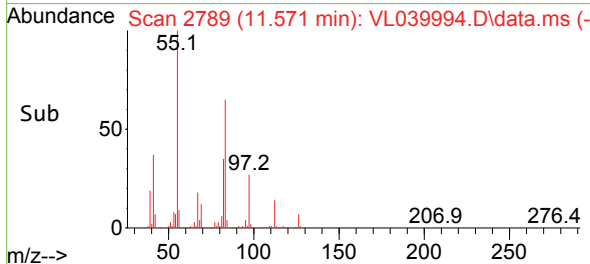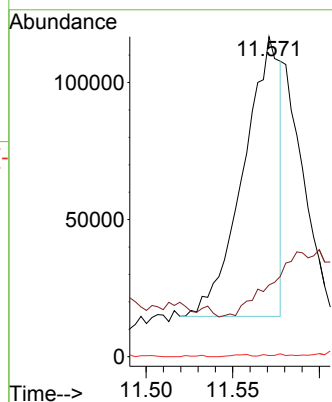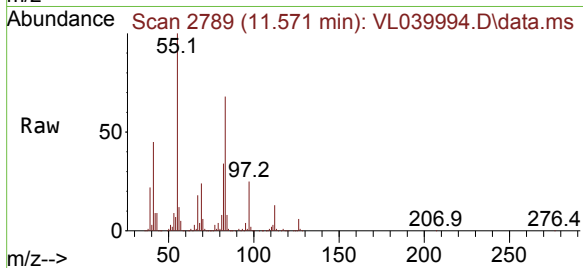

#59
m/p-Xylene
Concen: 0.326 ppbv
RT: 12.343 min Scan# 3029
Delta R.T. 0.003 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion: 91 Resp: 91962
Ion Ratio Lower Upper
91 100
106 11.8 37.0 55.6#

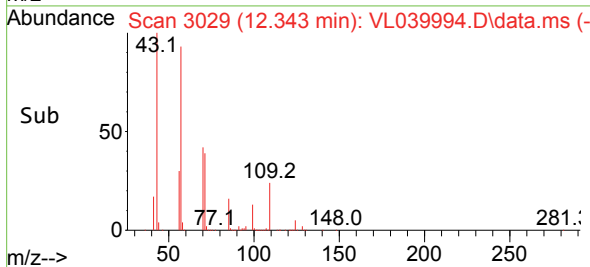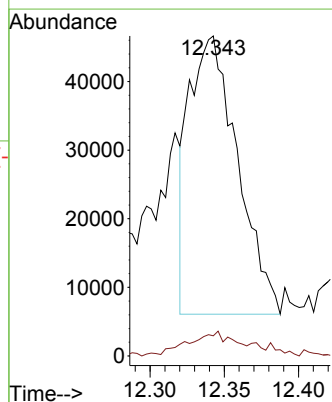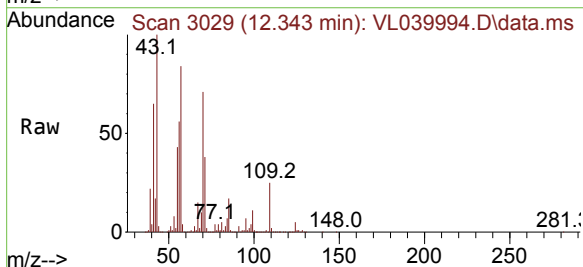



#62

Isopropylbenzene

Concen: 0.121 ppbv

RT: 14.024 min Scan# 3

Delta R.T. 0.029 min

Lab File: VL039994.D

Acq: 13 Dec 2022 2:58

Instrument :

MSVOA_L

ClientSampleId :





SG-1

Tgt Ion:105 Resp: 47024

Ion Ratio Lower Upper

105 100

120 30.8 21.4 32.2

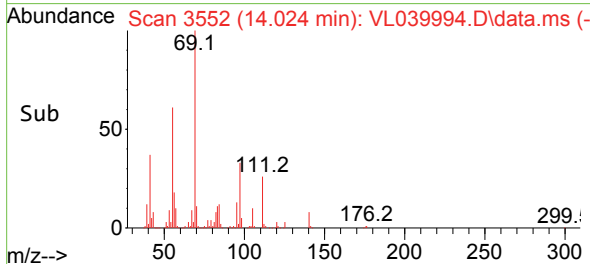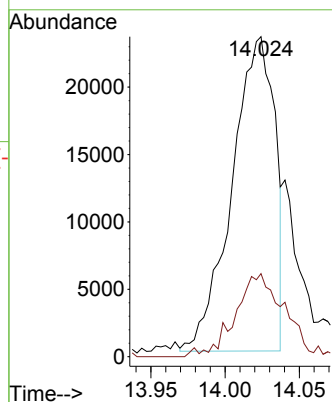

#63

1,1,2,2-Tetrachloroethane

Concen: 0.934 ppbv

RT: 13.040 min Scan# 3246

Delta R.T. 0.029 min

Lab File: VL039994.D

Acq: 13 Dec 2022 2:58




Tgt Ion: 83 Resp: 83853


Ion Ratio Lower Upper

83 100

131 0.0 4.6 13.8#

85 363.4 33.0 99.0#


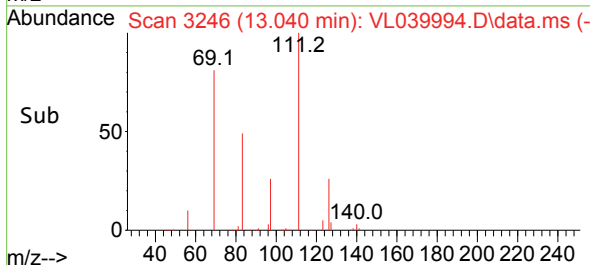

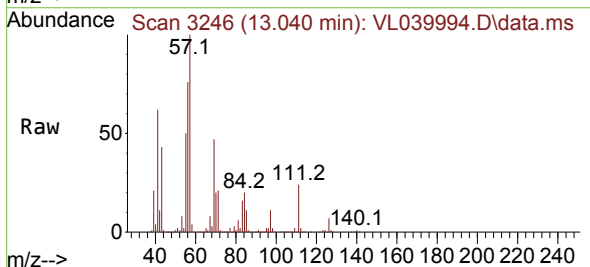




#68
1-Bromo-4-Fluorobenzene
Concen: 11.396 ppbv
RT: 13.773 min Scan# 3476
Delta R.T. 0.032 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Instrument :
MSVOA_L
ClientSampleId :
SG-1

Tgt Ion: 95 Resp: 2162394
Ion Ratio Lower Upper
95 100
174 63.4 53.7 80.5
175 4.5 4.0 6.0

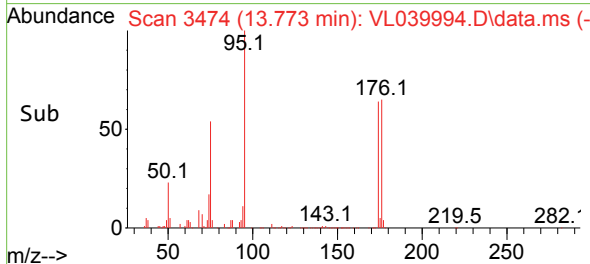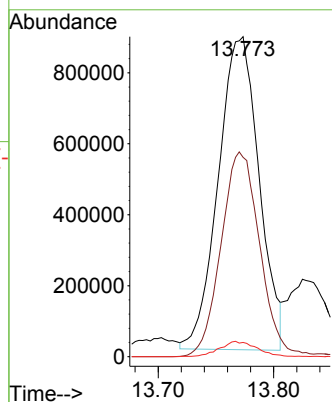

#80
Naphthalene,2-methyl-
Concen: 0.024 ppbv
RT: 24.400 min Scan# 6779
Delta R.T. 0.052 min
Lab File: VL039994.D
Acq: 13 Dec 2022 2:58

Tgt Ion:142 Resp: 1205
Ion Ratio Lower Upper
142 100
141 83.9 69.1 103.7
115 38.8 29.6 44.4

