


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121222\
Data File : VL039969.D
Acq On : 12 Dec 2022 9:59
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111822AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Dec 02 23:21:36 2022

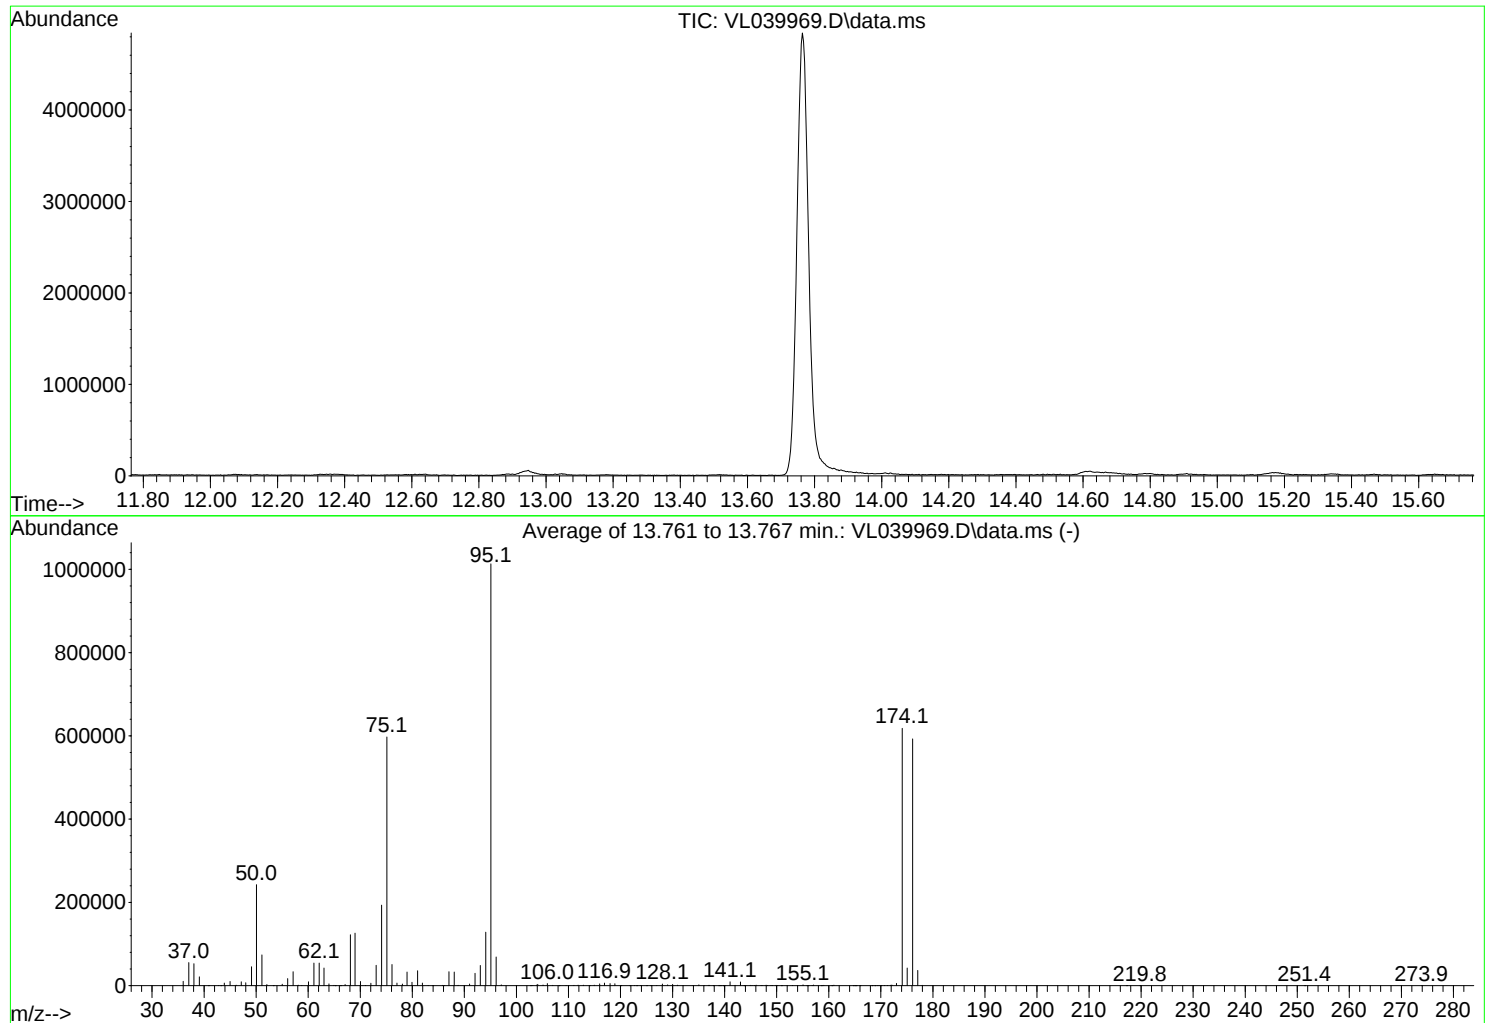

AutoFind: Scans 3470, 3471, 3472; Background Corrected with Scan 3444

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.9	242560	PASS
75	95	30	66	58.9	597141	PASS
95	95	100	100	100.0	1013248	PASS
96	95	5	9	6.8	68696	PASS
173	174	0.00	2	0.9	5279	PASS
174	95	50	120	61.0	618112	PASS
175	174	4	9	6.9	42432	PASS
176	174	93	101	95.9	592875	PASS
177	176	5	9	6.2	36611	PASS

Average of 13.761 to 13.767 min.: VL039969.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	10448	48.00	6872	60.05	9302	70.05	10111
37.05	55424	49.10	45501	61.10	54155	71.00	5111
38.05	52715	50.05	242560	62.10	54344	72.05	5941
39.10	21036	51.10	73720	63.05	42243	73.05	4888
40.85	161	52.05	2628	64.00	4467	74.10	193301
42.80	515	53.30	183	64.95	802	75.10	597141
43.20	164	55.00	3340	65.20	108	76.10	50800
43.90	6381	56.05	16827	66.20	72	77.05	6159
45.00	10064	57.10	33283	67.10	2909	78.10	3741
46.15	1098	58.10	1243	68.10	122269	79.00	32587
47.15	9432	58.75	411	69.00	126259	79.95	8266

Average of 13.761 to 13.767 min.: VL039969.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.00	35907	93.05	48510	107.00	954	118.00	4893
81.95	6095	94.10	128256	108.20	162	118.90	4527
83.05	530	95.10	1.01325e+006	109.55	261	120.05	183
83.90	52	96.10	68696	110.05	381	121.80	96
85.85	820	97.10	2085	111.05	946	122.70	383
86.20	337	102.70	146	111.85	1029	123.10	88
87.05	33539	103.15	330	112.85	1184	123.90	288
88.05	32643	103.90	1427	114.00	67	124.05	608
88.80	843	104.10	3175	114.95	1110	125.00	68
91.00	3879	105.10	1585	116.00	4140	125.80	159
92.05	29811	105.95	5138	116.90	6259	126.00	497

Average of 13.761 to 13.767 min.: VL039969.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.95	460	137.80	109	145.25	448	150.90	66
128.05	4008	138.85	227	145.70	298	152.00	399
129.05	2075	139.20	177	146.05	1125	153.05	398
130.00	3096	139.70	133	147.00	518	154.00	508
130.95	1135	139.90	111	147.20	397	155.05	2115
132.00	286	141.05	9452	147.95	1345	155.80	51
133.95	305	142.00	996	148.20	521	156.00	174
135.05	1955	143.05	8970	148.90	433	156.80	402
136.05	432	143.70	133	149.15	535	157.10	1627
136.85	784	144.05	417	149.85	779	158.60	114
137.10	823	144.90	727	150.20	264	159.05	920

Average of 13.761 to 13.767 min.: VL039969.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.60	154	170.70	455	217.20	59		
161.00	1041	171.30	266	219.80	92		
164.70	108	171.90	674	251.40	53		
165.00	72	172.00	1036	273.90	70		
165.25	189	172.15	1276				
166.00	77	173.00	5279				
168.30	56	174.10	618112				
168.85	223	175.05	42432				
169.40	283	176.10	592875				
169.65	345	177.10	36611				
170.00	162	177.95	877				