Quantitation Report (QT Reviewed)

Data Path : W:\HPCHEM1\MSVOA_L\DATA\VL121317\
Data File : VL031238.D
Acq On : 14 Dec 2017 19:04
Operator : SY/AP
Sample : I6907-03DL 40X
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
INFLUENTDL

Manual Integrations APPROVED
MMDadoda
12/15/2017 4:07:17 PM

Quant Time: Dec 15 07:17:33 2017
Quant Method : W:\HPCHEM1\MSVOA_L\METHODS\VL121317AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LThu Dec 1
QLast Update : Thu Dec 14 04:29:58 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units		Dev(Min)
1) Bromochloromethane	5.91	49	1711827	10.00	ppbv		0.00
33) 1,4-Difluorobenzene	7.45	114	4062527	10.00	ppbv		0.00
55) Chlorobenzene-d5	12.41	117	4087836	10.00	ppbv		0.00
System Monitoring Compounds							
68) 1-Bromo-4-Fluorobenzene	14.75	95	3195150	10.99	ppbv		0.00
Spiked Amount 10.000	Range 65 - 135		Recovery = 109.90%				
Target Compounds							Qvalue
12) 1,1,2-Trichlorotrifluoroet	4.68	101	21911	0.13	ppbv		97
15) Acetone	4.05	43	59768	0.26	ppbv	#	70
18) 1,1-Dichloroethene	4.49	96	10283m	0.14	ppbv		
24) 1,1-Dichloroethane	5.23	63	138461	0.52	ppbv		98
32) 1,1,1-Trichloroethane	6.77	97	447686	1.42	ppbv		98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : W:\HPCHEM1\MSVOA_L\DATA\VL121317\
Data File : VL031238.D
Acq On : 14 Dec 2017 19:04
Operator : SY/AP
Sample : I6907-03DL 40X
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 07:17:33 2017
Quant Method : W:\HPCHEM1\MSVOA_L\METHODS\VL121317AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LThu Dec
QLast Update : Thu Dec 14 04:29:58 2017
Response via : Initial Calibration

Instrument :
MSVOA_L
ClientSampleId :
INFLUENTDL
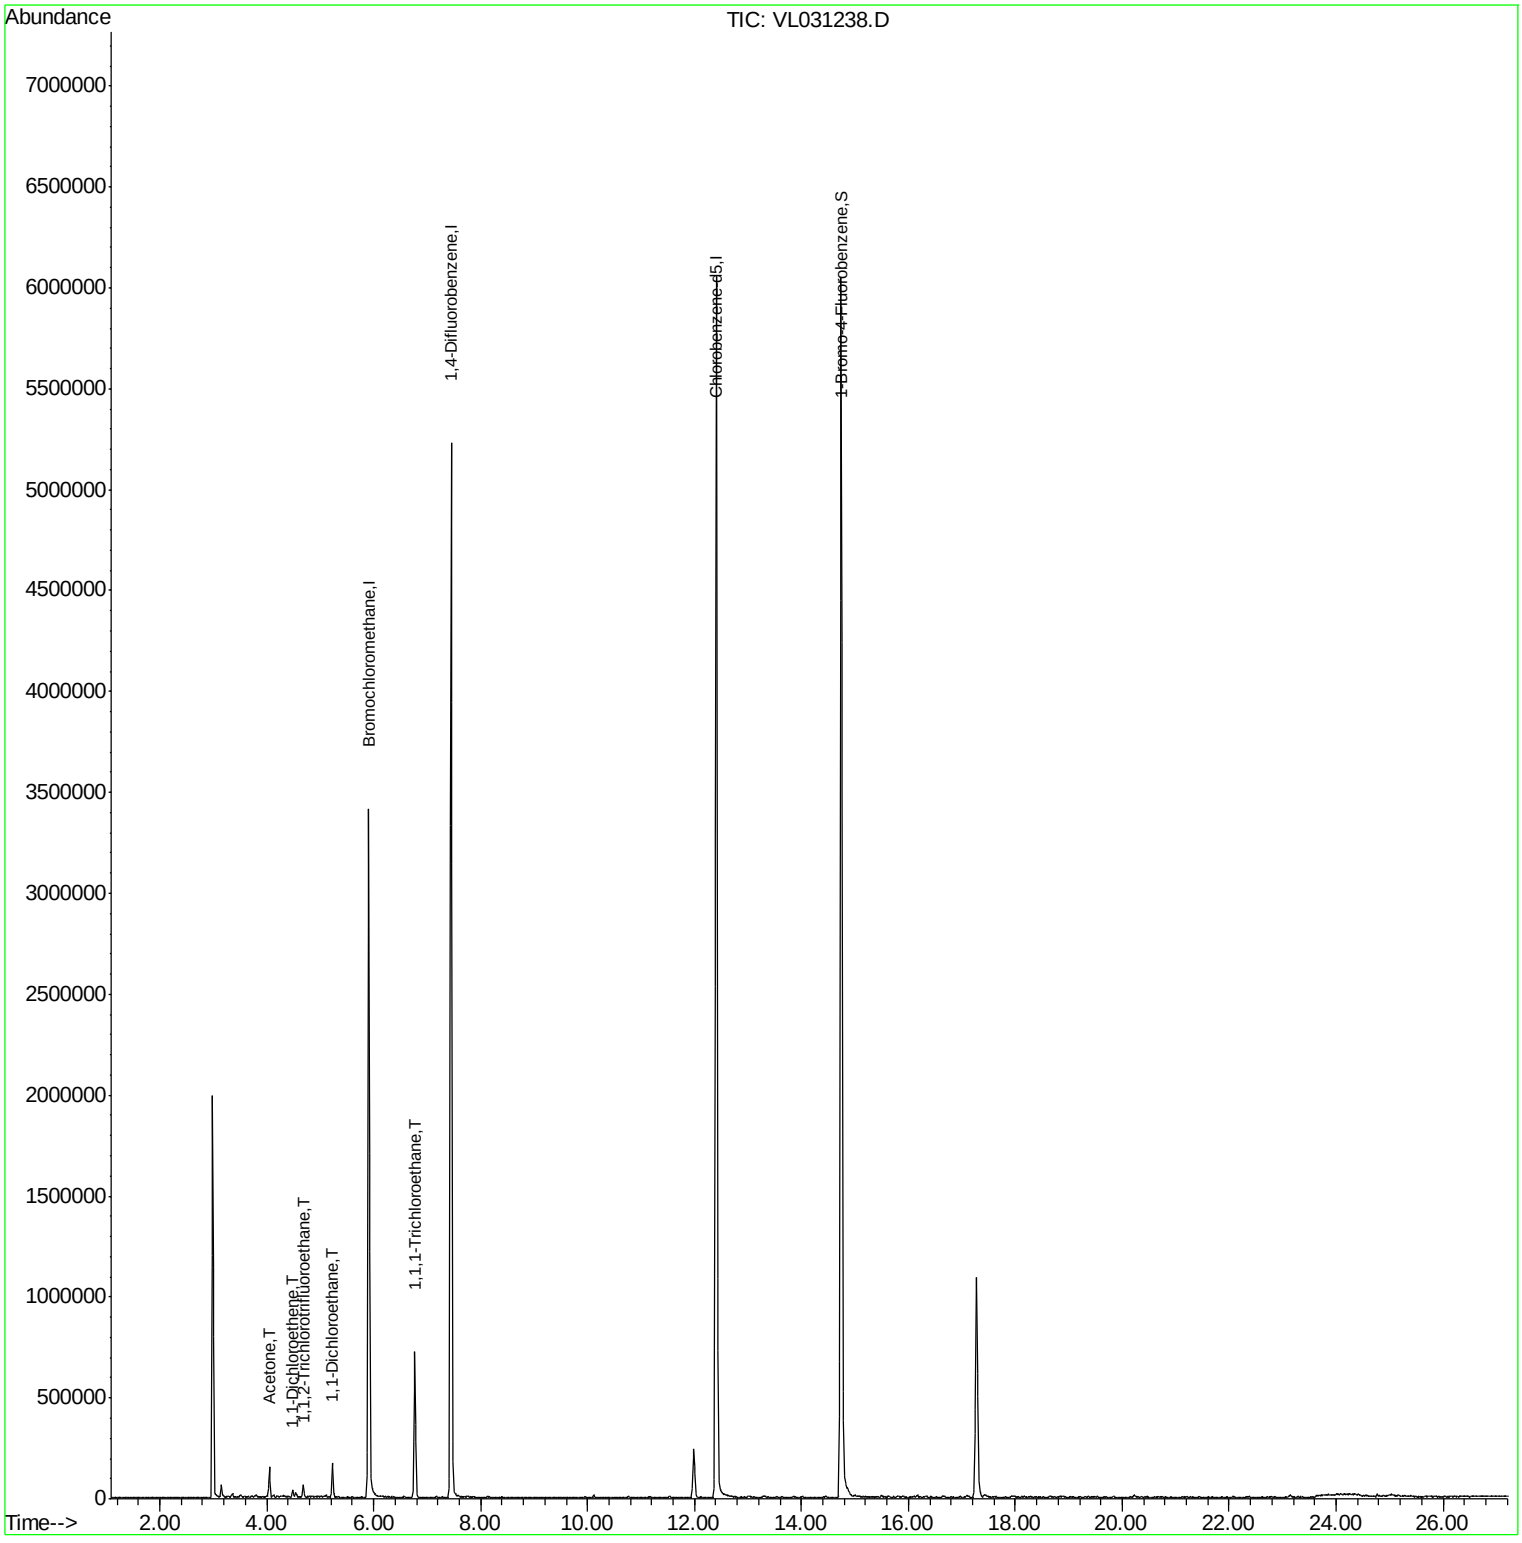
Manual Integrations APPROVED
MMDadoda
12/15/2017 4:07:17 PM