


Data Path : W:\HPCHEM1\MSVOA L\DATA\VL121317\  
Data File : VL031211.D  
Acq On : 13 Dec 2017 21:09  
Operator : SY/AP  
Sample : BFB  
Misc : 400ml/MSVOA L  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_L  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA\_L\METHODS\VL121317AIR.M  
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Thu Dec 14 04:29:58 2017  
Last Update : Thu Dec 14 04:29:58 2017

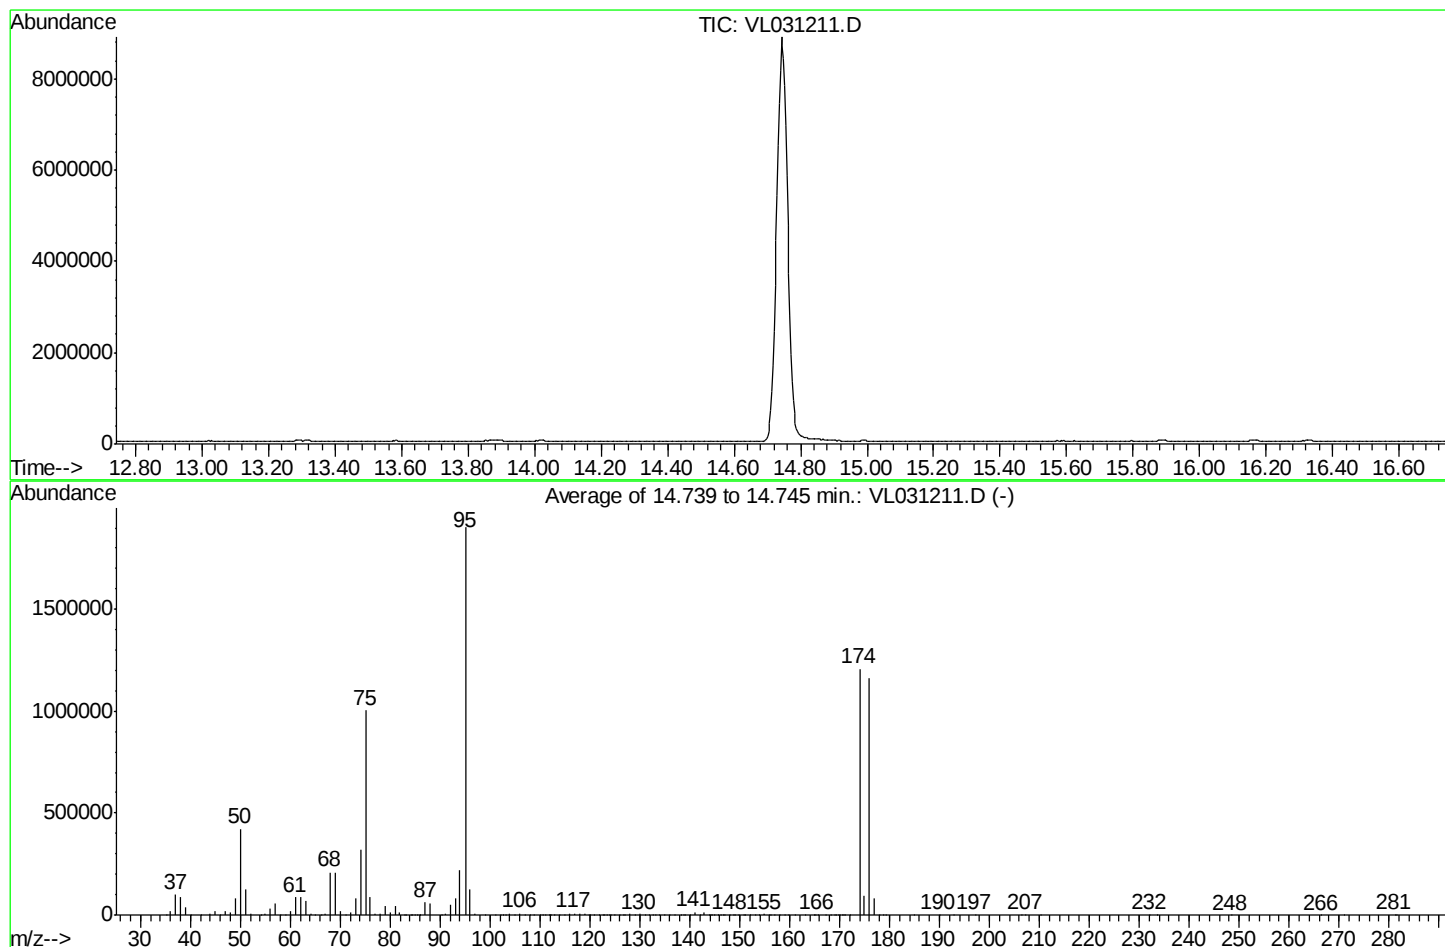

AutoFind: Scans 4246, 4247, 4248; Background Corrected with Scan 4215

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 8            | 40           | 22.3      | 423530  | PASS             |
| 75          | 95           | 30           | 66           | 52.8      | 1003925 | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 1902080 | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 125536  | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 120          | 63.4      | 1206784 | PASS             |
| 175         | 174          | 4            | 9            | 8.1       | 97370   | PASS             |
| 176         | 174          | 93           | 101          | 96.3      | 1162410 | PASS             |
| 177         | 176          | 5            | 9            | 6.9       | 79968   | PASS             |