


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL121318\
 Data File : VL032983.D
 Acq On : 13 Dec 2018 12:57
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL120718AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Dec 07 09:35:17 2018
 Last Update : Fri Dec 07 09:35:17 2018

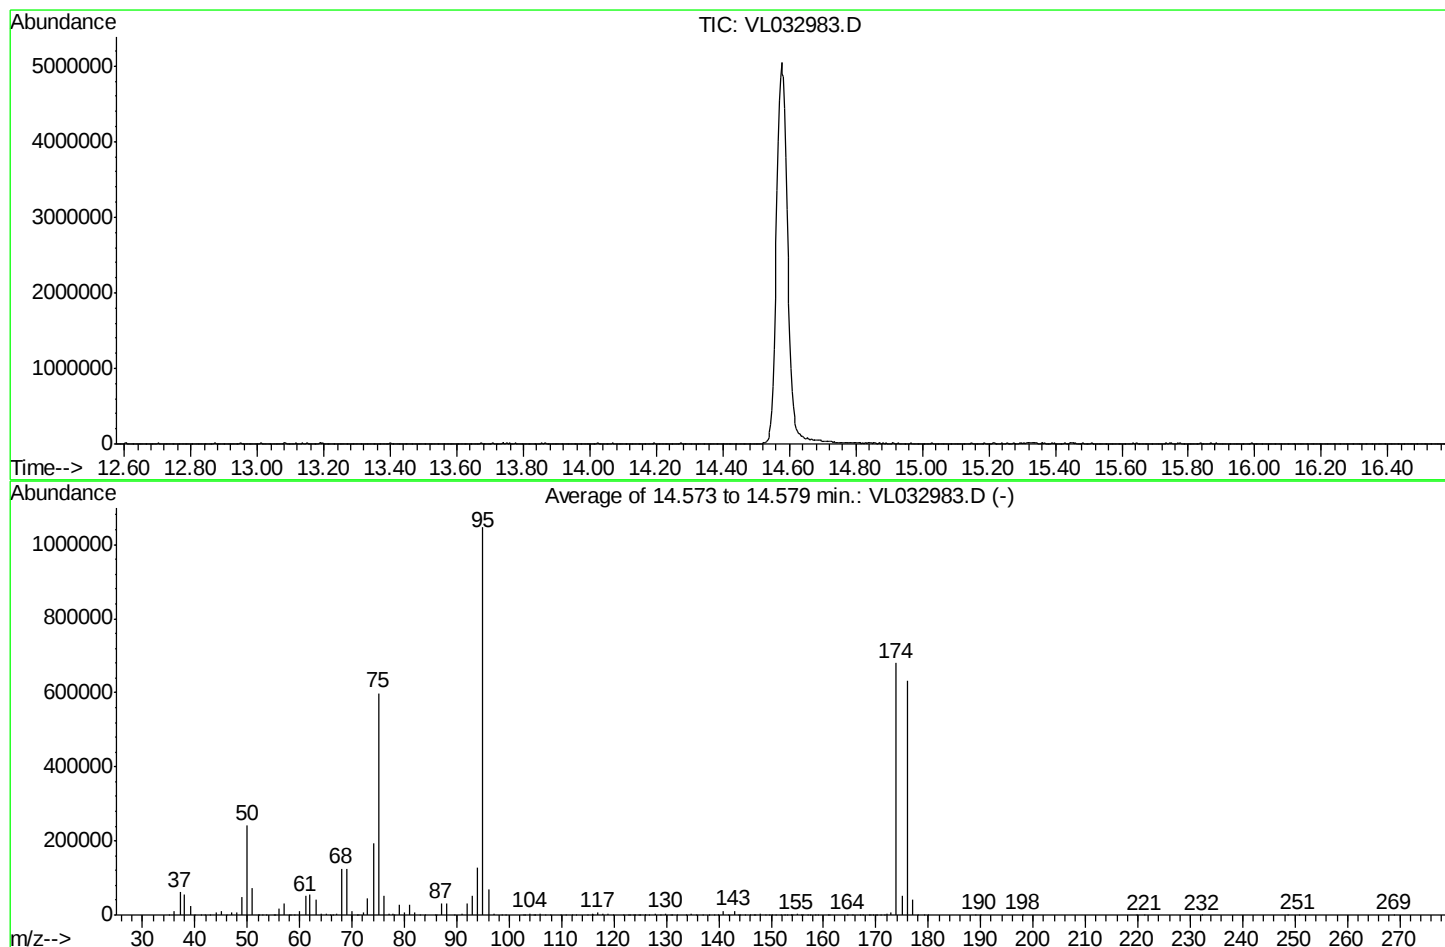

AutoFind: Scans 3619, 3620, 3621; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.1	241749	PASS
75	95	30	66	57.2	598165	PASS
95	95	100	100	100.0	1046556	PASS
96	95	5	9	6.5	67962	PASS
173	174	0.00	2	1.1	7708	PASS
174	95	50	120	65.0	680106	PASS
175	174	4	9	7.4	50613	PASS
176	174	93	101	93.2	633813	PASS
177	176	5	9	6.8	43120	PASS