


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL121421\
 Data File : VL038162.D
 Acq On : 14 Dec 2021 10:33
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL111821AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Nov 18 13:16:09 2021
 Last Update : Thu Nov 18 13:16:09 2021

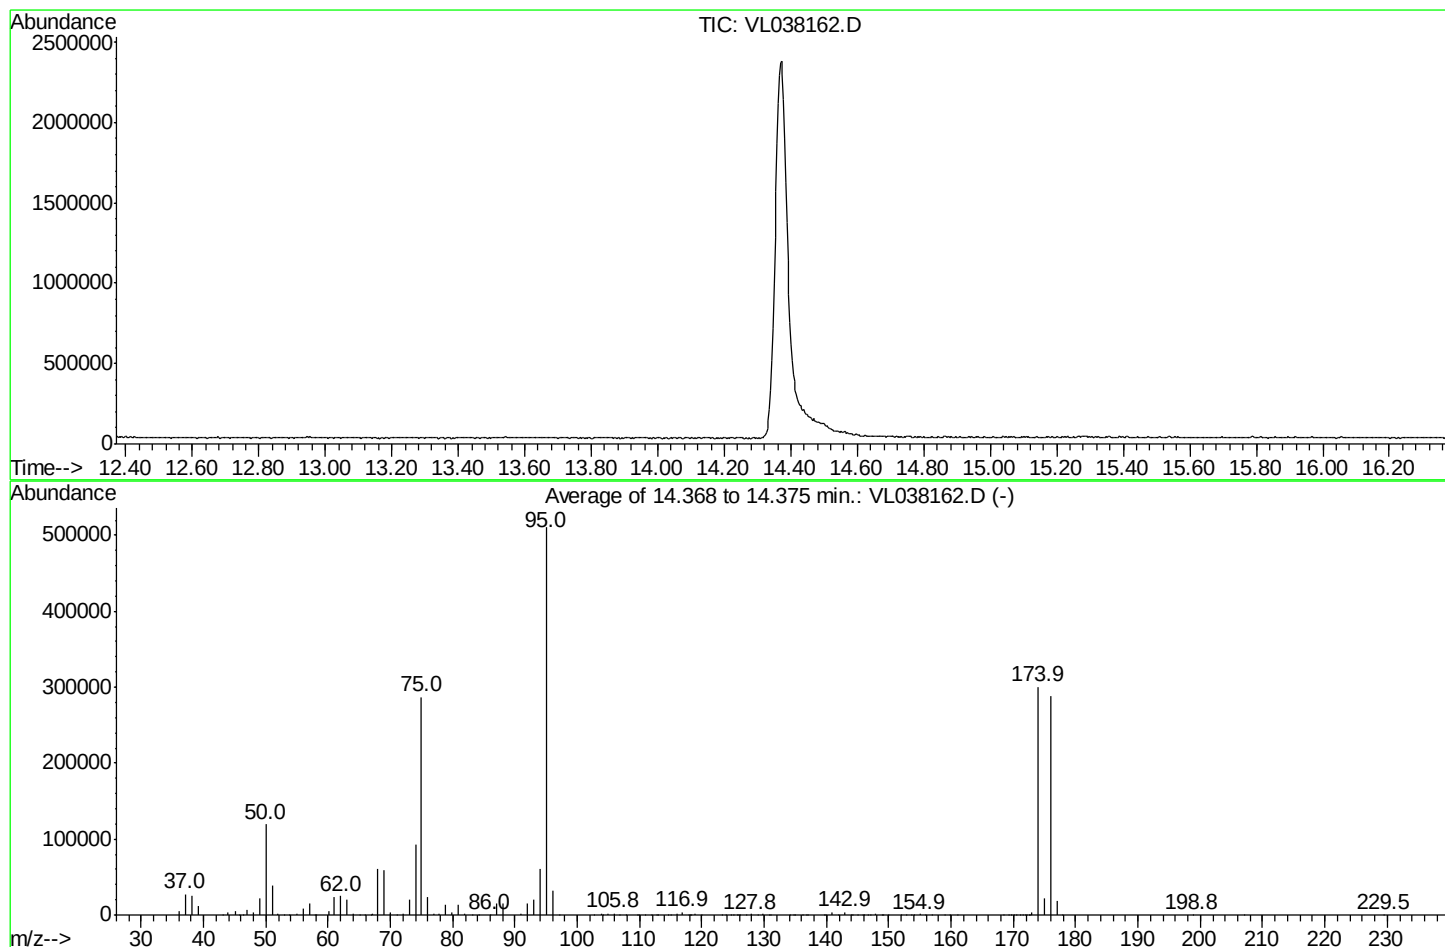

AutoFind: Scans 3602, 3603, 3604; Background Corrected with Scan 3579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.4	119408	PASS
75	95	30	66	56.2	287104	PASS
95	95	100	100	100.0	510506	PASS
96	95	5	9	6.3	32410	PASS
173	174	0.00	2	1.0	2984	PASS
174	95	50	120	58.8	300245	PASS
175	174	4	9	7.5	22552	PASS
176	174	93	101	96.3	289066	PASS
177	176	5	9	6.3	18261	PASS