
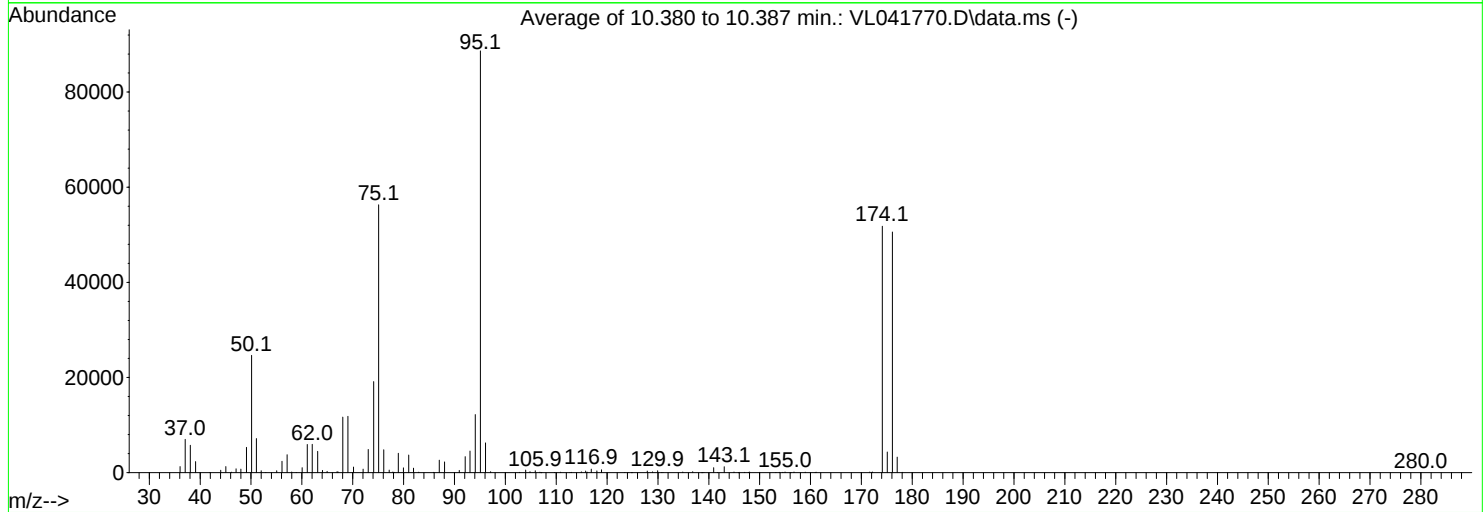


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121724\
Data File : VL041770.D
Acq On : 17 Dec 2024 08:44
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Dec 19 07:32:09 2024

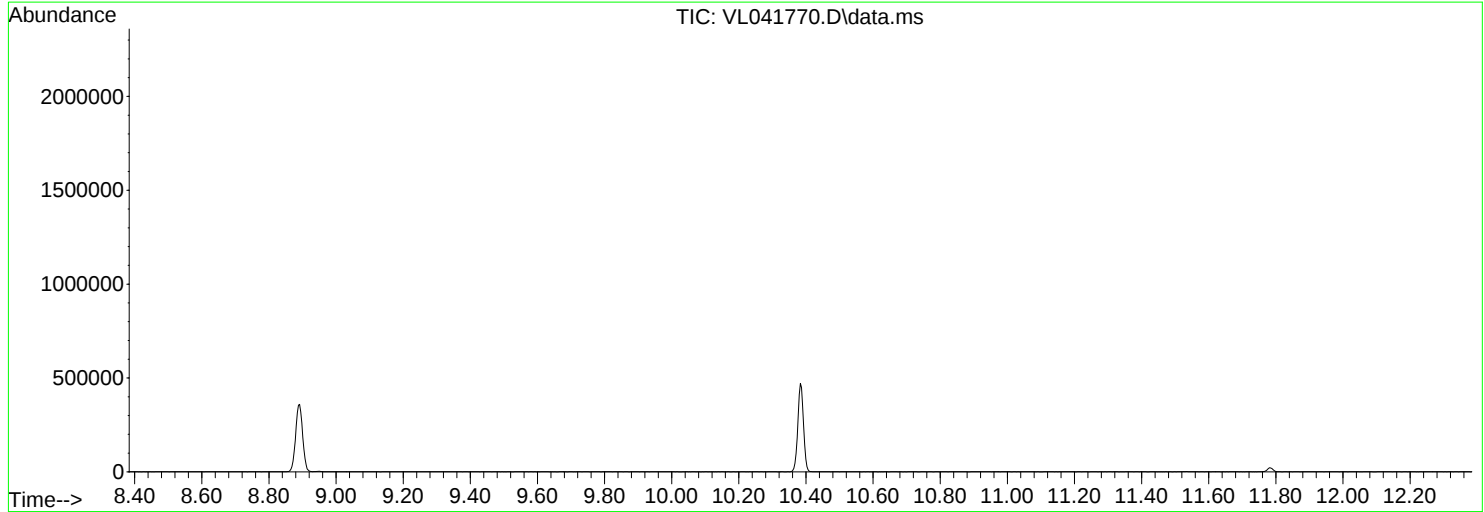

AutoFind: Scans 3180, 3181, 3182; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	27.8	24648	PASS
75	95	30	66	63.5	56309	PASS
95	95	100	100	100.0	88664	PASS
96	95	5	9	7.1	6255	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	58.4	51792	PASS
175	174	4	9	8.4	4336	PASS
176	174	93	101	97.7	50603	PASS
177	176	5	9	6.5	3270	PASS

Average of 10.380 to 10.387 min.: VL041770.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	1264	50.10	24648	62.05	5955	74.10	1913
37.05	6980	51.05	7162	63.10	4473	75.10	5630
38.05	5760	52.00	390	64.05	471	76.10	481
39.10	2328	52.90	45	64.95	272	77.15	54
41.95	34	55.05	398	66.90	196	77.90	123
44.05	522	56.10	2388	67.10	169	78.10	85
45.05	1291	57.10	3768	68.05	11682	78.95	4072
46.15	114	58.00	154	69.05	11842	79.95	1003
47.05	816	58.90	49	70.15	1176	81.00	3715
48.00	737	60.05	1038	72.05	743	81.95	931
49.10	5311	61.05	5919	73.05	4886	83.00	117

Average of 10.380 to 10.387 min.: VL041770.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.90	67	104.00	540	116.10	116	131.00	21
87.00	2615	104.85	194	116.90	733	134.90	138
88.05	2249	105.90	395	118.00	386	136.85	203
90.95	489	106.80	111	118.90	613	138.60	19
92.10	3349	107.00	19	123.50	24	139.05	41
93.05	4536	109.70	38	124.10	21	140.95	1038
94.10	12196	110.90	109	124.80	17	141.70	45
95.10	88664	112.70	36	127.90	328	143.05	1232
96.10	6255	113.00	57	128.95	186	144.95	128
97.10	213	114.95	162	129.95	420	145.80	19
102.80	56	115.80	324	130.75	50	146.00	70

Average of 10.380 to 10.387 min.: VL041770.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.05	71	160.90	30				
147.80	58	161.10	103				
148.05	149	171.65	148				
150.00	70	172.00	72				
153.20	38	172.20	132				
153.85	58	174.10	51792				
154.55	62	175.10	4336				
155.00	137	176.10	50603				
156.00	18	177.05	3270				
156.75	134	178.05	77				
158.95	112	280.00	29				

Instrument :

MSVOA_L

ClientSampleId :

BFB