

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121922\
 Data File : VL040038.D
 Acq On : 19 Dec 2022 21:30
 Operator : SY/MD
 Sample : N5971-06
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SS-3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2022
 Supervised By :Mahesh Dadoda 12/20/2022

Quant Time: Dec 20 05:16:16 2022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121922AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug

QLast Update : Tue Dec 20 04:50:21 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.169	49	1031267	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.632	114	2764287	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.446	117	2426145	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.758	95	1892231	10.210	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.100%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.710	85	47798	0.248	ppbv	97
3) Chlorodifluoromethane	2.658	51	56144m	0.369	ppbv	
4) Chloromethane	2.793	50	50418	0.529	ppbv #	84
6) Bromomethane	3.099	94	4248m	0.150	ppbv	
9) Propene	2.684	41	645615m	9.998	ppbv	
10) Heptane	7.555	43	215169	1.365	ppbv	99
11) Trichlorofluoromethane	3.539	101	36503m	0.174	ppbv	
13) Ethanol	3.227	45	10932615	1798.902	ppbv	91
15) Acetone	3.443	43	4427347	27.752	ppbv #	87
17) tert-Butyl alcohol	3.880	59	94113	0.598	ppbv #	72
19) Isopropyl Alcohol	3.568	45	344247	4.379	ppbv #	1
20) Methylene Chloride	3.912	84	465334	6.862	ppbv	99
26) Hexane	5.192	57	554111	4.772	ppbv #	41
27) Carbon Disulfide	4.102	76	671565	4.585	ppbv	99
30) Cyclohexane	6.581	84	339265	3.299	ppbv	94
34) 2-Butanone	4.768	43	149246	0.995	ppbv	96
35) Carbon Tetrachloride	6.475	117	8356m	0.049	ppbv	
36) Benzene	6.346	78	654389	2.651	ppbv	99
52) Tetrachloroethene	10.590	164	3367m	0.040	ppbv	
53) Toluene	9.198	91	1496513	5.475	ppbv	99
58) Ethyl Benzene	12.066	91	903848	2.622	ppbv	100
59) m/p-Xylene	12.323	91	813831	2.710	ppbv	97
60) o-Xylene	13.037	91	485290	1.687	ppbv	99
61) Styrene	12.877	104	107546	0.697	ppbv	98
62) Isopropylbenzene	14.008	105	148723	0.359	ppbv	100
64) n-propylbenzene	14.893	120	15262m	0.146	ppbv	
72) 4-Ethyltoluene	15.172	105	101243	0.317	ppbv #	96
73) 1,3,5-Trimethylbenzene	15.333	105	83645	0.290	ppbv	90
74) 1,2,4-Trimethylbenzene	16.085	105	127424	0.401	ppbv #	63

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121922\
Data File : VL040038.D
Acq On : 19 Dec 2022 21:30
Operator : SY/MD
Sample : N5971-06
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SS-3

Quant Time: Dec 20 05:16:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121922AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Tue Dec 20 04:50:21 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 12/20/2022
Supervised By : Mahesh Dadoda 12/20/2022

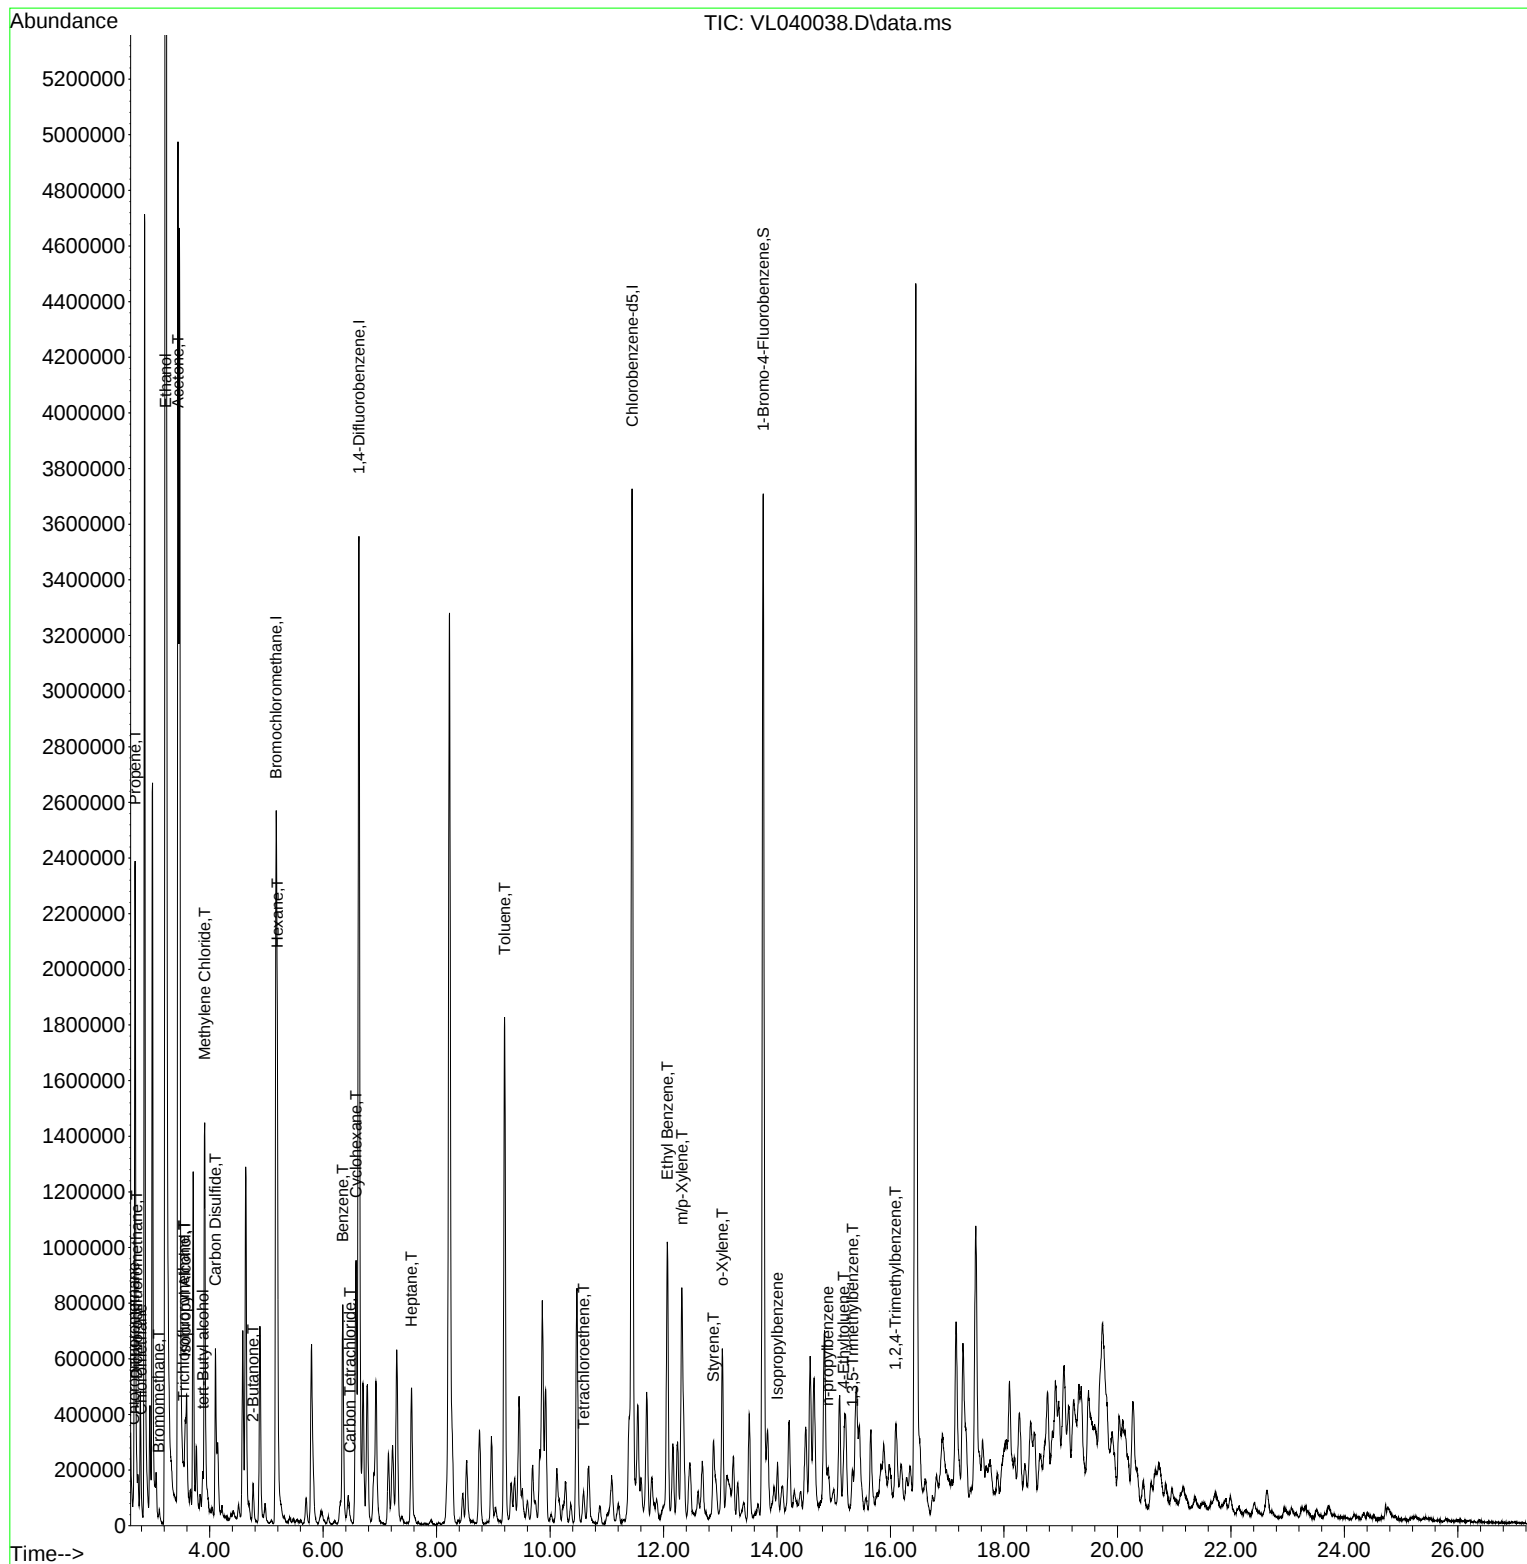

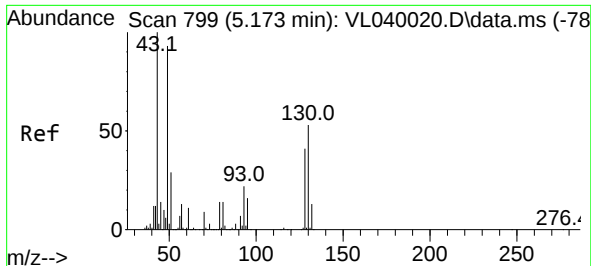

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.169 min Scan# 799
Delta R.T. -0.004 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30




Instrument :
MSVOA_L
ClientSampleId :
SS-3



Tgt Ion: 49 Resp: 103126
Ion Ratio Lower Upper
49 100
128 48.3 22.4 67.3
130 62.6 28.9 86.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

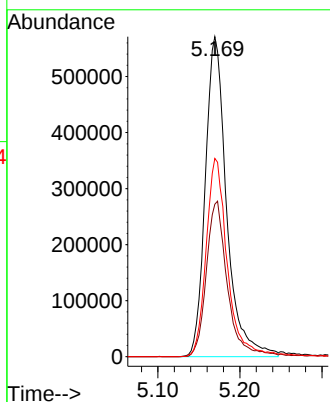

#2
Dichlorodifluoromethane
Concen: 0.248 ppbv
RT: 2.710 min Scan# 33
Delta R.T. 0.000 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30


Tgt Ion: 85 Resp: 47798
Ion Ratio Lower Upper
85 100
87 31.8 26.6 40.0

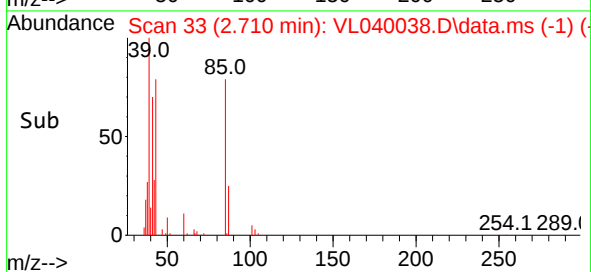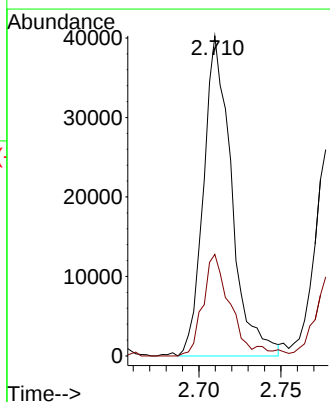

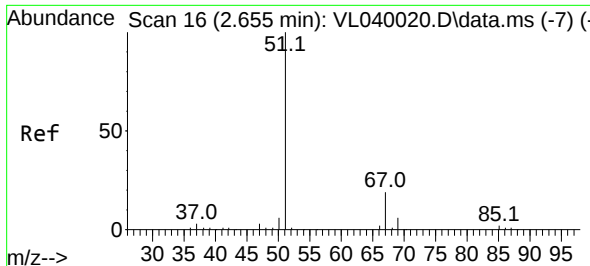

#3
Chlorodifluoromethane
Concen: 0.369 ppbv m
RT: 2.658 min Scan# 1
Delta R.T. 0.003 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30




Instrument :
MSVOA_L
ClientSampleId :
SS-3

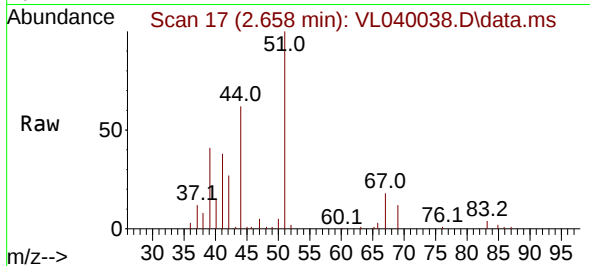

Tgt Ion: 51 Resp: 56144
Ion Ratio Lower Upper
51 100
67 17.3 15.3 22.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

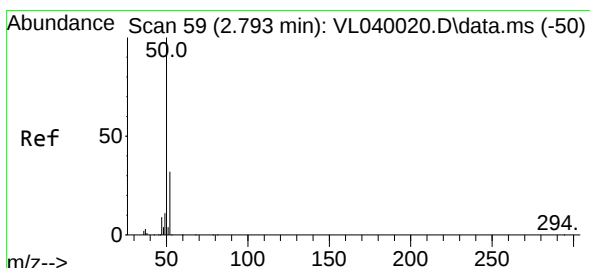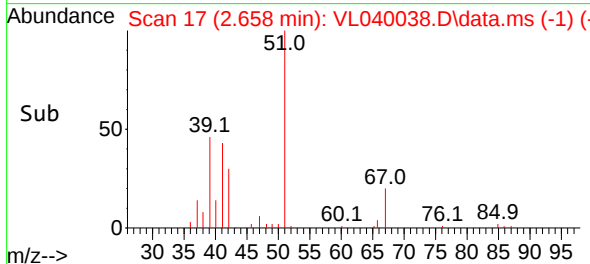

#4
Chloromethane
Concen: 0.529 ppbv
RT: 2.793 min Scan# 59
Delta R.T. 0.000 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30


Tgt Ion: 50 Resp: 50418
Ion Ratio Lower Upper
50 100
52 40.7 25.5 38.3#

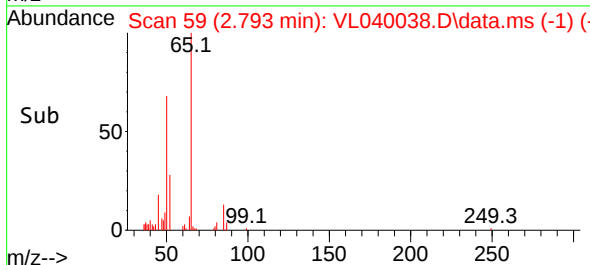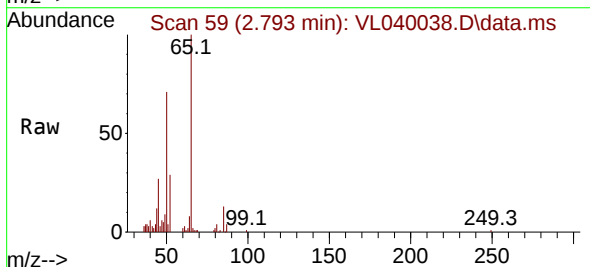



#6
Bromomethane
Concen: 0.150 ppbv m
RT: 3.099 min Scan# 11
Delta R.T. 0.000 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30




Instrument :
MSVOA_L
ClientSampleId :
SS-3

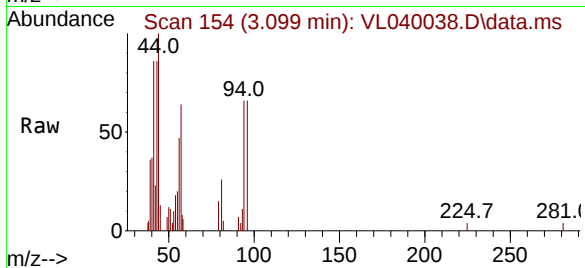

Tgt Ion: 94 Resp: 4248
Ion Ratio Lower Upper
94 100
96 100.4 72.0 108.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

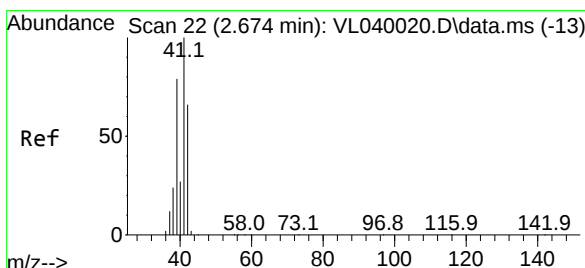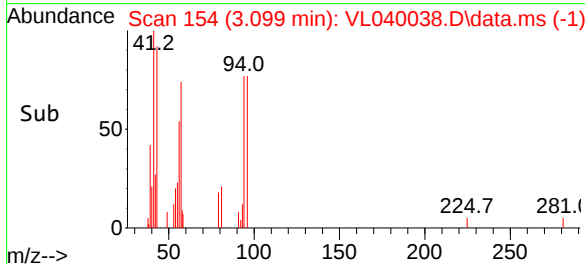

#9
Propene
Concen: 9.998 ppbv m
RT: 2.684 min Scan# 25
Delta R.T. 0.010 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30


Tgt Ion: 41 Resp: 645615
Ion Ratio Lower Upper
41 100
42 136.3 54.8 82.2#

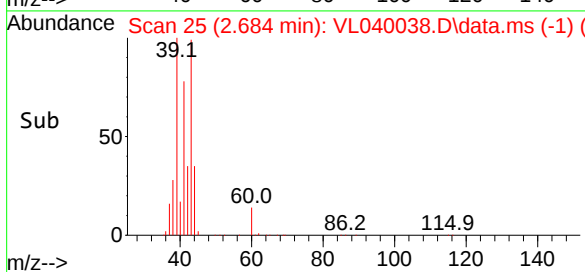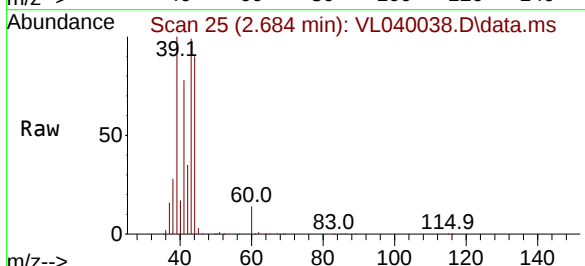



#10
Heptane
Concen: 1.365 ppbv
RT: 7.555 min Scan# 11
Delta R.T. -0.010 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30




Instrument :
MSVOA_L
ClientSampleId :
SS-3



Tgt Ion: 43 Resp: 215169
Ion Ratio Lower Upper
43 100
57 51.0 41.2 61.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

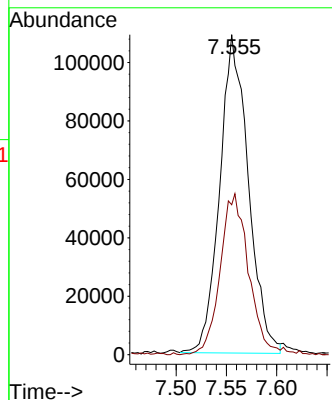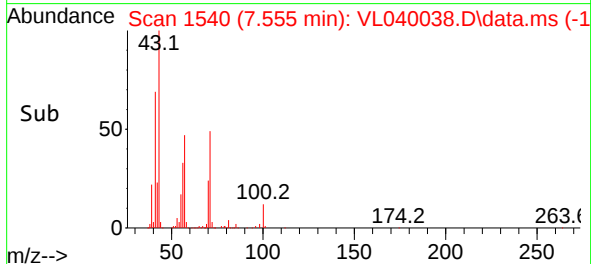

#11
Trichlorofluoromethane
Concen: 0.174 ppbv m
RT: 3.539 min Scan# 291
Delta R.T. -0.003 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30


Tgt Ion:101 Resp: 36503
Ion Ratio Lower Upper
101 100
103 49.8 51.7 77.5#

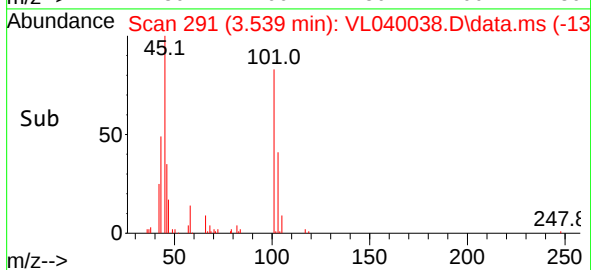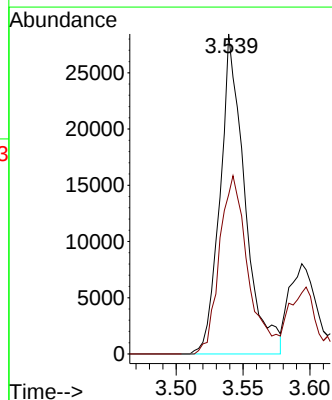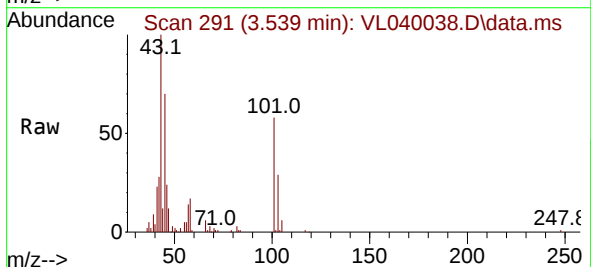



#13
Ethanol
Concen: 1798.902 ppbv
RT: 3.227 min Scan# 194
Delta R.T. 0.000 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30




Instrument :
MSVOA_L
ClientSampleId :
SS-3




Tgt Ion: 45 Resp: 1093261
Ion Ratio Lower Upper
45 100
46 39.5 13.7 54.7

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

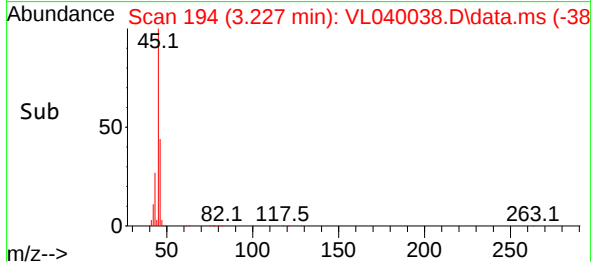


#15
Acetone
Concen: 27.752 ppbv
RT: 3.443 min Scan# 261
Delta R.T. -0.006 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30

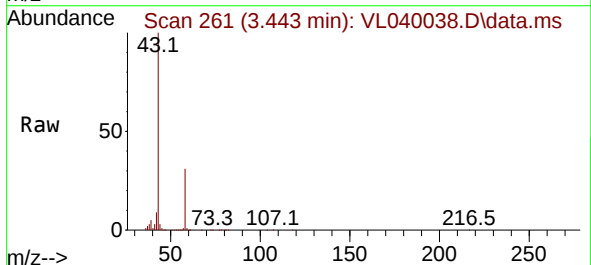

Tgt Ion: 43 Resp: 4427347
Ion Ratio Lower Upper
43 100
58 34.2 21.8 32.8#

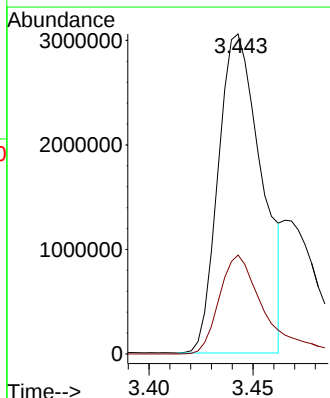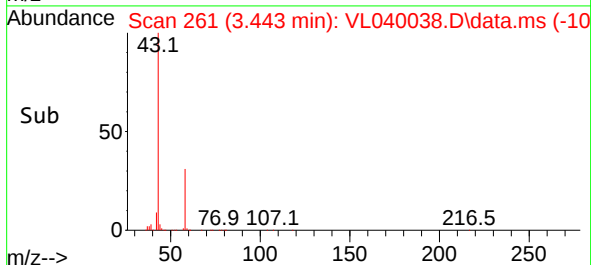







#17
tert-Butyl alcohol
Concen: 0.598 ppbv
RT: 3.880 min Scan# 390
Delta R.T. 0.023 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30

Instrument :
MSVOA_L
ClientSampleId :
SS-3

Tgt Ion: 59 Resp: 9411
Ion Ratio Lower Upper
59 100
57 0.0 8.4 12.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

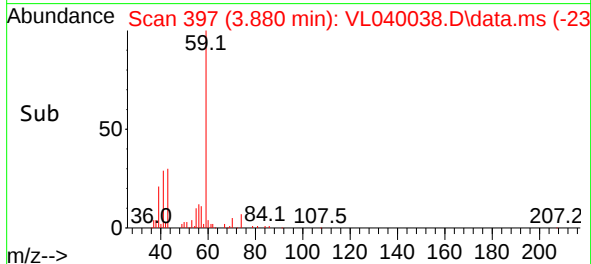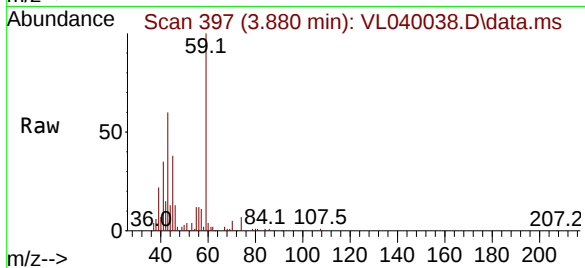

#19
Isopropyl Alcohol
Concen: 4.379 ppbv
RT: 3.568 min Scan# 300
Delta R.T. 0.013 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30


Tgt Ion: 45 Resp: 344247
Ion Ratio Lower Upper
45 100
58 439.4 1.7 2.5

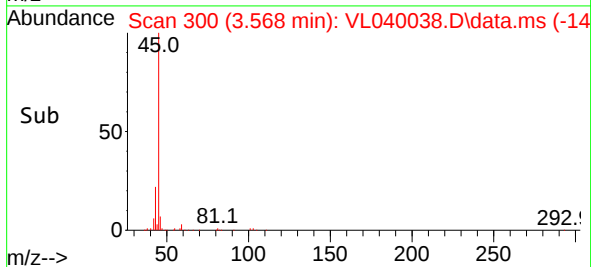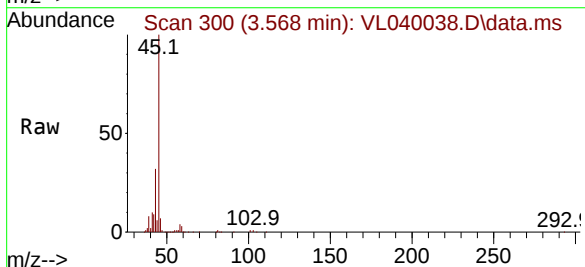



#20
Methylene Chloride
Concen: 6.862 ppbv
RT: 3.912 min Scan# 407
Delta R.T. -0.003 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30

Instrument :
MSVOA_L
ClientSampleId :
SS-3






Tgt Ion: 84 Resp: 465334

Ion	Ratio	Lower	Upper
84	100		
49	151.1	120.5	180.7
51	46.3	35.2	52.8
86	60.8	49.8	74.6

Manual Integrations
APPROVED




Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

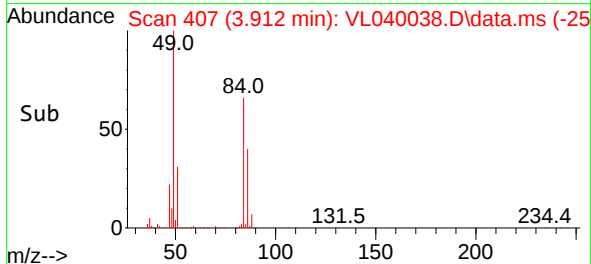


#26
Hexane
Concen: 4.772 ppbv
RT: 5.192 min Scan# 805
Delta R.T. -0.003 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30

Tgt Ion: 57 Resp: 554111


Ion	Ratio	Lower	Upper
57	100		
41	89.4	72.1	108.1
43	80.7	192.1	288.1#
56	55.2	42.5	63.7

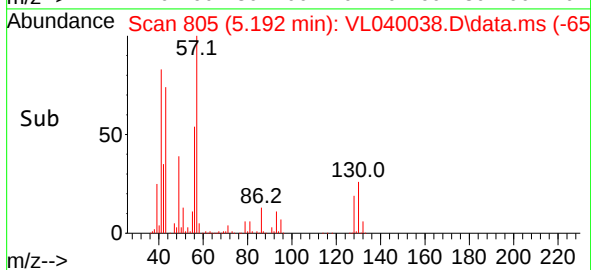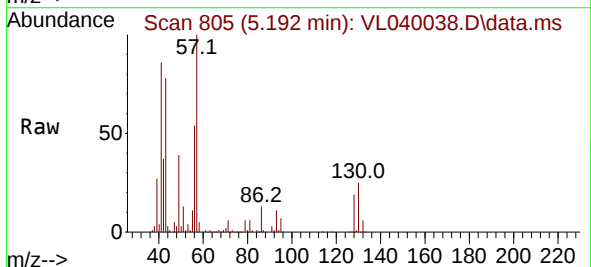



#27
Carbon Disulfide
Concen: 4.585 ppbv
RT: 4.102 min Scan# 41
Delta R.T. -0.003 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30




Instrument :
MSVOA_L
ClientSampleId :
SS-3

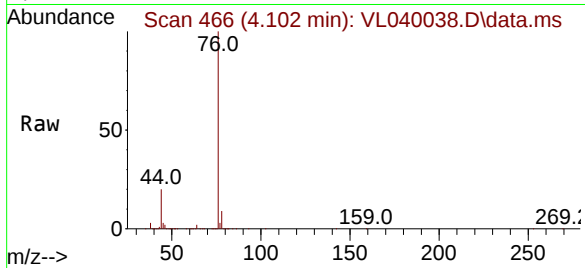


Tgt Ion: 76 Resp: 67156
Ion Ratio Lower Upper
76 100
44 19.7 15.3 22.9
78 9.4 7.8 11.6

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

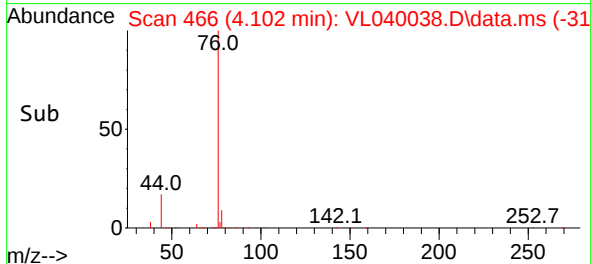


#30
Cyclohexane
Concen: 3.299 ppbv
RT: 6.581 min Scan# 1237
Delta R.T. -0.006 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30

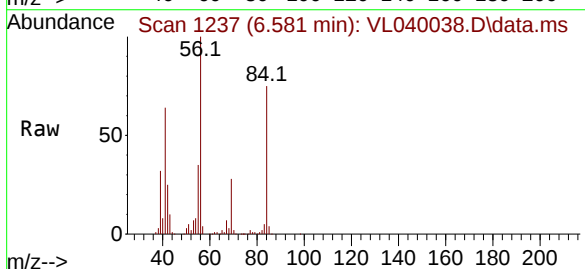

Tgt Ion: 84 Resp: 339265
Ion Ratio Lower Upper
84 100
56 148.3 110.2 165.4
41 86.1 67.8 101.8

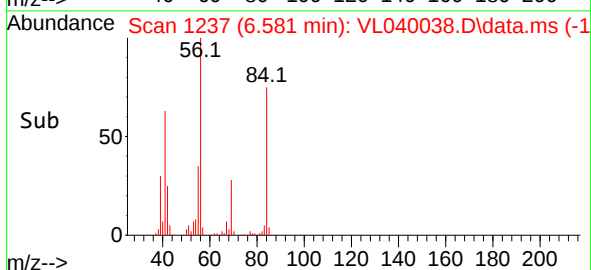



#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 6.632 min Scan# 114

Delta R.T. -0.003 min

Lab File: VL040038.D

Acq: 19 Dec 2022 21:30

Instrument :

MSVOA_L

ClientSampleId :

SS-3

Tgt Ion:114 Resp: 276428

Ion Ratio Lower Upper

114 100

63 24.8 20.2 30.2





88 17.7 14.6 21.8

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2022

Supervised By :Mahesh Dadoda 12/20/2022

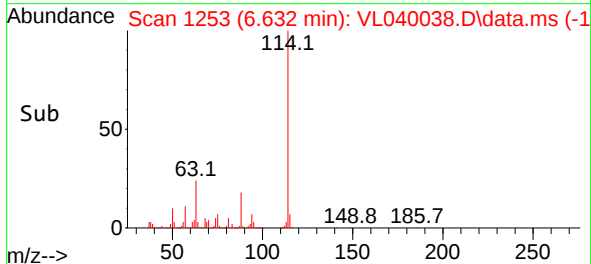

#34

2-Butanone

Concen: 0.995 ppbv

RT: 4.768 min Scan# 673

Delta R.T. 0.000 min

Lab File: VL040038.D




Acq: 19 Dec 2022 21:30


Tgt Ion: 43 Resp: 149246

Ion Ratio Lower Upper

43 100


72 24.6 18.0 27.0

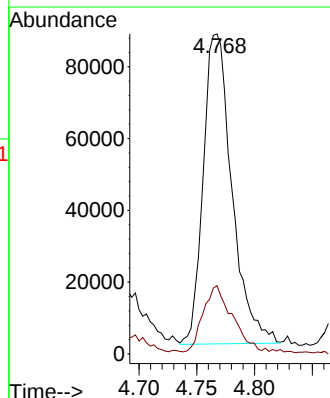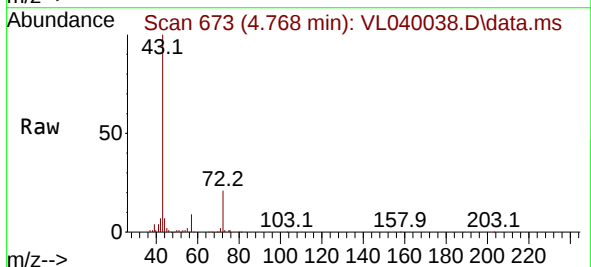



#35
Carbon Tetrachloride
Concen: 0.049 ppbv m
RT: 6.475 min Scan# 1164
Delta R.T. -0.003 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30




Instrument :
MSVOA_L
ClientSampleId :
SS-3



Tgt Ion:117 Resp: 8350
Ion Ratio Lower Upper
117 100
119 62.6 77.3 115.9
121 23.6 25.4 38.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

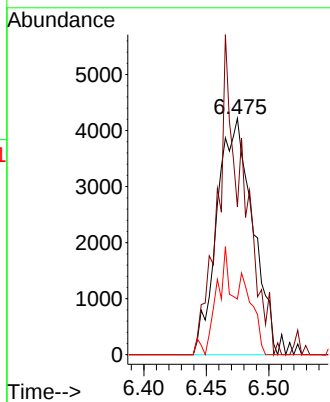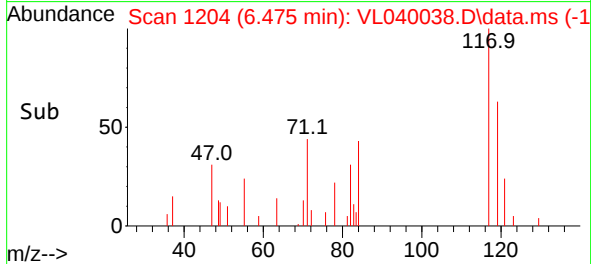

#36
Benzene
Concen: 2.651 ppbv
RT: 6.346 min Scan# 1164
Delta R.T. -0.006 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30


Tgt Ion: 78 Resp: 654389
Ion Ratio Lower Upper
78 100
77 21.5 17.5 26.3
50 18.5 14.2 21.2

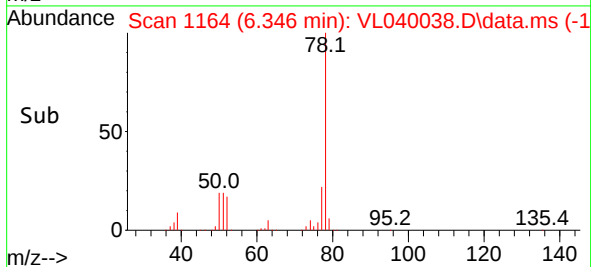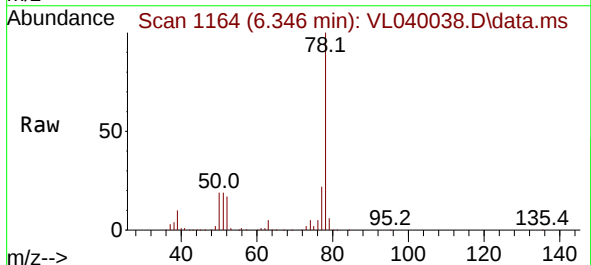



#52
Tetrachloroethene
Concen: 0.040 ppbv m
RT: 10.590 min Scan# 2488
Delta R.T. -0.013 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30




Instrument : MSVOA_L
ClientSampleId : SS-3

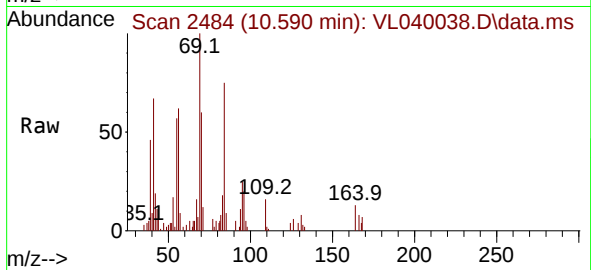

Tgt Ion:164 Resp: 336
Ion Ratio Lower Upper
164 100
166 61.3 97.4 146.0
129 29.3 84.3 126.5
131 61.0 85.8 128.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

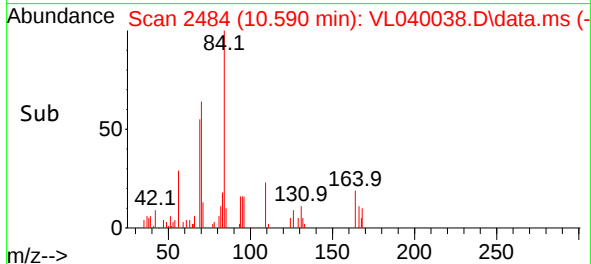

#53
Toluene
Concen: 5.475 ppbv
RT: 9.198 min Scan# 2051
Delta R.T. -0.006 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30


Tgt Ion: 91 Resp: 1496513
Ion Ratio Lower Upper
91 100
92 60.3 48.7 73.1

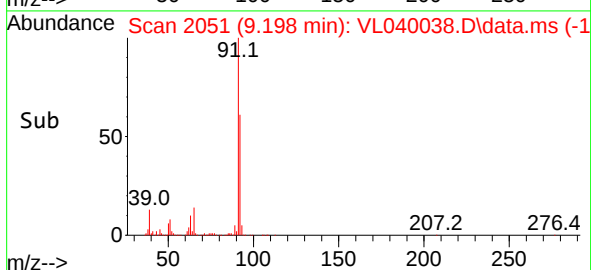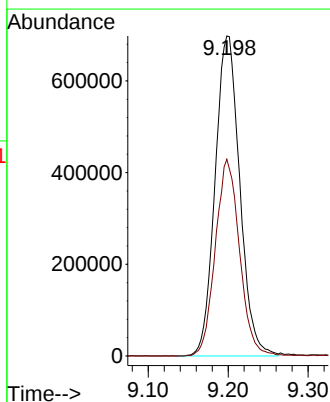



#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.446 min Scan# 21
Delta R.T. -0.006 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30




Instrument :
MSVOA_L
ClientSampleId :
SS-3

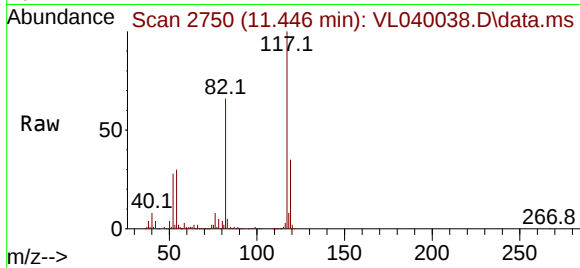

Tgt Ion:117 Resp: 242614
Ion Ratio Lower Upper
117 100
82 64.9 51.2 76.8
119 32.9 23.2 34.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

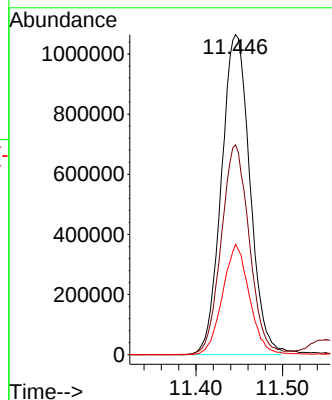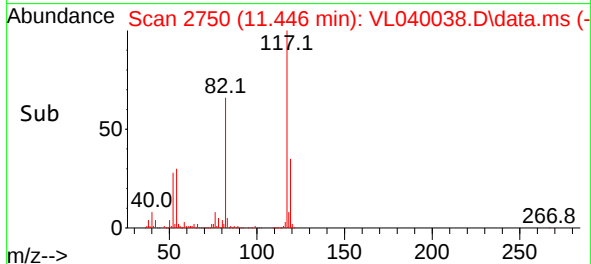

#58
Ethyl Benzene
Concen: 2.622 ppbv
RT: 12.066 min Scan# 2943
Delta R.T. -0.010 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30

Tgt Ion: 91 Resp: 903848
Ion Ratio Lower Upper
91 100
106 29.3 23.5 35.3

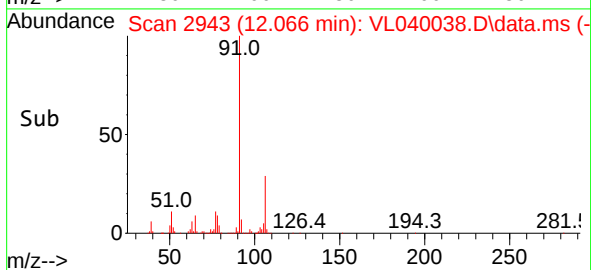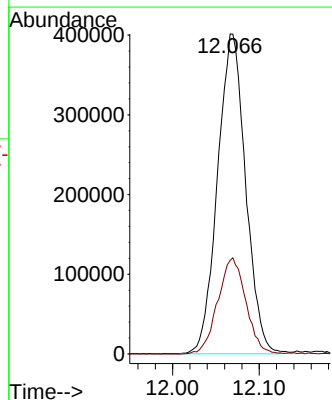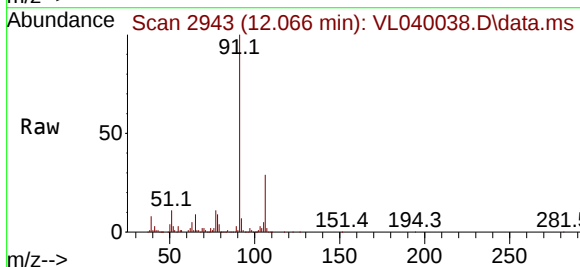







#59
m/p-Xylene
Concen: 2.710 ppbv
RT: 12.323 min Scan# 3035
Delta R.T. -0.038 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30

Instrument :
MSVOA_L
ClientSampleId :
SS-3

Tgt Ion: 91 Resp: 81383
Ion Ratio Lower Upper
91 100
106 46.2 35.5 53.3




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

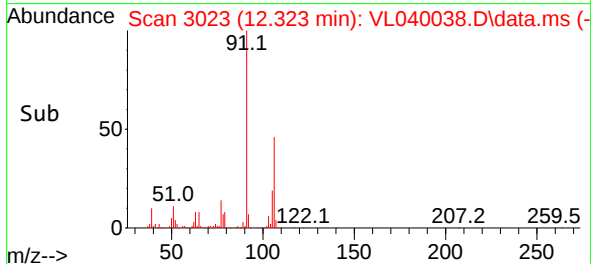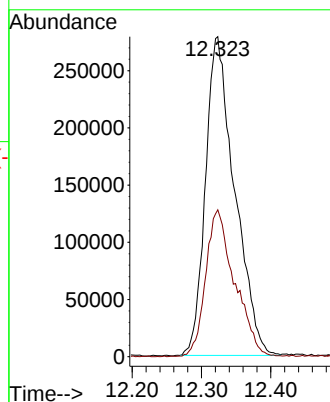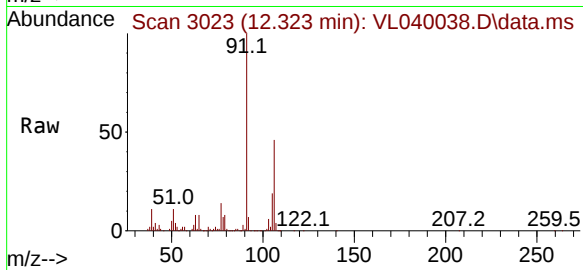

#60
o-Xylene
Concen: 1.687 ppbv
RT: 13.037 min Scan# 3245
Delta R.T. -0.010 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30


Tgt Ion: 91 Resp: 485290
Ion Ratio Lower Upper
91 100
106 43.8 22.4 67.0

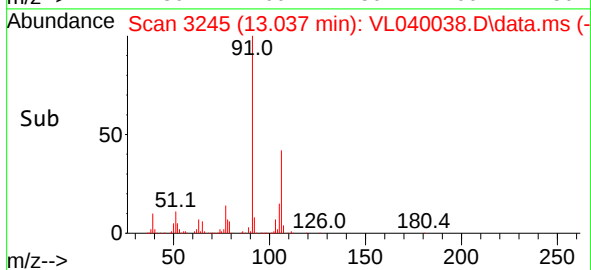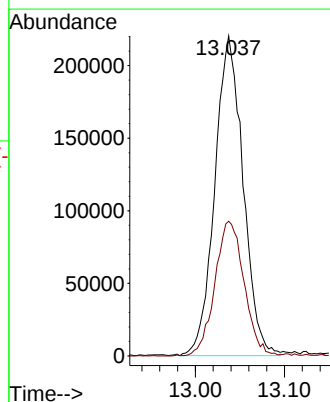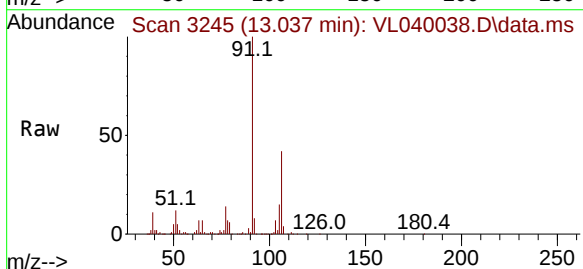

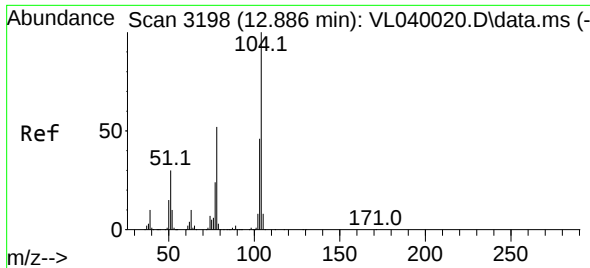

#61
Styrene
Concen: 0.697 ppbv
RT: 12.877 min Scan# 3195
Delta R.T. -0.010 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30




Instrument :
MSVOA_L
ClientSampleId :
SS-3

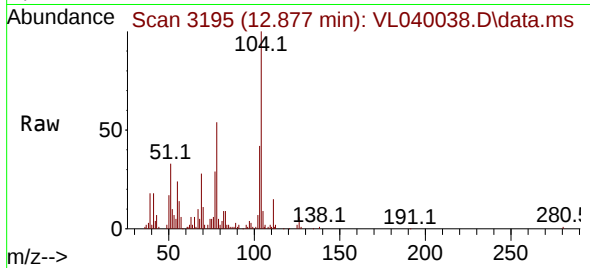

Tgt Ion:104 Resp: 107540
Ion Ratio Lower Upper
104 100
78 54.0 42.4 63.6
103 48.3 37.2 55.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

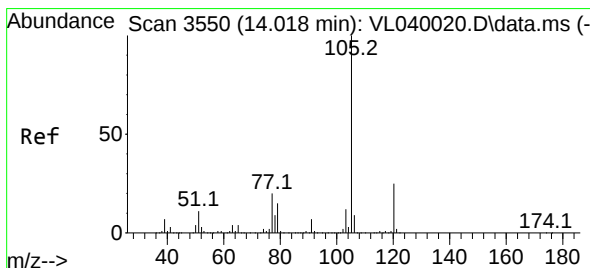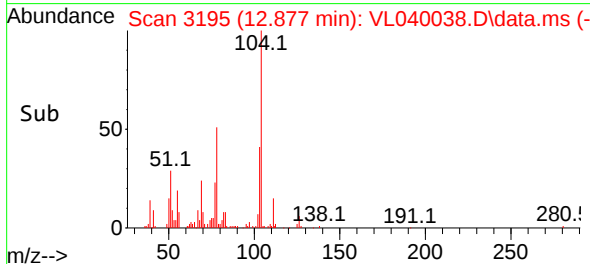

#62
Isopropylbenzene
Concen: 0.359 ppbv
RT: 14.008 min Scan# 3547
Delta R.T. -0.010 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30

Tgt Ion:105 Resp: 148723
Ion Ratio Lower Upper
105 100
120 25.7 20.6 31.0

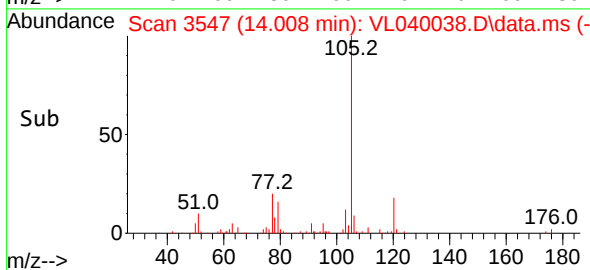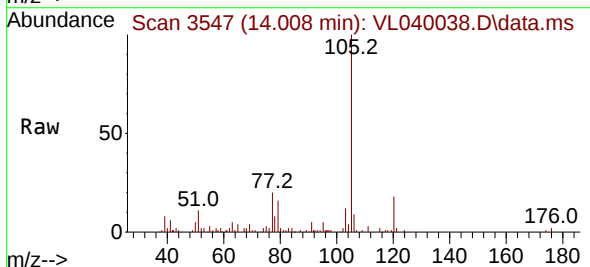

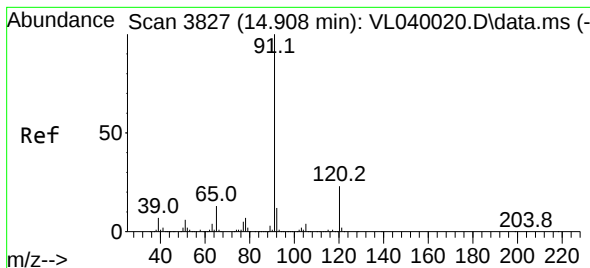





#64
n-propylbenzene
Concen: 0.146 ppbv m
RT: 14.893 min Scan# 3822
Delta R.T. -0.016 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30

Instrument :
MSVOA_L
ClientSampleId :
SS-3

Tgt Ion: 120 Resp: 1526
Ion Ratio Lower Upper
120 100
91 505.5 384.3 576.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

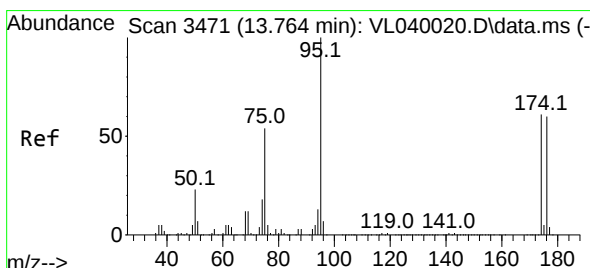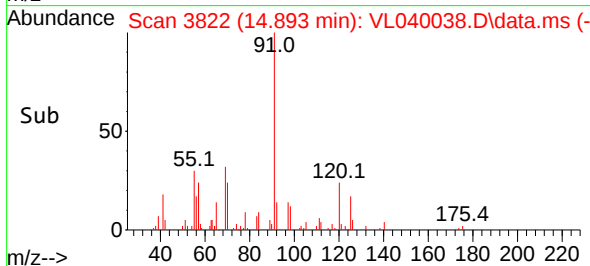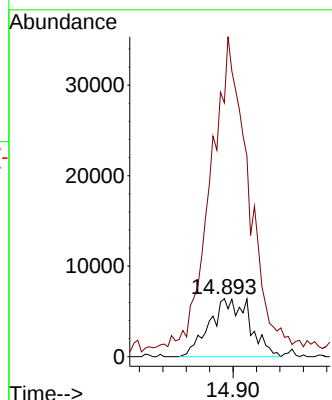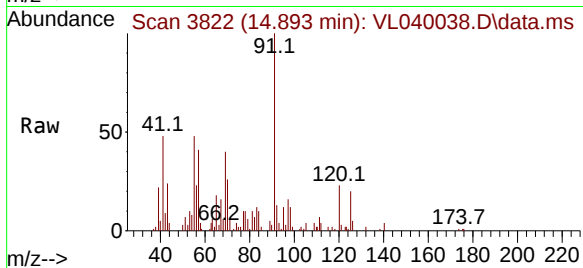

#68
1-Bromo-4-Fluorobenzene
Concen: 10.210 ppbv
RT: 13.758 min Scan# 3469
Delta R.T. -0.006 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30


Tgt Ion: 95 Resp: 1892231
Ion Ratio Lower Upper
95 100
174 60.4 48.6 73.0
175 4.4 3.4 5.2

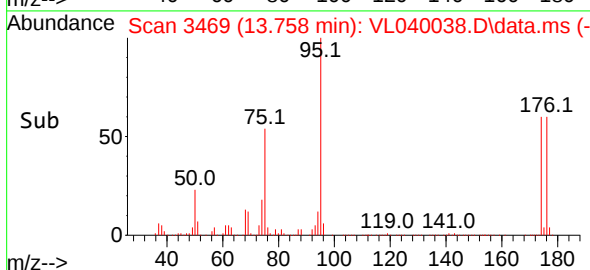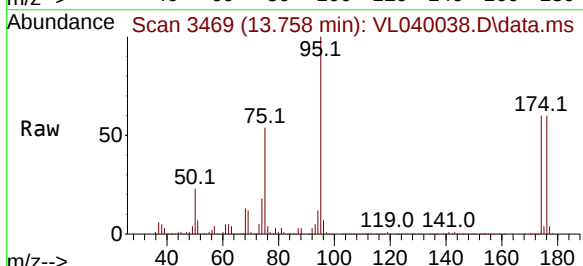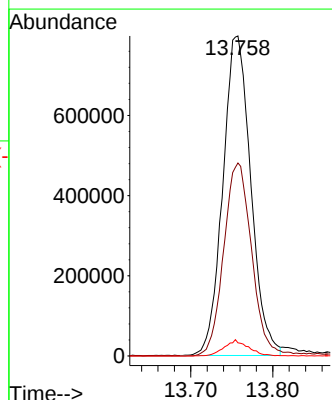

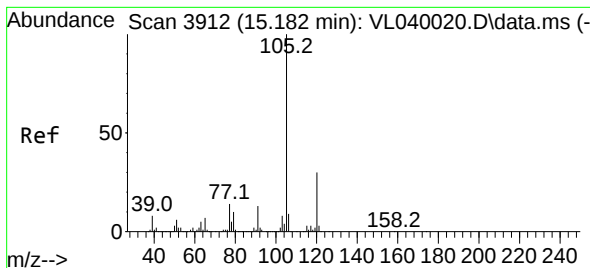

#72
4-Ethyltoluene
Concen: 0.317 ppbv
RT: 15.172 min Scan# 3909
Delta R.T. -0.010 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30




Instrument :
MSVOA_L
ClientSampleId :
SS-3

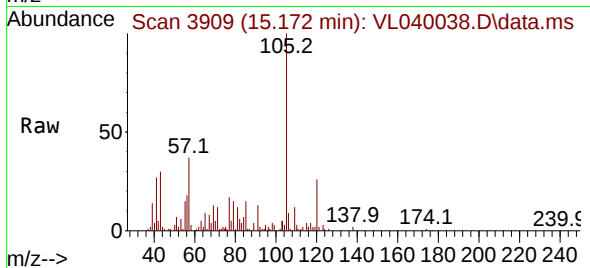


Tgt Ion:105 Resp: 10124
Ion Ratio Lower Upper
105 100
120 29.2 23.5 35.3
91 16.2 10.5 15.7
77 18.0 11.5 17.3#

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 12/20/2022
Supervised By :Mahesh Dadoda 12/20/2022

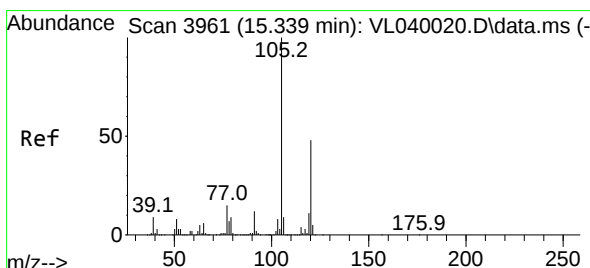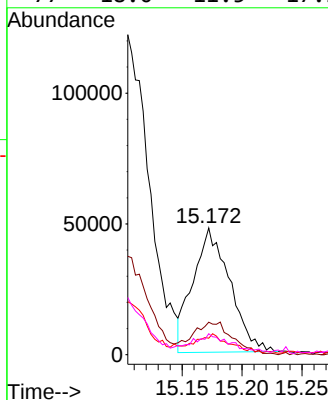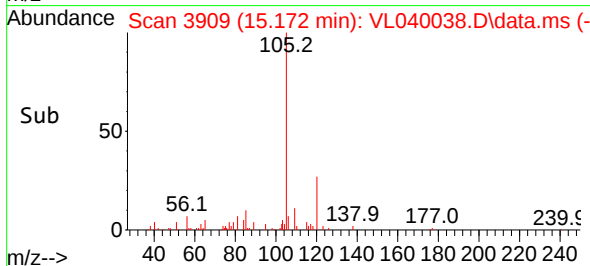


#73
1,3,5-Trimethylbenzene
Concen: 0.290 ppbv
RT: 15.333 min Scan# 3959
Delta R.T. -0.006 min
Lab File: VL040038.D
Acq: 19 Dec 2022 21:30

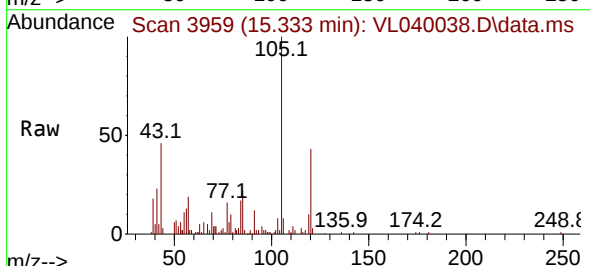


Tgt Ion:105 Resp: 83645
Ion Ratio Lower Upper
105 100
120 41.6 38.4 57.6

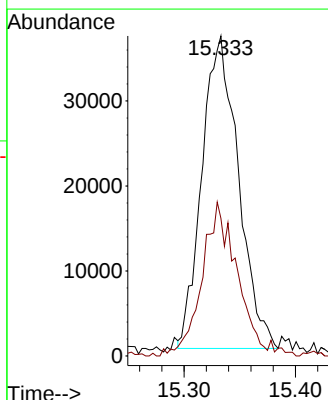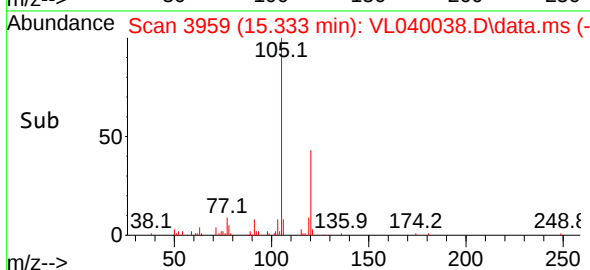



#74
 1,2,4-Trimethylbenzene
 Concen: 0.401 ppbv
 RT: 16.085 min Scan# 4193
 Delta R.T. -0.010 min
 Lab File: VL040038.D
 Acq: 19 Dec 2022 21:30

Instrument :
 MSVOA_L
 ClientSampleId :
 SS-3

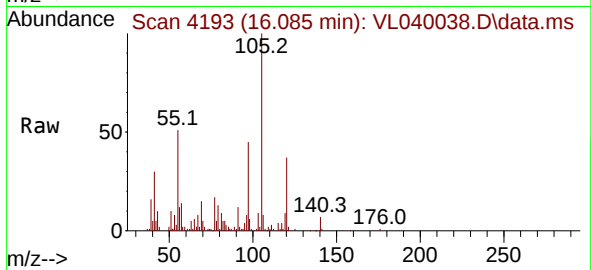

Tgt Ion:105 Resp: 127424
 Ion Ratio Lower Upper
 105 100
 120 36.8 39.3 58.9
 91 10.4 44.2 66.4
 77 15.9 18.8 28.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2022
 Supervised By :Mahesh Dadoda 12/20/2022

