

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121922\
 Data File : VL040047.D
 Acq On : 20 Dec 2022 3:20
 Operator : SY/MD
 Sample : VIBLK
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VIBLK

Quant Time: Dec 20 05:19:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121922AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Dec 20 04:50:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.166	49	999900	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.629	114	2809124	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.446	117	2425348	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.754	95	1806363	9.750	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	97.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121922\
Data File : VL040047.D
Acq On : 20 Dec 2022 3:20
Operator : SY/MD
Sample : VIBLK
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Quant Time: Dec 20 05:19:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121922AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Dec 20 04:50:21 2022
Response via : Initial Calibration




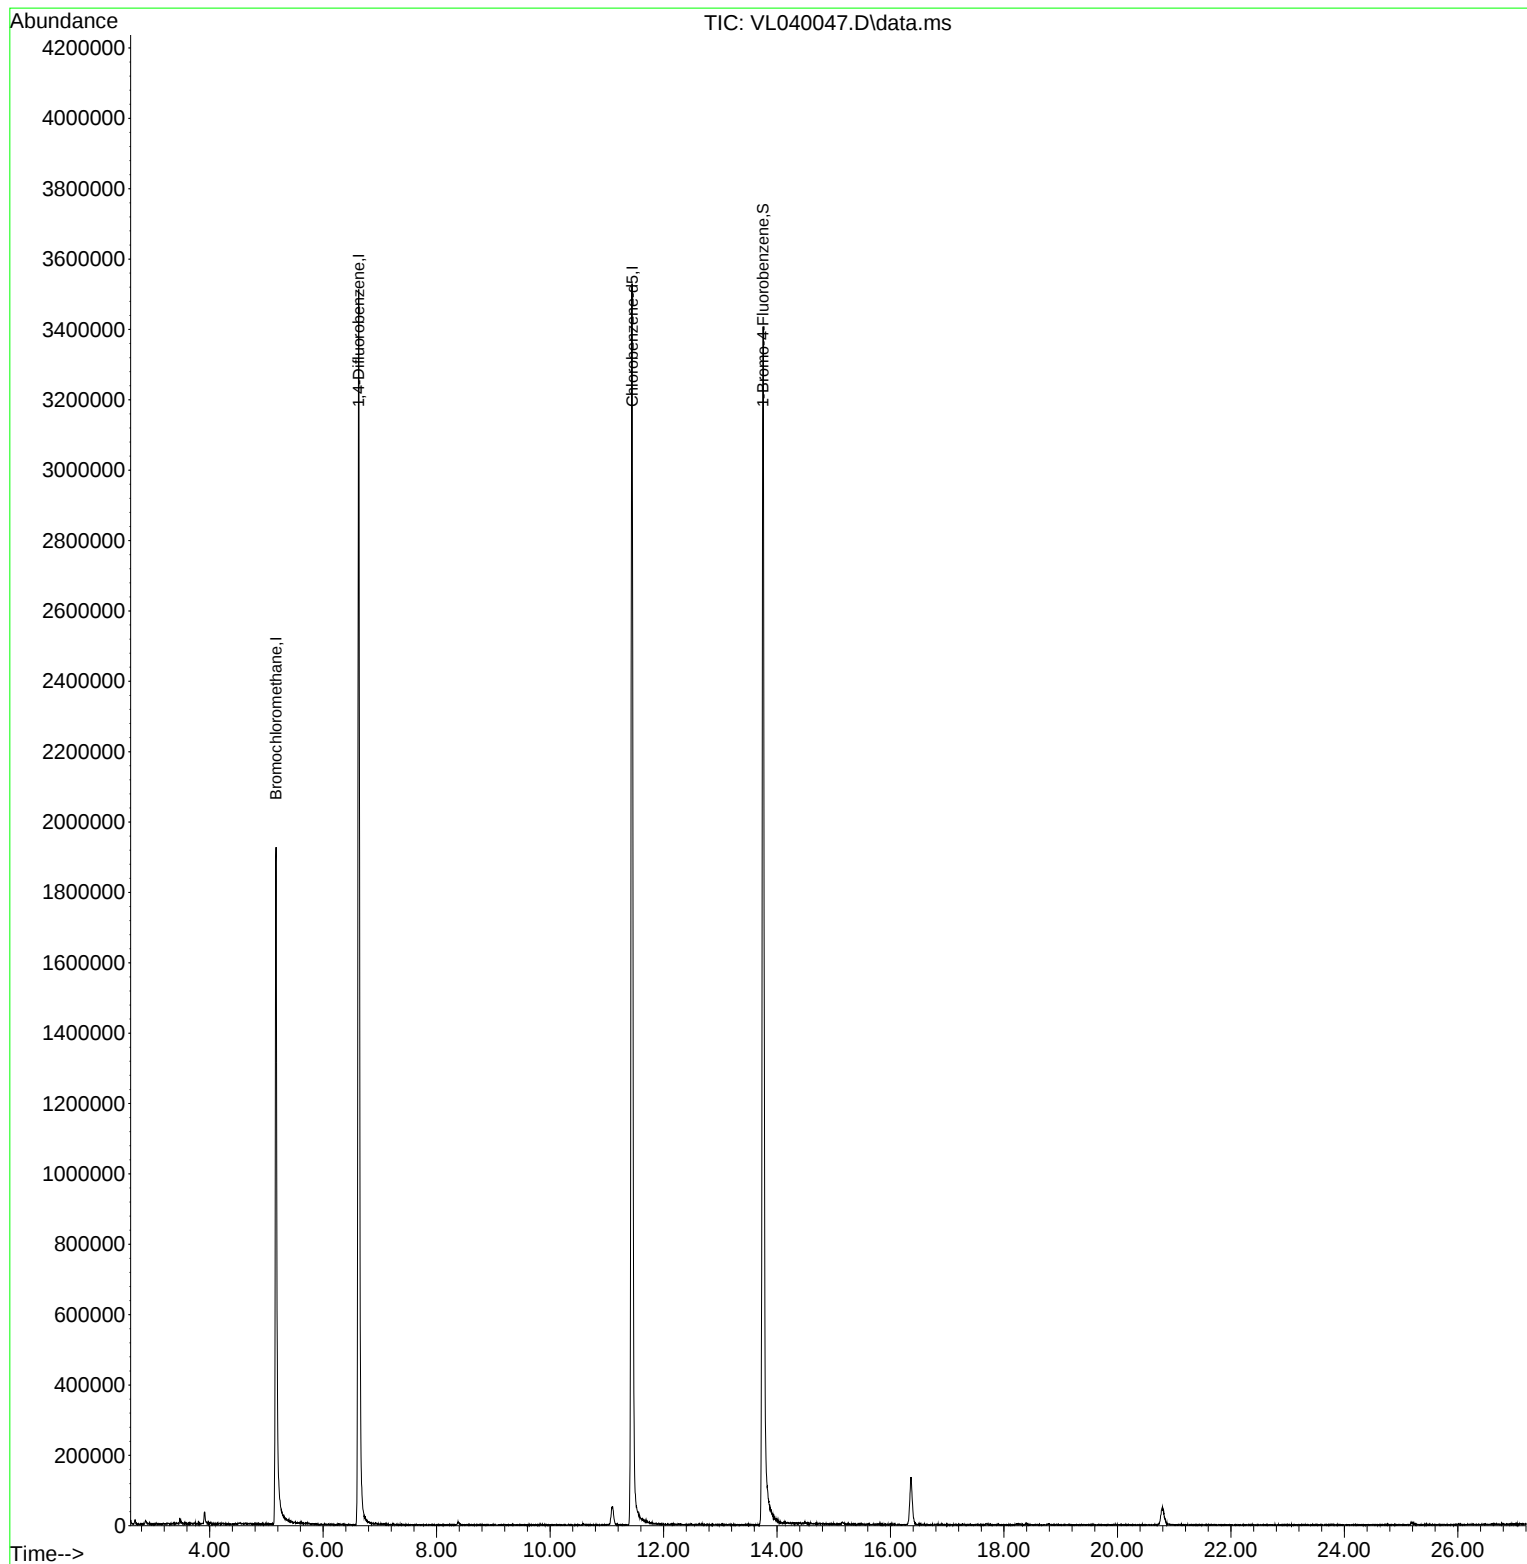


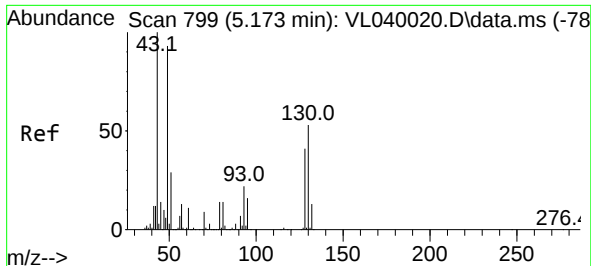

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.166 min Scan# 799
Delta R.T. -0.007 min
Lab File: VL040047.D
Acq: 20 Dec 2022 3:20




Instrument :
MSVOA_L
ClientSampleId :
VIBLK


Tgt Ion: 49 Resp: 999900
Ion Ratio Lower Upper
49 100
128 49.2 22.4 67.3
130 61.6 28.9 86.8

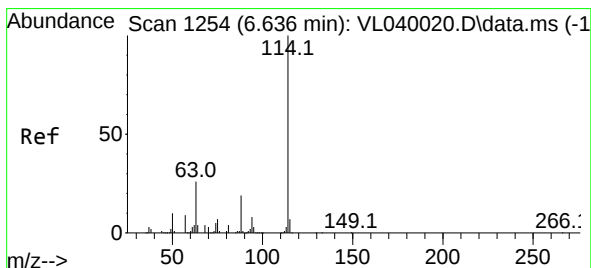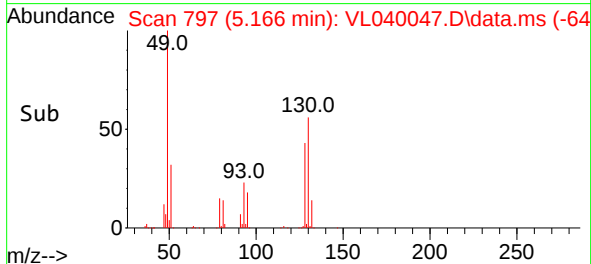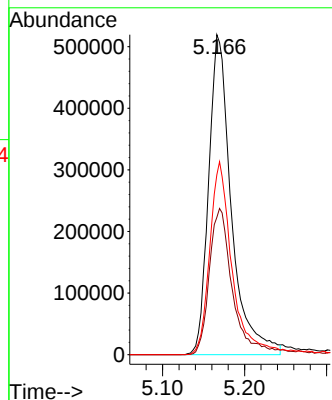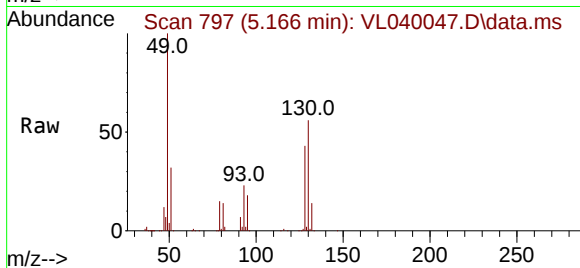

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.629 min Scan# 1252
Delta R.T. -0.006 min
Lab File: VL040047.D
Acq: 20 Dec 2022 3:20

Tgt Ion: 114 Resp: 2809124
Ion Ratio Lower Upper
114 100
63 24.6 20.2 30.2
88 18.2 14.6 21.8


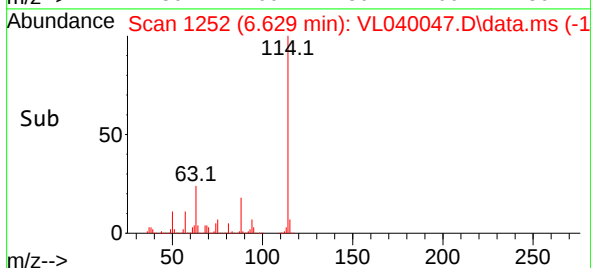
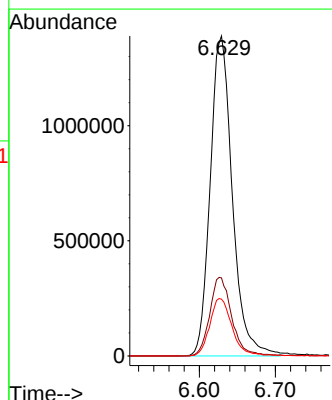
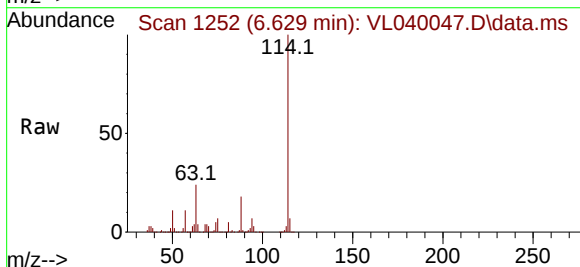


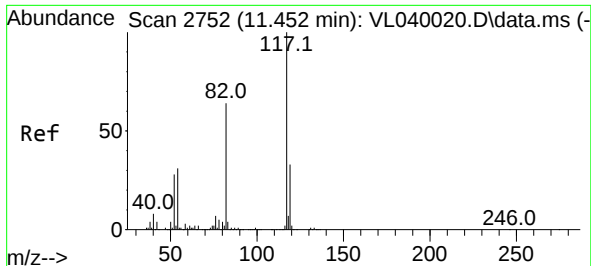

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.446 min Scan# 21
Delta R.T. -0.006 min
Lab File: VL040047.D
Acq: 20 Dec 2022 3:20

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 2425348
Ion Ratio Lower Upper
117 100
82 65.4 51.2 76.8
119 33.5 23.2 34.8

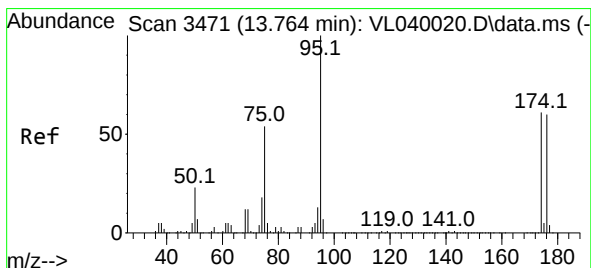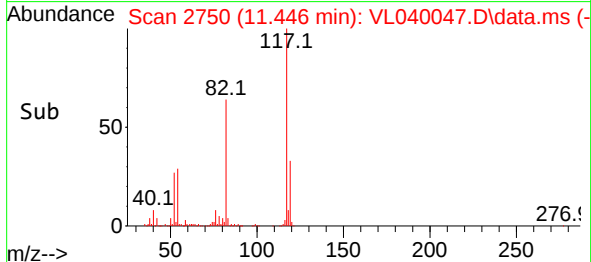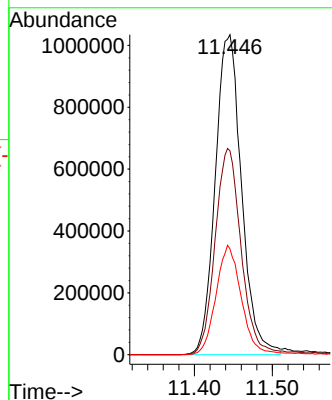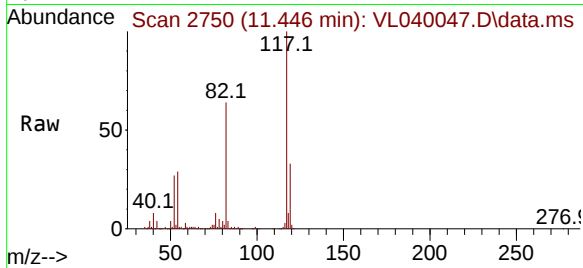

#68
1-Bromo-4-Fluorobenzene
Concen: 9.750 ppbv
RT: 13.754 min Scan# 3468
Delta R.T. -0.010 min
Lab File: VL040047.D
Acq: 20 Dec 2022 3:20

Tgt Ion: 95 Resp: 1806363
Ion Ratio Lower Upper
95 100
174 64.8 48.6 73.0
175 4.7 3.4 5.2

