
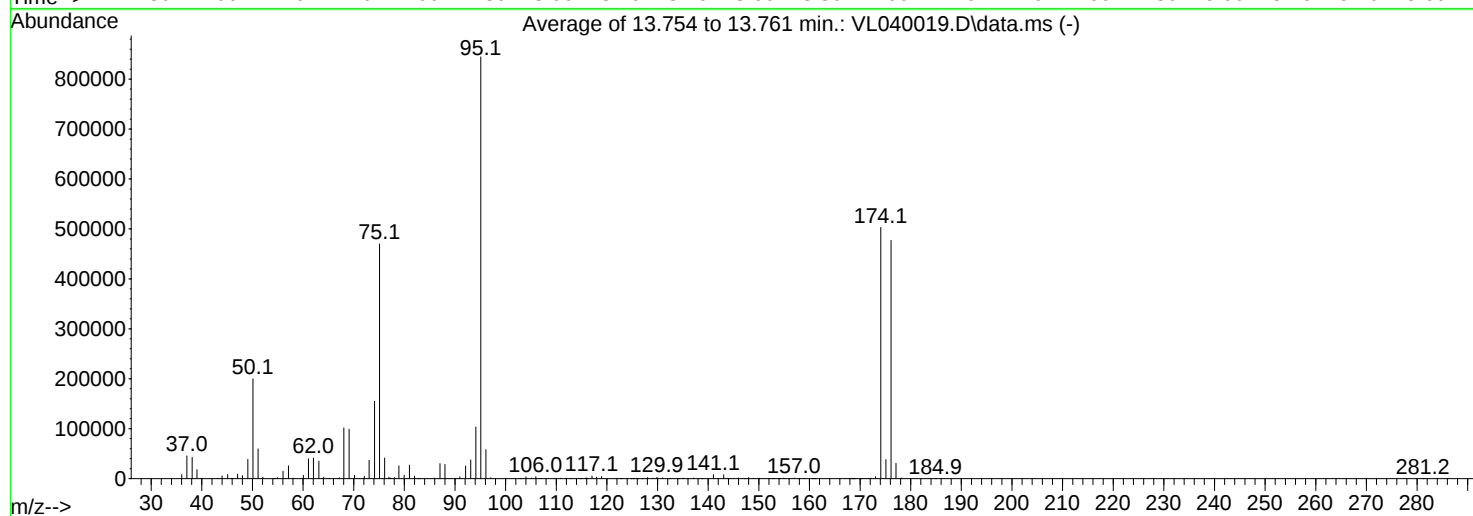


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121922\
 Data File : VL040019.D
 Acq On : 19 Dec 2022 8:57
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121922AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Dec 20 04:50:21 2022

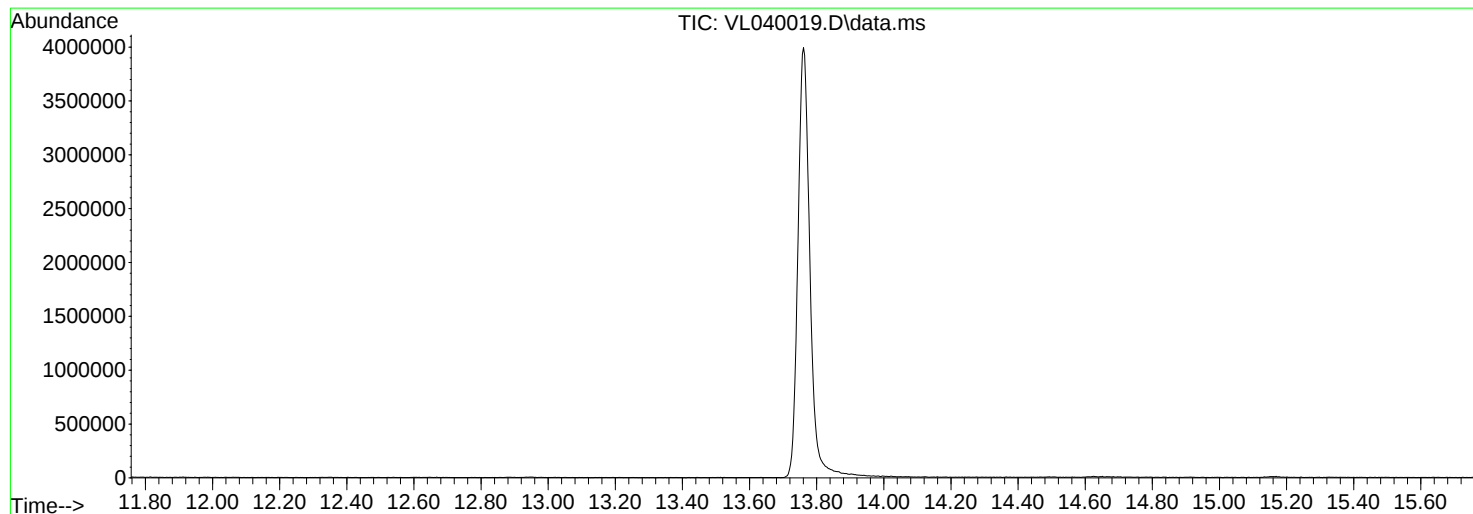

AutoFind: Scans 3468, 3469, 3470; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.7	200043	PASS
75	95	30	66	55.6	469995	PASS
95	95	100	100	100.0	844587	PASS
96	95	5	9	6.9	58061	PASS
173	174	0.00	2	0.8	3904	PASS
174	95	50	120	59.5	502933	PASS
175	174	4	9	7.6	38043	PASS
176	174	93	101	94.9	477035	PASS
177	176	5	9	6.5	30883	PASS

Average of 13.754 to 13.761 min.: VL040019.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8181	46.25	696	58.10	1143	70.15	670
37.05	45576	47.05	8983	60.05	6813	71.05	43
38.10	42696	48.00	5997	61.05	39877	72.10	461
39.05	18024	49.10	38381	62.05	41061	73.05	3686
39.90	553	50.10	200043	63.10	35256	74.10	155179
40.10	292	51.10	59704	64.05	3042	75.10	469995
43.05	284	52.05	2704	65.15	699	76.10	41264
43.30	207	54.30	147	66.90	449	76.95	2981
44.00	5393	54.95	2086	67.15	1760	77.20	1219
45.10	8398	56.05	14873	68.05	101584	78.10	2219
45.90	162	57.10	25547	69.10	98960	78.90	25504

Instrument :

MSVOA_L

ClientSampleId :

BFB

Average of 13.754 to 13.761 min.: VL040019.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	7226	92.10	25347	106.80	238	117.05	4998
81.00	27117	93.10	37448	107.15	466	117.95	2822
82.00	5283	94.10	103494	109.70	507	118.95	4311
82.70	140	95.10	844587	110.90	938	121.80	221
83.20	441	96.10	58061	111.85	370	122.70	70
85.90	1205	97.10	1995	112.80	305	123.00	224
87.05	30032	102.80	337	113.05	709	124.05	392
88.00	28496	103.00	127	114.70	110	124.80	53
88.80	441	104.00	3401	115.05	582	125.20	63
90.00	62	105.10	1444	115.90	1560	125.90	257
90.95	3417	105.95	3799	116.10	890	126.10	85

Average of 13.754 to 13.761 min.: VL040019.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.90	134	137.10	1201	146.00	1248	153.85	183
127.10	359	138.70	60	146.75	453	154.10	173
128.05	2399	139.10	235	147.20	97	154.90	998
129.05	1024	140.10	357	148.00	1927	155.10	423
129.90	2668	141.05	8062	148.90	524	155.90	56
131.00	1569	141.90	714	149.85	344	157.00	1391
132.30	72	142.10	247	150.15	578	157.90	92
134.20	164	143.05	7755	151.00	228	158.90	542
135.00	843	143.90	599	152.00	299	159.10	385
135.20	514	144.10	94	152.70	93	160.60	86
135.85	144	145.00	823	153.10	353	160.85	606

Average of 13.754 to 13.761 min.: VL040019.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
161.10	80	171.20	335	281.20	56		
167.15	200	171.70	691				
167.85	195	172.10	1051				
168.30	94	172.30	338				
168.60	159	173.05	3904				
168.80	126	174.10	502933				
169.20	593	175.10	38043				
170.00	93	176.10	477035				
170.10	100	177.10	30883				
170.25	259	178.15	1192				
170.75	348	184.90	69				