


Data Path : W:\HPCHEM1\MSVOA L\Data\VL122017\
 Data File : VL031263.D
 Acq On : 20 Dec 2017 8:57
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL121317AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Dec 14 04:29:58 2017
 Last Update : Thu Dec 14 04:29:58 2017

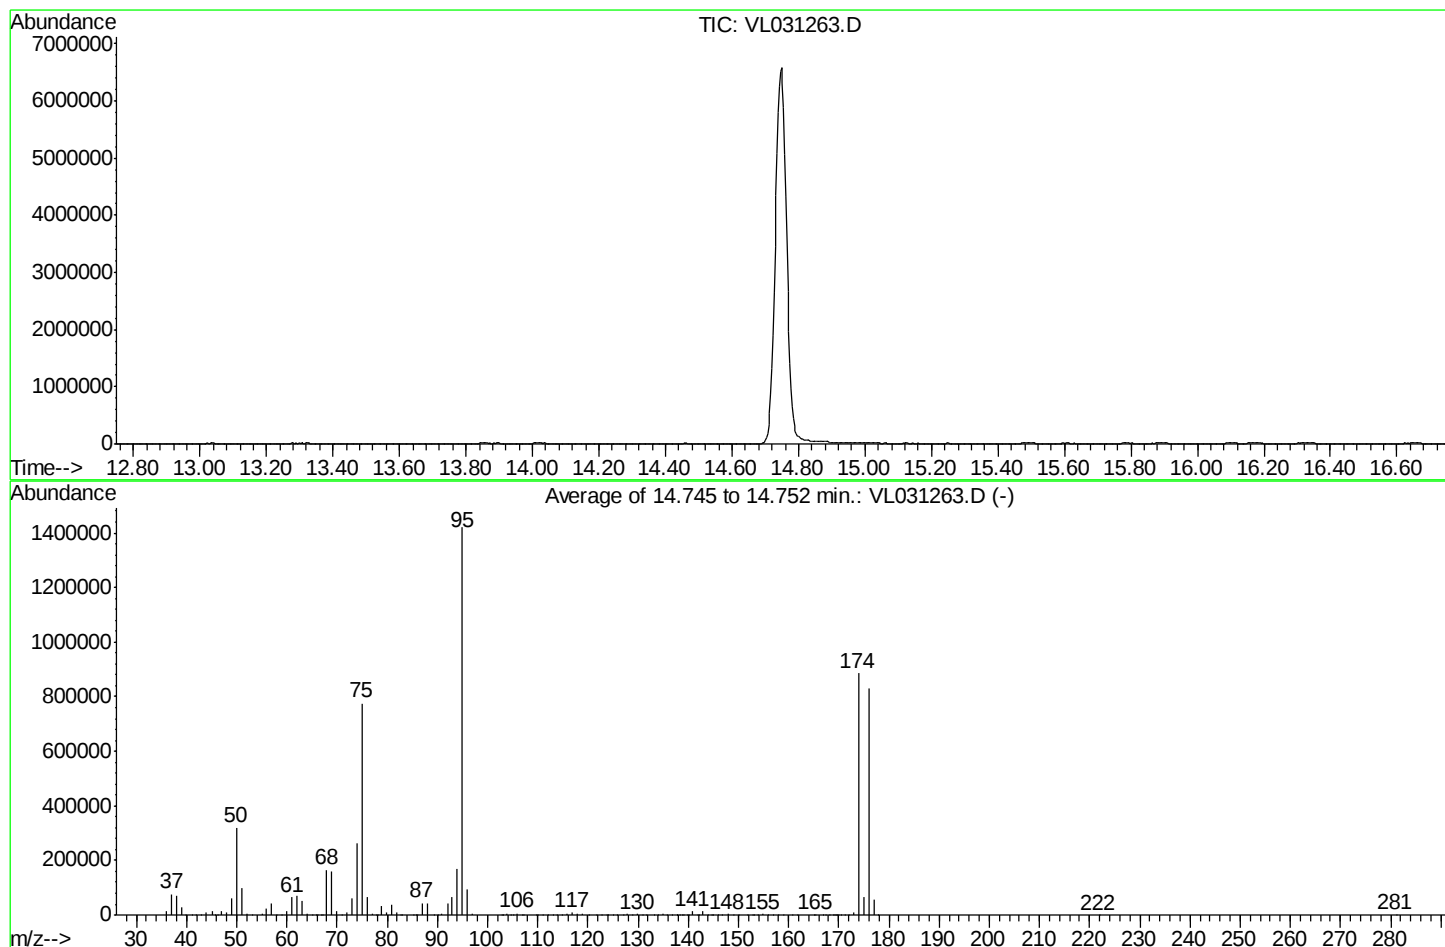

AutoFind: Scans 4248, 4249, 4250; Background Corrected with Scan 4221

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.5	319963	PASS
75	95	30	66	54.5	774122	PASS
95	95	100	100	100.0	1420458	PASS
96	95	5	9	6.7	95581	PASS
173	174	0.00	2	1.2	10320	PASS
174	95	50	120	62.3	885461	PASS
175	174	4	9	7.3	64664	PASS
176	174	93	101	93.7	829973	PASS
177	176	5	9	6.7	55381	PASS