
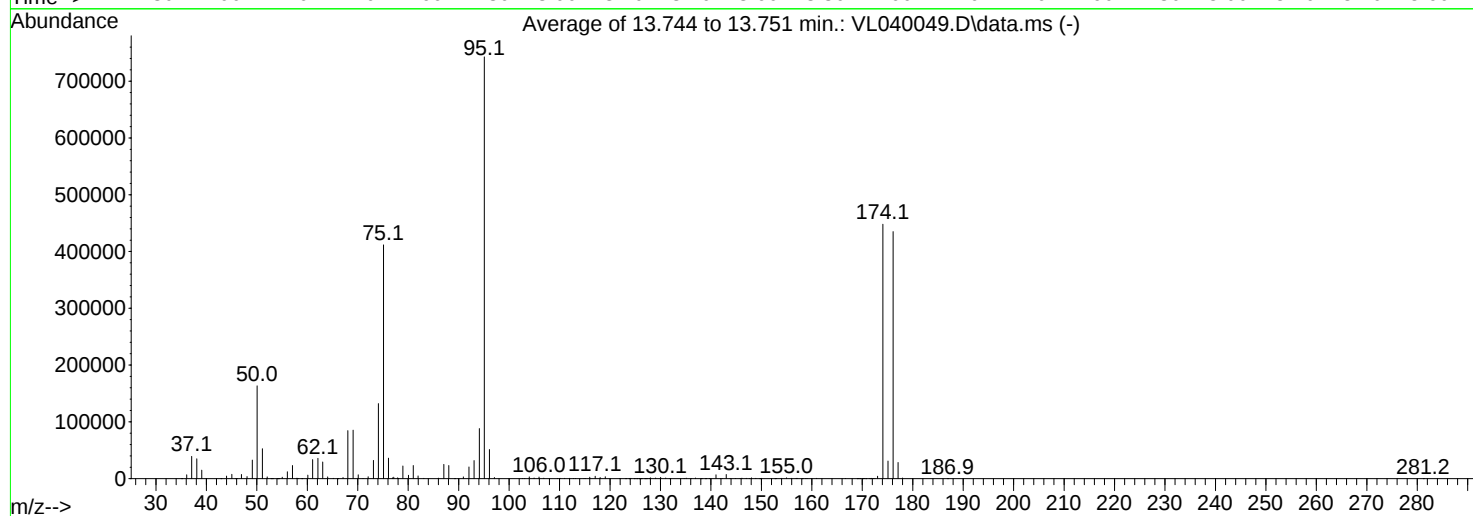


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL122022\
 Data File : VL040049.D
 Acq On : 20 Dec 2022 9:13
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121922AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Dec 20 04:50:21 2022

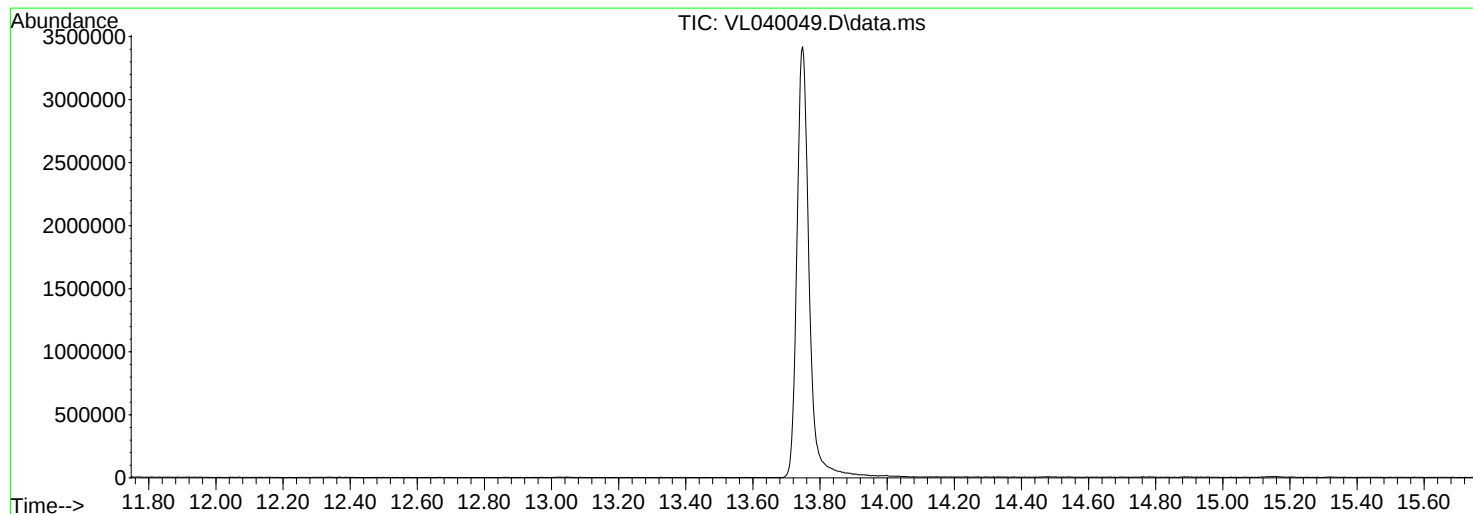

AutoFind: Scans 3465, 3466, 3467; Background Corrected with Scan 3438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.0	163563	PASS
75	95	30	66	55.4	411563	PASS
95	95	100	100	100.0	742827	PASS
96	95	5	9	6.9	51221	PASS
173	174	0.00	2	0.9	4251	PASS
174	95	50	120	60.3	448149	PASS
175	174	4	9	6.9	31104	PASS
176	174	93	101	97.1	435072	PASS
177	176	5	9	6.5	28453	PASS

Average of 13.744 to 13.751 min.: VL040049.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	58	46.95	7480	56.05	12196	66.00	10
36.10	6784	48.05	3774	57.05	23227	67.10	194
37.10	39323	49.10	32715	57.95	771	68.05	8443
38.10	35069	50.05	163563	58.20	428	69.10	8540
39.10	14901	51.10	52813	58.90	78	70.10	6757
40.00	294	52.05	3189	60.10	6183	71.05	307
42.90	131	52.80	53	61.05	33512	72.05	3503
44.00	4561	53.10	57	62.10	35712	73.10	32037
45.05	7668	54.10	143	63.05	29208	74.10	132144
45.80	109	54.30	59	64.05	3217	75.10	411563
46.10	342	55.05	2610	65.15	734	76.10	36011

Average of 13.744 to 13.751 min.: VL040049.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.90	1377	88.05	23125	104.00	3168	115.10	280
77.15	2468	89.20	59	104.95	1146	116.00	2595
77.90	1324	90.95	3194	105.95	2932	117.05	4269
78.10	666	92.05	20728	106.90	904	118.05	1999
78.95	22403	93.05	31819	109.60	172	119.05	3548
80.05	5803	94.10	88256	110.10	718	121.95	303
81.00	23179	95.10	742827	111.00	589	123.10	98
81.95	4945	96.10	51221	111.95	493	123.80	96
83.10	683	97.10	2081	112.80	276	124.15	549
86.00	841	102.70	172	113.15	346	124.80	122
87.05	25101	103.10	217	114.85	392	125.30	72

Average of 13.744 to 13.751 min.: VL040049.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.80	84	135.10	981	143.80	380	152.70	87
126.20	143	136.10	273	144.90	426	153.00	199
126.90	78	136.95	1189	145.80	307	153.95	519
127.20	91	138.10	58	146.15	764	155.00	1388
127.80	699	138.90	67	147.00	481	156.00	496
128.05	1549	139.10	160	147.70	246	156.90	611
129.05	1097	139.75	436	148.05	1407	157.10	456
130.05	2211	141.00	6697	148.90	605	158.10	92
131.05	1134	141.90	428	149.70	81	158.80	312
131.85	128	142.20	264	150.05	608	159.05	403
134.70	287	143.05	7256	152.00	371	160.95	453

Average of 13.744 to 13.751 min.: VL040049.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
166.65	185	172.50	343				
169.00	58	173.05	4251				
169.30	161	174.10	448149				
169.50	146	175.10	31104				
170.10	151	176.10	435072				
170.45	167	177.10	28453				
170.70	98	178.00	1042				
171.40	229	186.90	128				
171.60	91	281.20	152				
171.85	639						
172.20	406						