
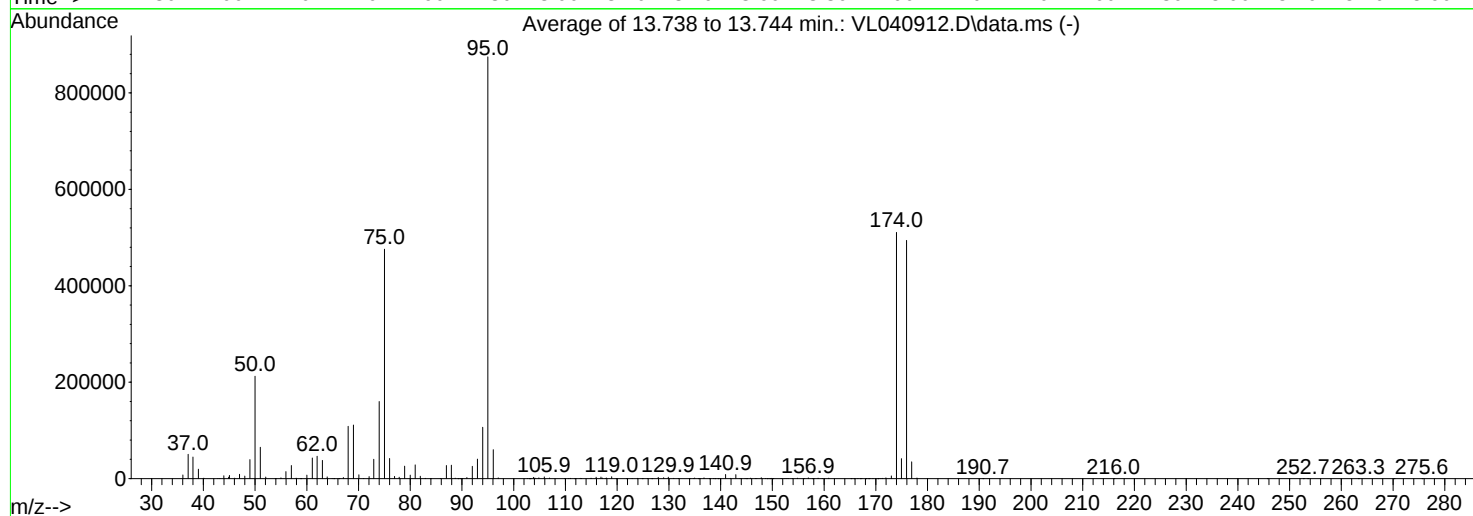


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL122023\
 Data File : VL040912.D
 Acq On : 20 Dec 2023 9:52
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL122023AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Thu Dec 21 07:32:42 2023

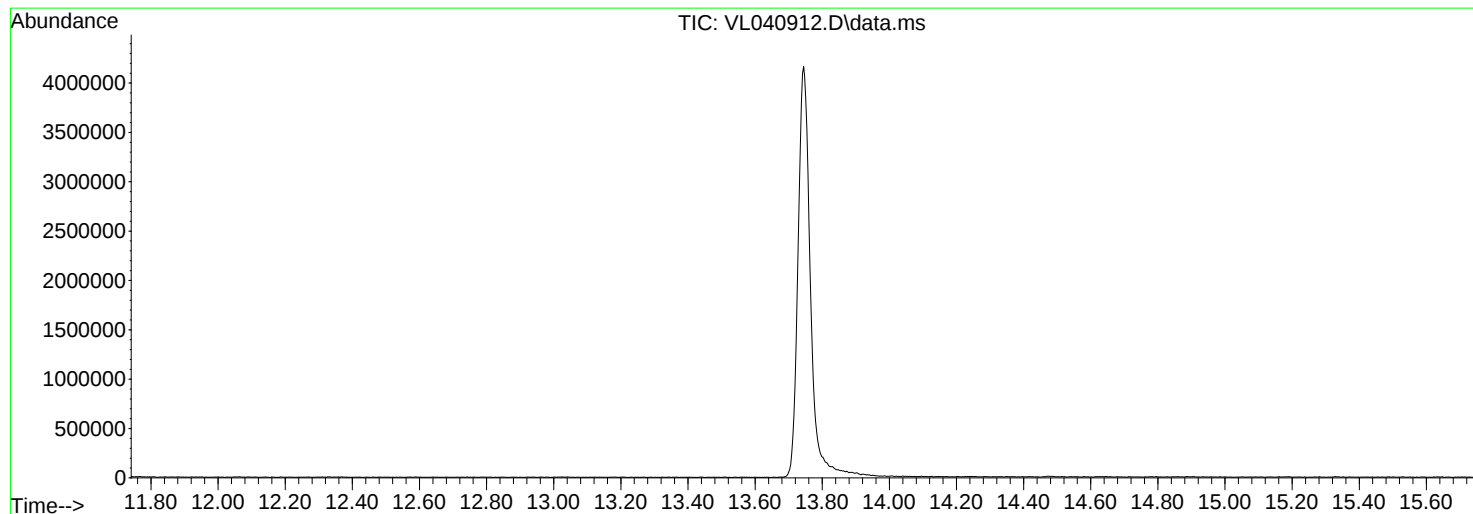

AutoFind: Scans 3463, 3464, 3465; Background Corrected with Scan 3438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	212336	PASS
75	95	30	66	54.4	475925	PASS
95	95	100	100	100.0	874837	PASS
96	95	5	9	6.9	60227	PASS
173	174	0.00	2	1.1	5707	PASS
174	95	50	120	58.4	510741	PASS
175	174	4	9	8.1	41565	PASS
176	174	93	101	96.8	494293	PASS
177	176	5	9	7.0	34797	PASS

Average of 13.738 to 13.744 min.: VL040912.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7686	47.00	8980	58.80	56	69.00	11106
37.05	50408	48.00	5398	60.00	7442	70.05	785
38.00	44797	49.00	39485	61.05	42699	71.00	21
39.05	19673	50.00	212336	62.00	46309	72.05	429
40.10	944	51.00	65109	63.00	37853	72.95	40085
42.80	226	52.05	3354	63.95	3609	74.00	160043
43.20	233	53.90	168	64.90	266	75.00	475925
43.95	5926	55.00	1564	65.20	191	76.00	41971
44.90	2942	55.95	14536	66.20	71	76.95	4604
45.05	6780	57.00	27139	67.05	2434	77.85	3003
46.05	954	57.95	952	68.00	108576	78.90	25859

Average of 13.738 to 13.744 min.: VL040912.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.00	7470	89.95	108	103.80	2634	113.10	353
80.95	28611	90.95	2455	104.10	1312	114.95	869
81.95	5003	92.00	25565	104.85	1738	115.95	2933
82.90	535	93.00	40563	105.90	3762	116.85	3412
83.90	139	94.00	106680	106.95	1270	117.10	1354
85.85	449	95.00	874837	109.80	383	117.80	797
87.00	27168	96.05	60227	110.65	321	117.95	1434
87.95	27981	97.00	1748	110.95	794	118.95	4142
88.70	879	102.70	378	111.80	145	119.80	54
89.25	126	103.00	115	112.05	462	121.80	152
89.70	73	103.20	80	112.85	723	122.90	403

Average of 13.738 to 13.744 min.: VL040912.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.95	729	135.00	1269	142.95	8295	149.50	156
124.85	114	135.70	149	143.75	369	149.85	618
125.90	303	136.00	202	144.00	346	150.10	160
126.70	99	136.80	1675	144.75	247	151.70	407
127.95	2734	137.85	190	145.00	121	152.45	238
129.00	1954	138.65	269	145.80	1049	152.80	210
129.90	2885	138.90	51	146.70	273	153.05	249
130.95	841	139.50	86	147.00	234	153.90	344
131.85	192	140.00	390	147.85	1879	154.85	1181
133.90	115	140.95	8552	148.70	229	156.00	128
134.80	446	141.90	806	149.00	174	156.95	1551

Average of 13.738 to 13.744 min.: VL040912.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.80	82	168.60	63	174.95	41565	275.60	52
158.05	332	168.85	209	175.95	494293		
158.85	1064	169.45	354	176.95	34797		
159.65	306	170.00	309	177.95	1209		
160.90	1000	170.40	69	190.70	104		
165.20	70	170.60	358	216.00	66		
165.80	59	171.00	343	245.70	82		
166.55	458	171.35	816	252.65	131		
167.00	52	171.95	1635	253.50	108		
167.30	278	173.00	5707	263.30	118		
168.10	172	174.00	510741	270.20	73		