


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL122121\
 Data File : VL038211.D
 Acq On : 21 Dec 2021 12:42
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL122121AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Dec 21 17:47:08 2021
 Last Update : Tue Dec 21 17:47:08 2021

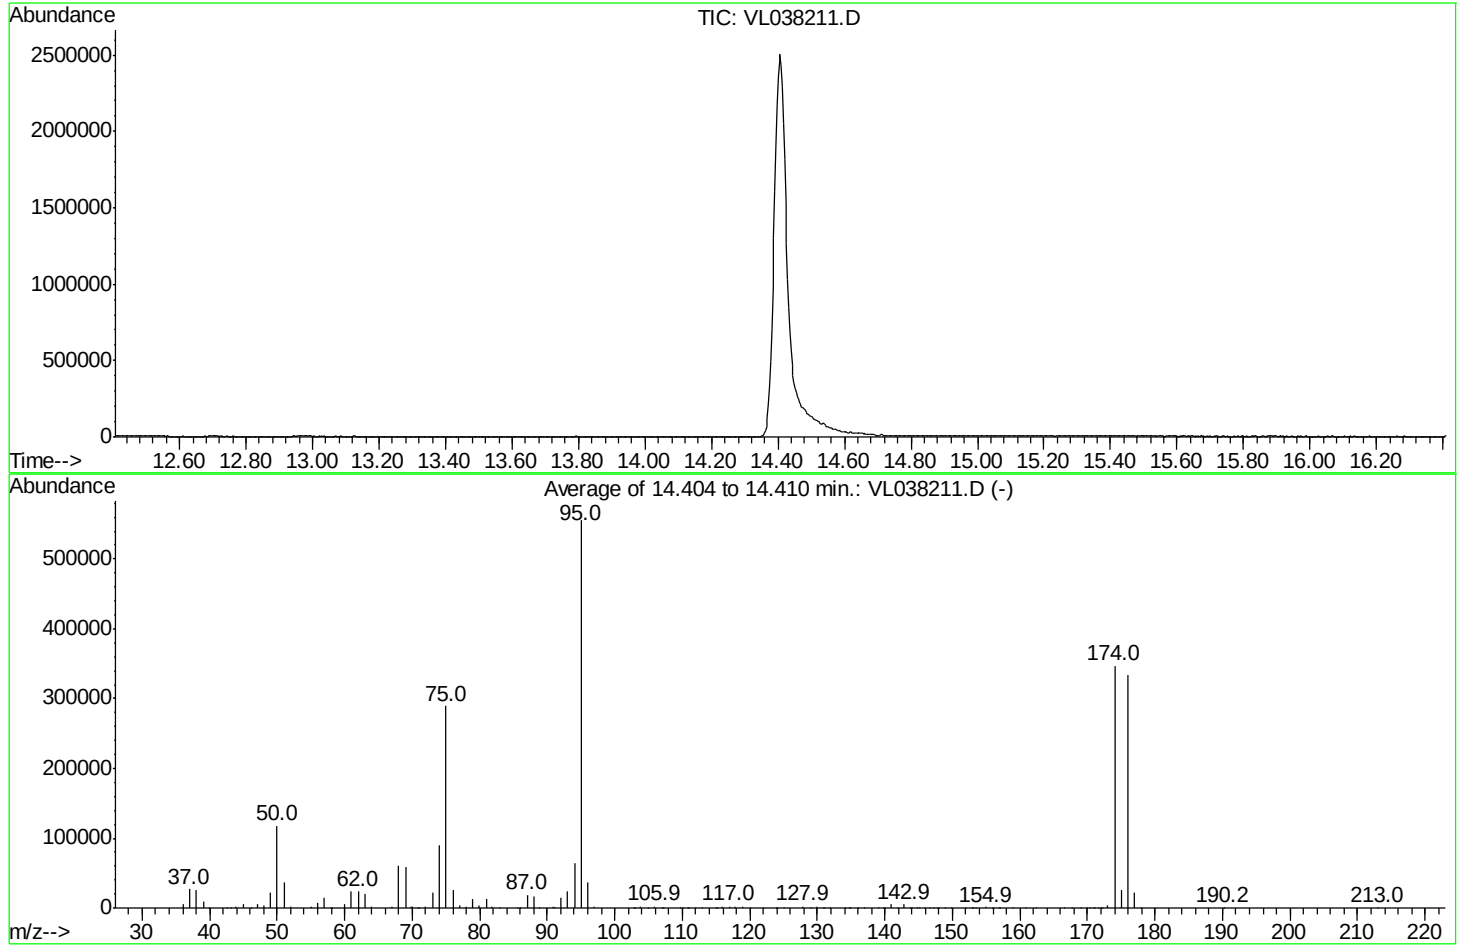

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.2	118013	PASS
75	95	30	66	52.1	289514	PASS
95	95	100	100	100.0	555456	PASS
96	95	5	9	6.6	36824	PASS
173	174	0.00	2	0.9	2998	PASS
174	95	50	120	62.4	346645	PASS
175	174	4	9	7.5	25997	PASS
176	174	93	101	96.2	333461	PASS
177	176	5	9	6.5	21568	PASS