


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL122222\
 Data File : VL040060.D
 Acq On : 22 Dec 2022 9:17
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121922AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Dec 20 04:50:21 2022

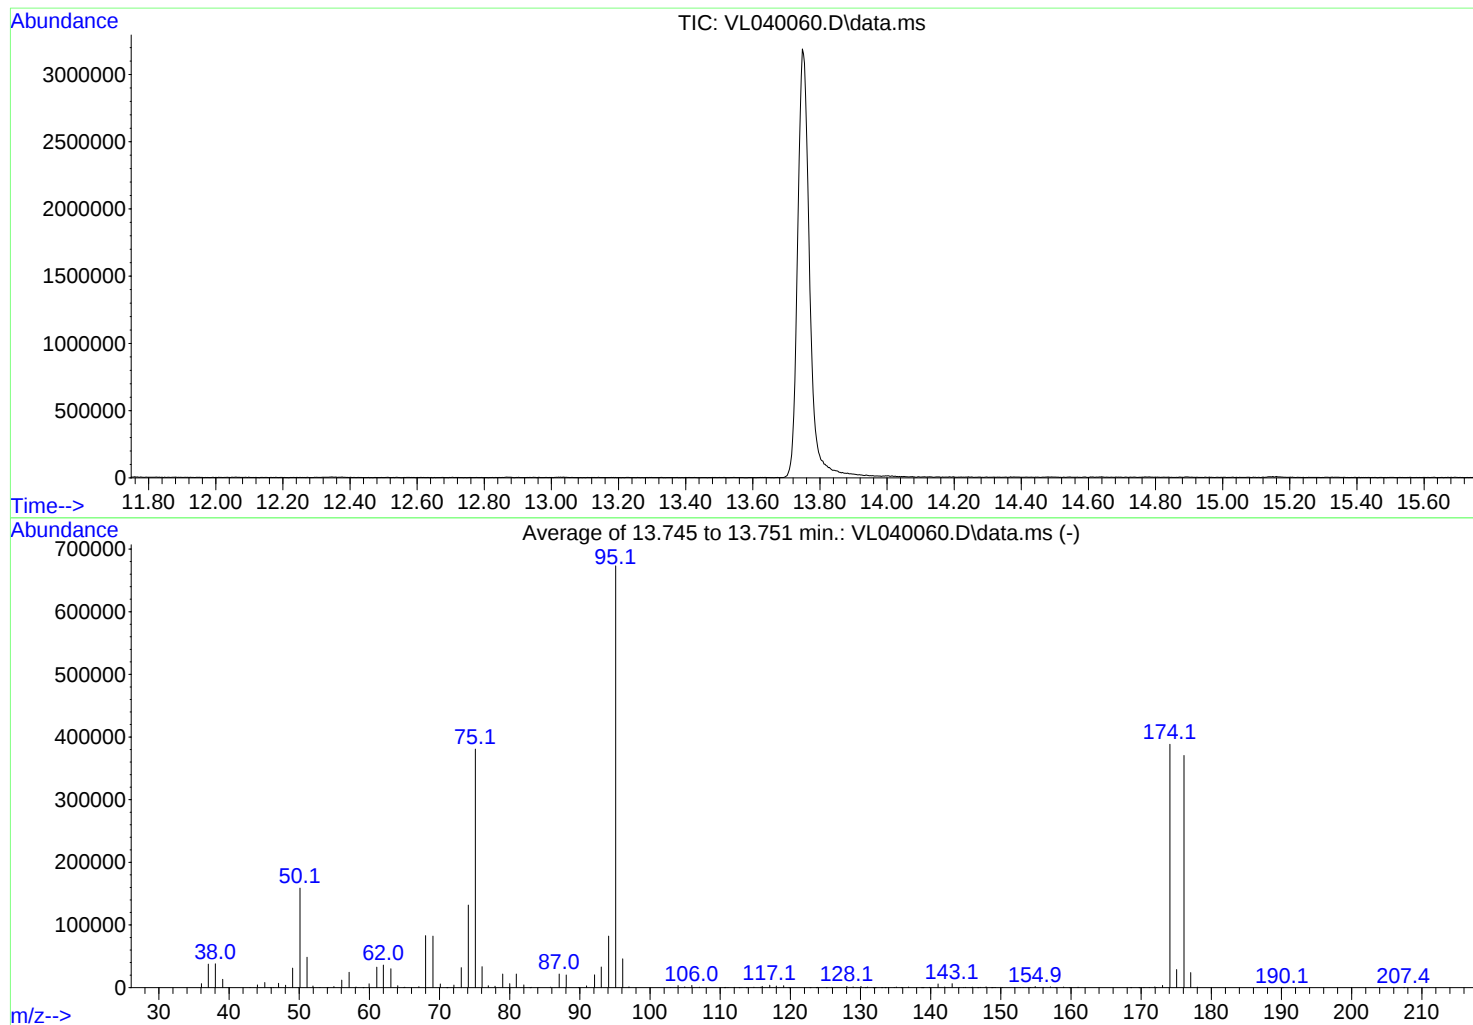

AutoFind: Scans 3465, 3466, 3467; Background Corrected with Scan 3441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	158891	PASS
75	95	30	66	56.6	380757	PASS
95	95	100	100	100.0	673259	PASS
96	95	5	9	6.8	45864	PASS
173	174	0.00	2	0.9	3504	PASS
174	95	50	120	57.7	388565	PASS
175	174	4	9	7.4	28901	PASS
176	174	93	101	95.3	370475	PASS
177	176	5	9	6.5	23987	PASS

Average of 13.745 to 13.751 min.: VL040060.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6309	48.05	3792	59.10	109	70.10	601
37.05	37480	49.05	31245	59.95	6136	71.05	15
38.05	37995	50.10	158891	61.05	32605	72.05	397
39.10	13222	51.10	48656	62.00	35995	73.10	3183
40.00	349	51.95	2717	63.05	30064	74.10	131923
43.00	268	52.95	362	64.05	3195	75.10	380757
44.05	4456	54.00	122	64.90	394	76.05	33525
45.10	8113	54.95	1857	65.05	770	76.95	3074
45.90	66	56.05	11917	67.05	1616	77.90	2392
46.30	323	57.10	24464	68.00	82971	79.00	21816
47.05	6787	58.10	1117	69.05	82288	80.00	6289

Average of 13.745 to 13.751 min.: VL040060.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.95	21752	93.05	32883	110.60	87	118.00	2492
82.00	4260	94.10	82376	110.80	501	119.05	3228
82.90	130	95.10	673259	111.10	171	119.80	140
83.05	420	96.10	45864	112.00	448	122.80	57
84.15	163	97.00	1289	112.70	155	123.70	124
85.80	695	102.95	218	113.10	165	123.90	448
87.05	21707	104.00	3336	113.70	58	125.10	122
88.05	20213	104.95	1198	114.80	823	125.90	427
89.80	112	105.95	3519	115.80	886	128.05	2130
90.95	2943	107.05	893	116.00	2066	128.95	1271
92.10	20339	110.00	394	117.05	3835	130.05	2125

Average of 13.745 to 13.751 min.: VL040060.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
130.70	120	138.70	118	146.70	97	153.90	136
131.00	1037	138.90	111	147.05	434	154.20	243
131.80	62	139.85	657	147.90	1251	154.90	1709
132.10	66	141.05	5867	148.70	104	156.05	269
133.00	62	142.00	933	149.00	358	157.05	1368
133.50	95	143.05	6480	149.20	175	157.80	72
134.00	163	144.05	380	150.00	617	158.95	1013
134.80	279	144.70	172	150.20	221	159.80	72
135.10	1069	144.95	559	151.95	184	161.00	715
135.80	136	145.80	230	152.75	218	168.50	87
136.85	1078	145.95	904	153.15	255	169.70	129

Average of 13.745 to 13.751 min.: VL040060.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.40	294	207.40	75				
171.15	235						
171.95	1420						
172.20	400						
173.05	3504						
174.10	388565						
175.05	28901						
176.10	370475						
177.05	23987						
178.05	804						
190.10	147						