


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL122921\
 Data File : VL038230.D
 Acq On : 29 Dec 2021 11:56
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL122121AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Dec 21 17:47:08 2021
 Last Update : Tue Dec 21 17:47:08 2021

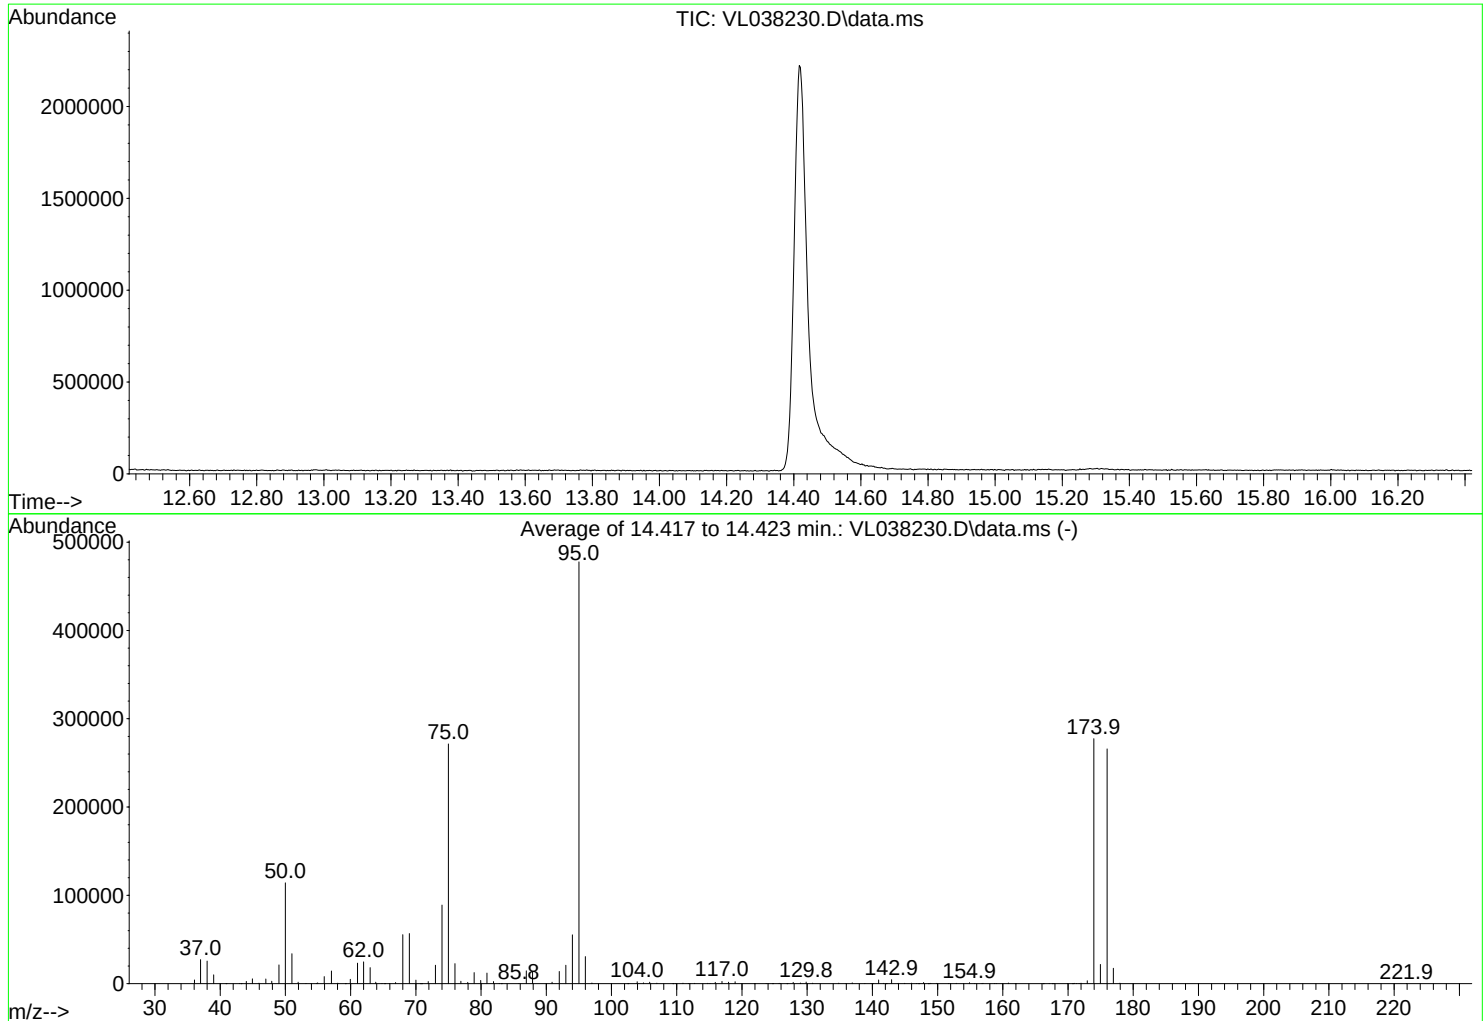

AutoFind: Scans 3617, 3618, 3619; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	114216	PASS
75	95	30	66	56.8	271531	PASS
95	95	100	100	100.0	477696	PASS
96	95	5	9	6.4	30715	PASS
173	174	0.00	2	1.2	3337	PASS
174	95	50	120	58.1	277504	PASS
175	174	4	9	7.8	21691	PASS
176	174	93	101	95.8	265856	PASS
177	176	5	9	6.6	17454	PASS

Average of 14.417 to 14.423 min.: VL038230.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	4174	47.90	2694	58.05	484	68.00	5551
37.00	27117	49.00	21264	59.20	85	69.00	5680
38.00	25483	50.00	114216	59.95	4898	70.00	401
39.00	9958	51.00	33819	61.05	23147	70.70	5
40.90	55	51.95	1619	62.00	24723	70.90	62
42.95	258	53.15	142	63.00	18091	71.90	2367
43.20	62	53.95	220	63.85	1694	73.00	20797
44.00	2606	54.80	456	64.80	283	74.00	88957
44.95	5363	54.95	885	65.20	56	75.00	271531
45.95	482	55.95	8011	65.95	165	76.00	22645
47.00	5313	57.05	14355	66.90	1290	76.90	2686

Average of 14.417 to 14.423 min.: VL038230.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.95	1525	92.00	13857	109.40	60	118.95	2109
78.95	12555	93.00	20829	109.85	267	121.90	67
79.95	3698	94.00	55213	110.95	486	123.70	158
80.90	11961	95.00	477696	111.80	233	124.00	196
81.90	2416	96.00	30715	112.00	139	124.70	51
82.80	281	97.00	819	112.75	426	125.70	295
83.10	55	102.50	61	114.75	357	125.90	125
85.80	285	103.95	2189	115.10	113	126.90	51
86.95	14511	104.90	975	115.90	1439	127.85	1527
87.90	13862	105.85	1687	116.95	2603	128.95	748
90.90	1698	106.95	467	117.95	1698	129.85	1774

Average of 14.417 to 14.423 min.: VL038230.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
130.85	570	143.95	347	152.85	408	167.10	146
134.85	603	144.95	417	153.95	144	167.60	59
135.95	209	146.00	589	154.90	1061	167.90	175
136.90	836	146.80	113	155.70	117	169.90	273
138.85	244	147.10	88	156.80	228	170.70	79
139.80	273	147.85	1284	156.95	404	170.95	317
140.00	89	148.60	95	158.75	277	171.30	141
140.95	4156	148.95	413	159.00	174	171.70	190
141.75	317	149.90	411	160.85	691	172.00	521
142.10	110	151.70	167	161.90	75	172.95	3337
142.95	4517	151.95	181	166.20	50	173.95	277504

Average of 14.417 to 14.423 min.: VL038230.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.95	21691						
176.00	265856						
176.95	17454						
177.95	606						
221.90	169						

Instrument :

MSVOA_L

ClientSampleId :

BFB