

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL030322\
Data File : VL038514.D
Acq On : 3 Mar 2022 14:59
Operator : SY/AP
Sample : CAN 10722
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10722

Quant Time: Mar 04 05:56:12 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL022222AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
QLast Update : Tue Feb 22 19:45:51 2022
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.66	49	791071	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.16	114	1777968	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.07	117	1562684	10.00	ppbv	0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.40	95	1290027	9.98	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.80%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL030322\
Data File : VL038514.D
Acq On : 3 Mar 2022 14:59
Operator : SY/AP
Sample : CAN 10722
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10722

Quant Time: Mar 04 05:56:12 2022
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL022222AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
QLast Update : Tue Feb 22 19:45:51 2022
Response via : Initial Calibration

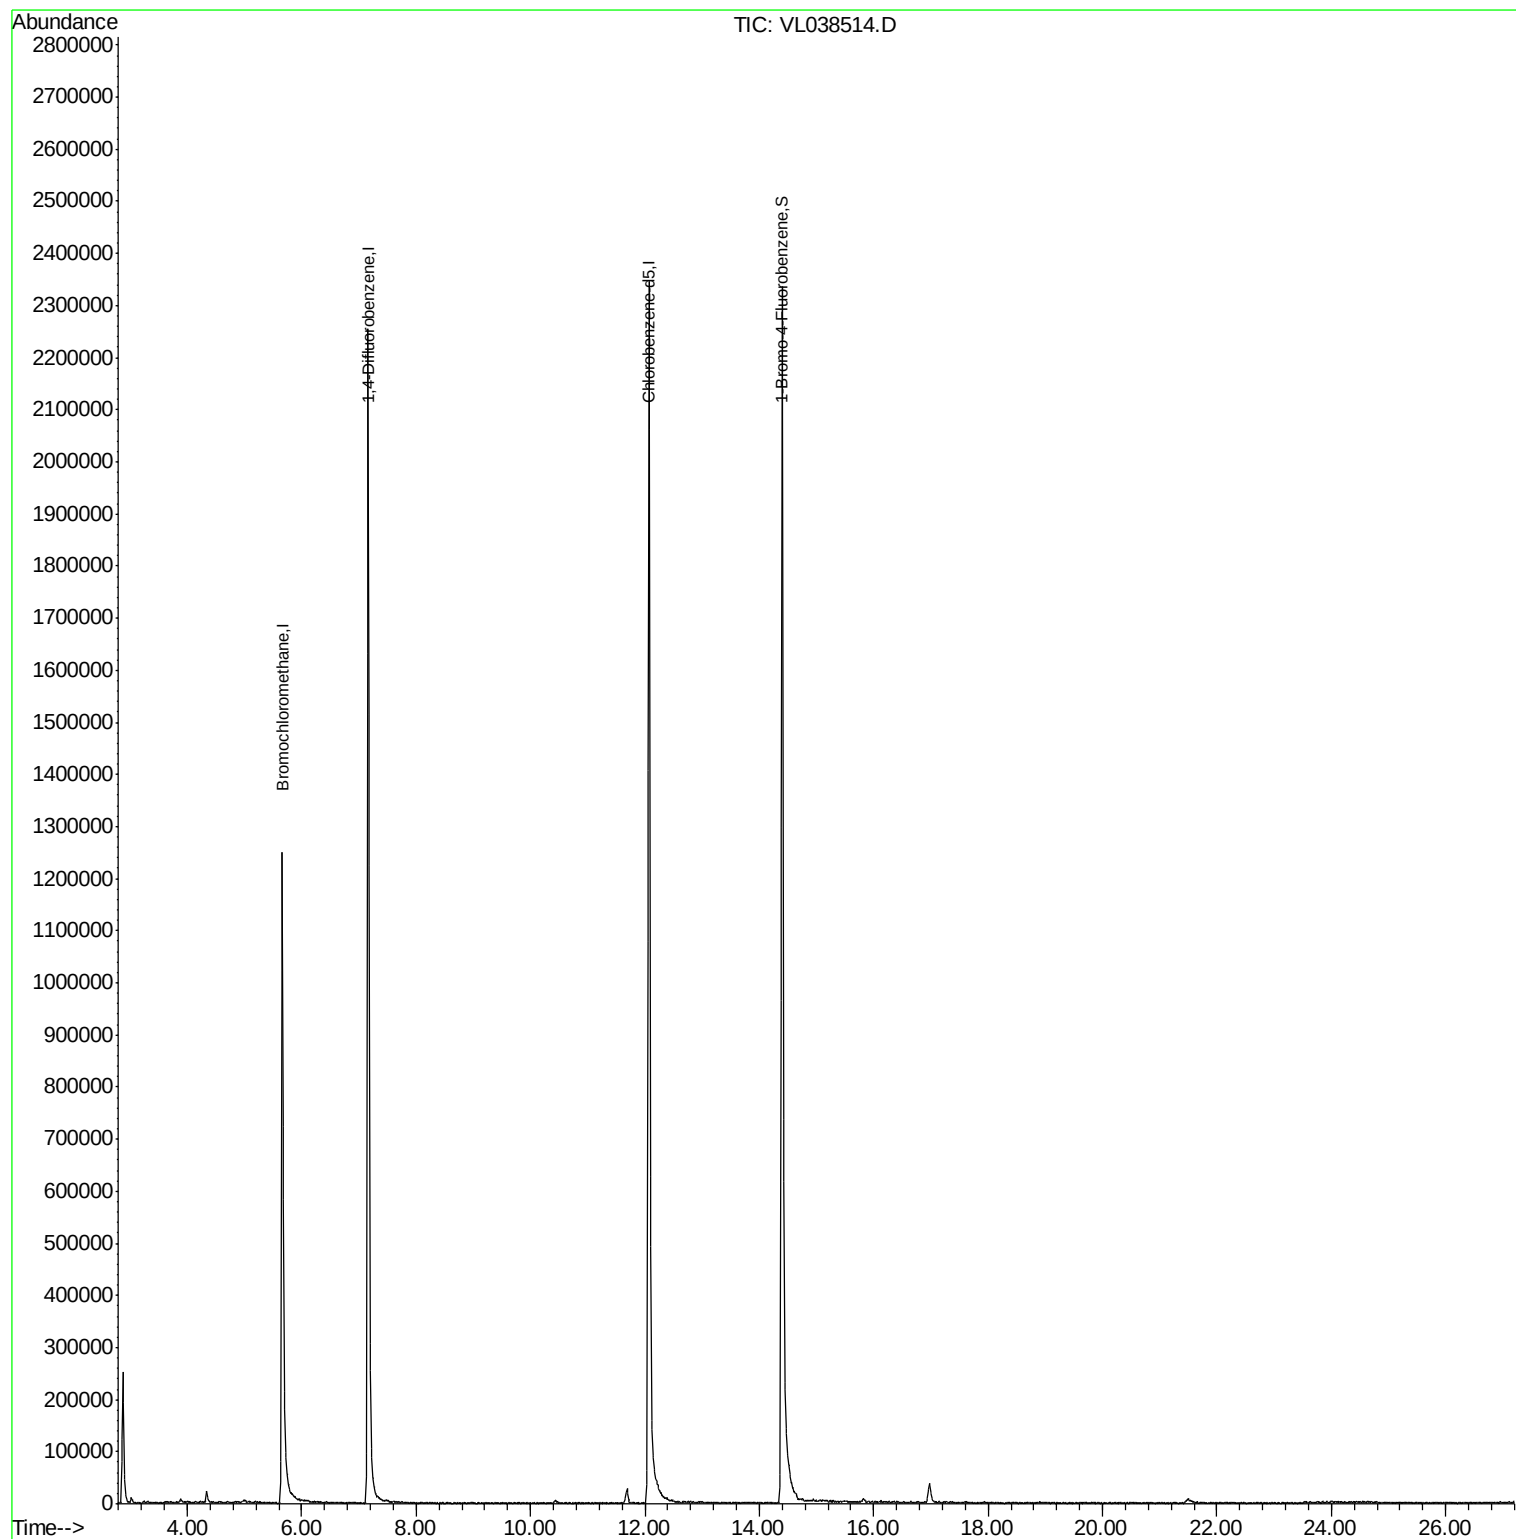

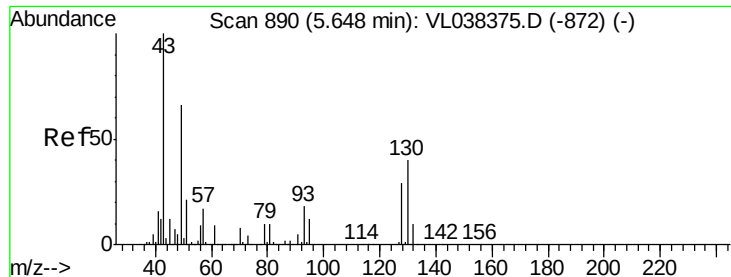

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.66 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 3 Mar 2022 14:59 CAN 10722


Tot Ion: 49 Resp: 791071

Ion Ratio Lower Upper

49 100

128 45.3 24.3 72.9




130 57.5 30.1 90.5

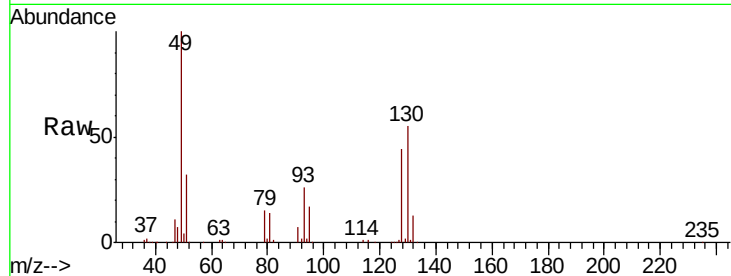

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

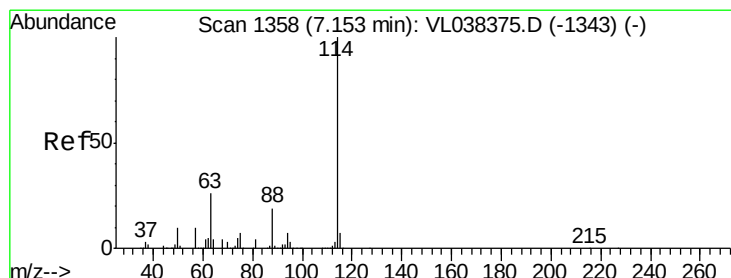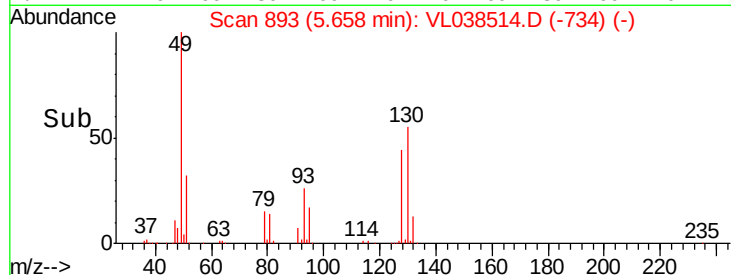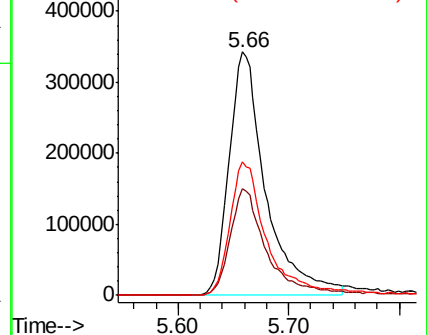

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.16 min Scan# 1361

Delta R.T. 0.01 min

Lab File: VL038514.D

Acq: 3 Mar 2022 14:59


Tgt Ion: 114 Resp: 1777968

Ion Ratio Lower Upper

114 100

63 28.6 22.2 33.2



88 18.9 15.2 22.8

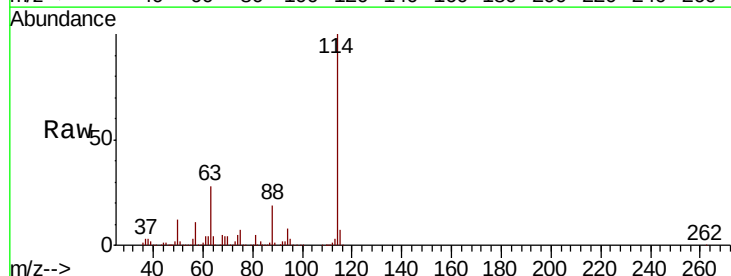


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0





Ion 88.10 (87.80 to 88.80): VL0

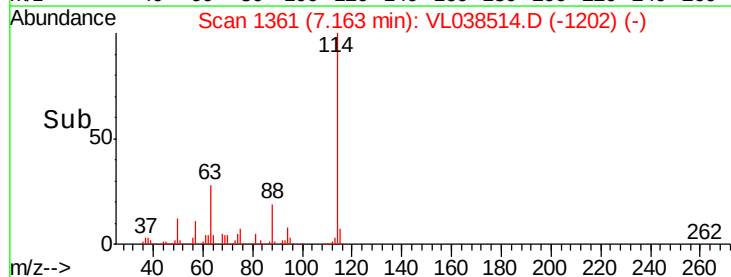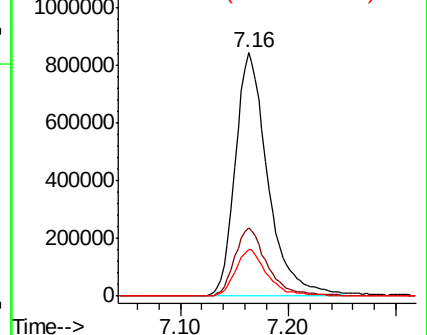

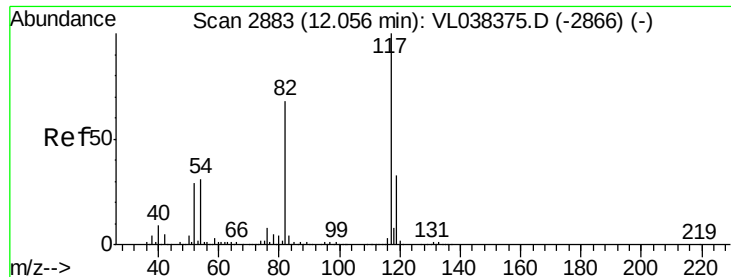

#55
 Chlorobenzene-d5
 Concen: 10.000 ppbv
 RT: 12.07 min
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId :
 Acq: 3 Mar 2022 14:59

Tot Ion: 117 Resp: 1562684
 Ion Ratio Lower Upper
 117 100
 82 73.5 54.9 82.3
 119 33.9 46.1 69.1#

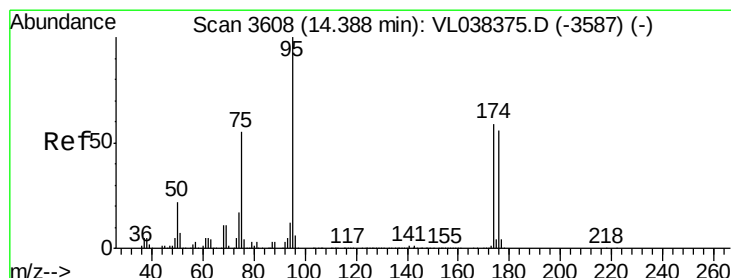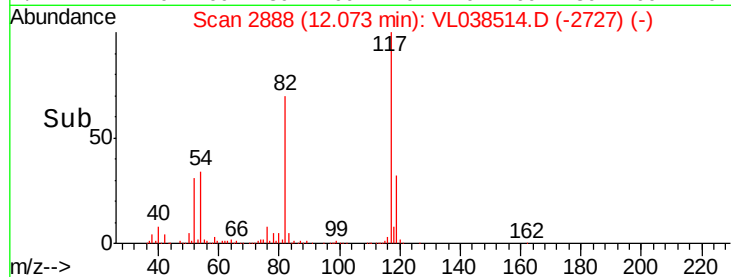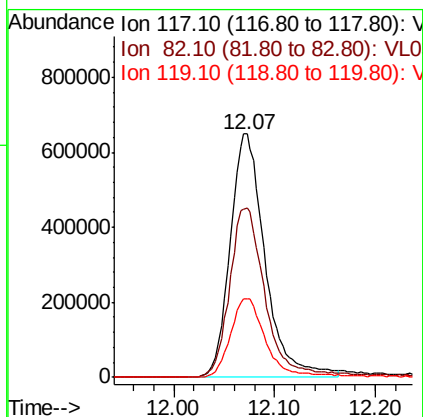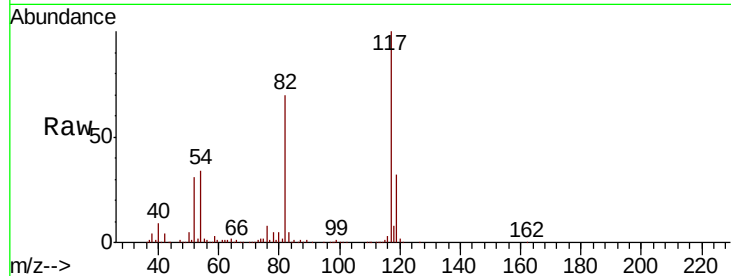

#68
 1-Bromo-4-Fluorobenzene
 Concen: 9.977 ppbv
 RT: 14.40 min Scan# 3611
 Delta R.T.: 0.01 min
 Lab File: VL038514.D
 Acq: 3 Mar 2022 14:59

Tgt Ion: 95 Resp: 1290027
 Ion Ratio Lower Upper
 95 100
 174 58.8 49.0 73.4
 175 4.2 3.6 5.4

