

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL030322\
Data File : VL038530.D
Acq On : 4 Mar 2022 1:41
Operator : SY/AP
Sample : CAN 10606
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10606

Quant Time: Mar 04 06:45:41 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL022222AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
QLast Update : Tue Feb 22 19:45:51 2022
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.64	49	806834	10.00	ppbv	-0.01
33) 1,4-Difluorobenzene	7.14	114	1795941	10.00	ppbv	-0.02
55) Chlorobenzene-d5	12.04	117	1635016	10.00	ppbv	-0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.37	95	1310085	9.68	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	96.80%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL030322\
Data File : VL038530.D
Acq On : 4 Mar 2022 1:41
Operator : SY/AP
Sample : CAN 10606
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10606





Quant Time: Mar 04 06:45:41 2022
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL022222AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
QLast Update : Tue Feb 22 19:45:51 2022
Response via : Initial Calibration

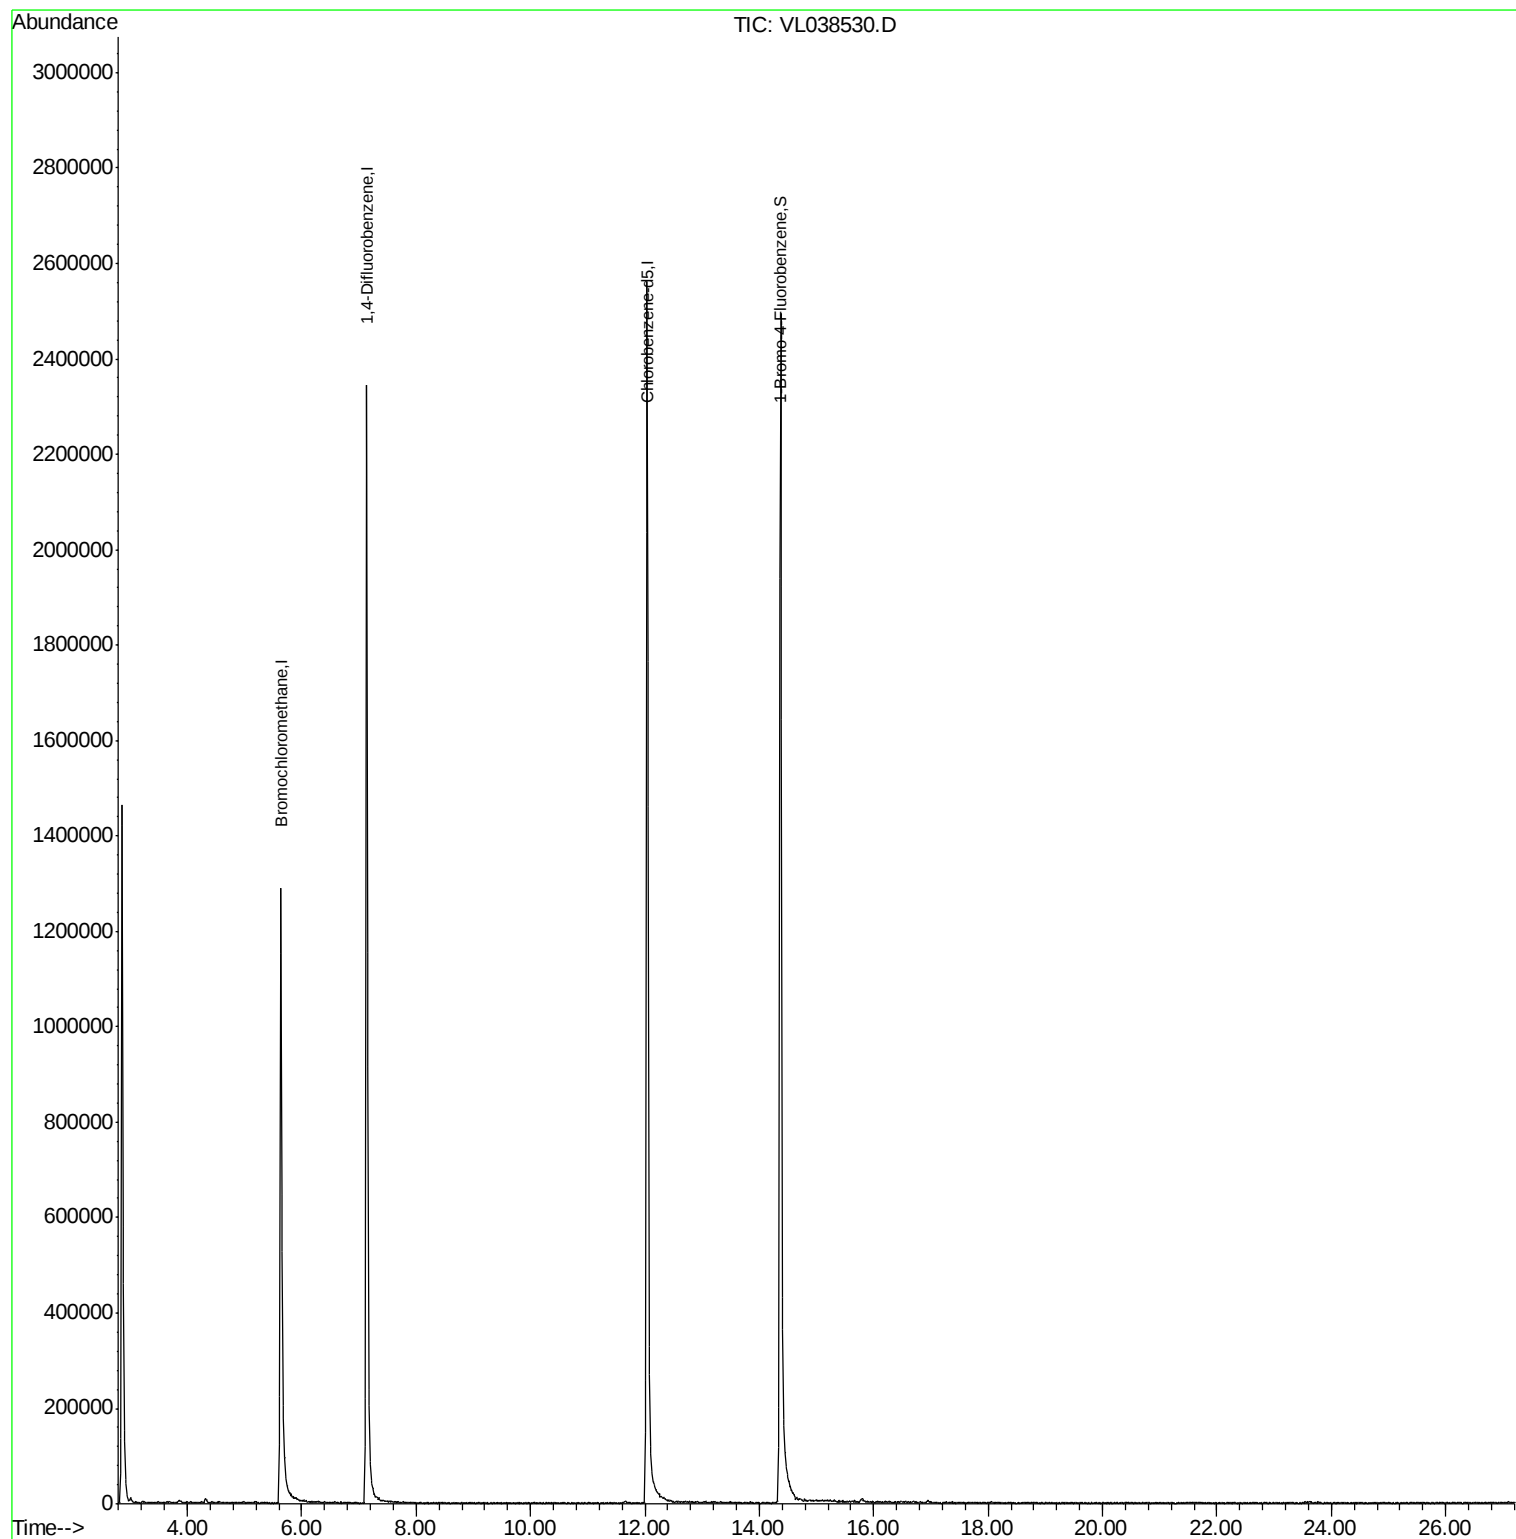

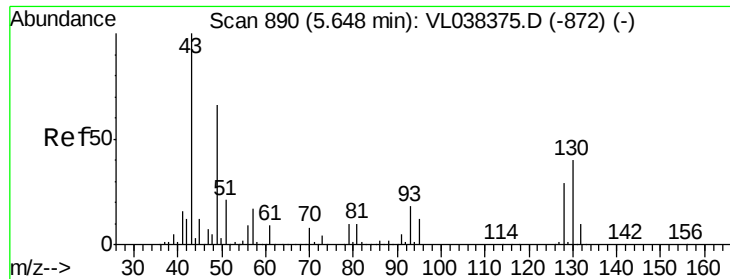




#1
 Bromochloromethane
 Concen: 10.000 ppbv
 RT: 5.64
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId:
 Acq: 4 Mar 2022 1:41


Tot Ion: 49 Resp: 806834
 Ion Ratio Lower Upper
 49 100
 128 45.5 24.3 72.9
 130 57.3 30.1 90.5

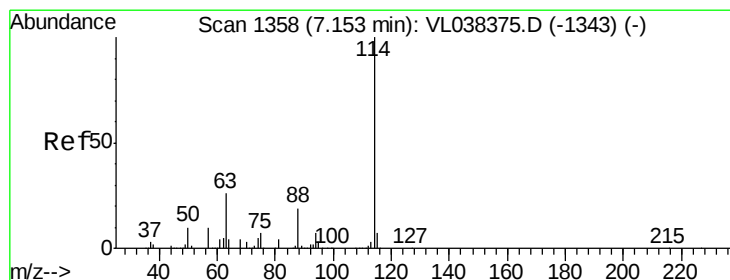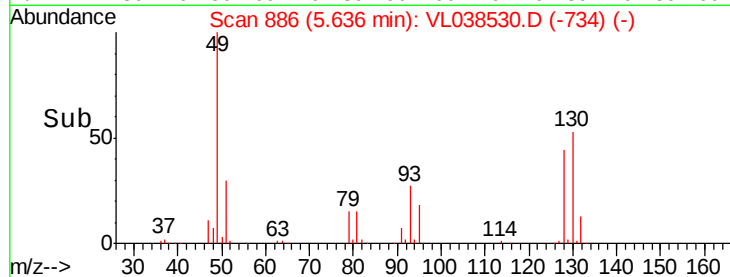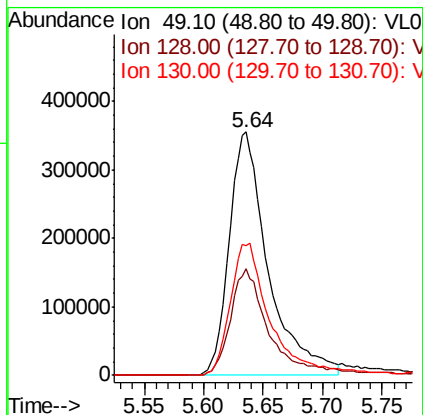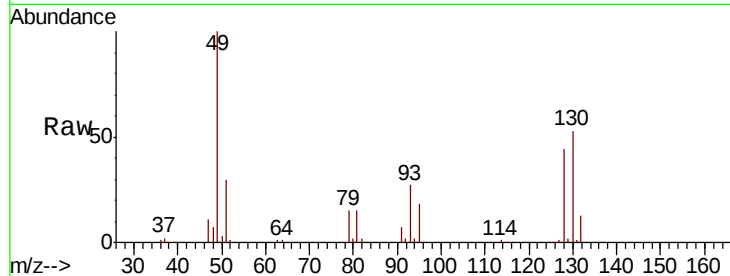

#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.14 min Scan# 1353
 Delta R.T. -0.02 min
 Lab File: VL038530.D
 Acq: 4 Mar 2022 1:41





Tgt Ion: 114 Resp: 1795941
 Ion Ratio Lower Upper
 114 100
 63 29.2 22.2 33.2
 88 19.4 15.2 22.8

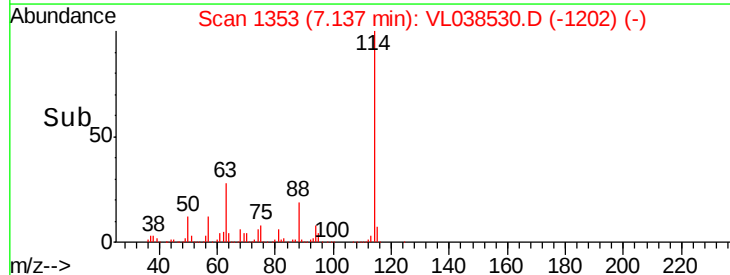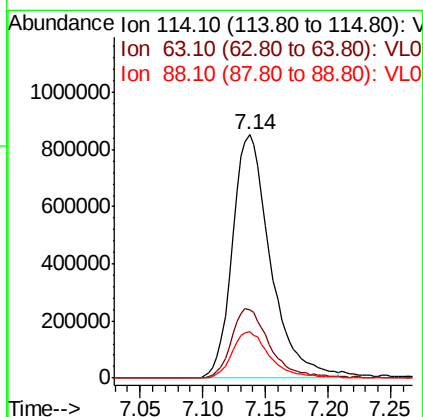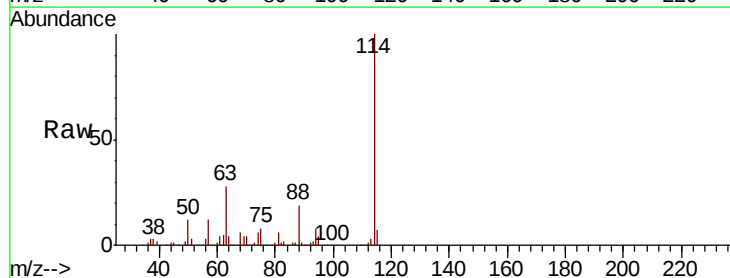

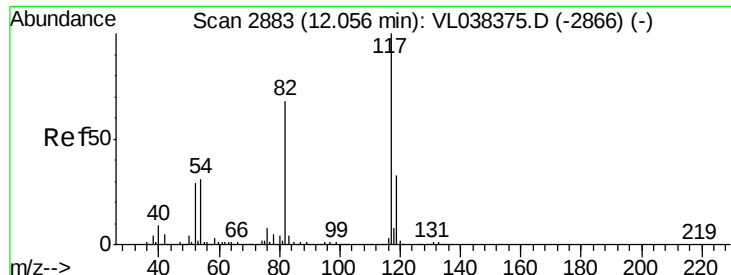

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.04 min
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId :
Acq: 4 Mar 2022 1:41

Tot Ion:117 Resp: 1635016
Ion Ratio Lower Upper
117 100
82 71.3 54.9 82.3
119 32.8 46.1 69.1#

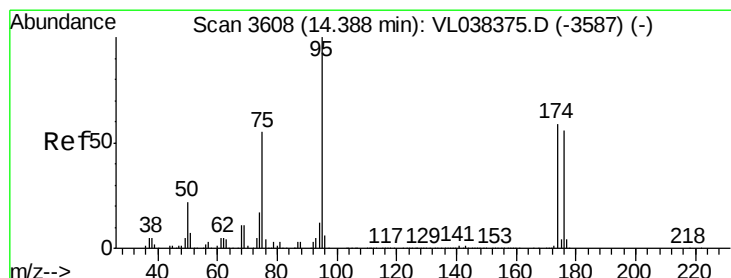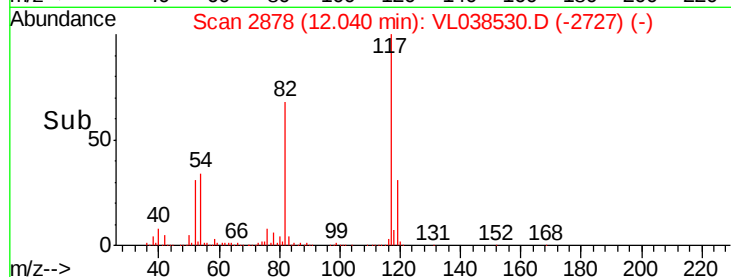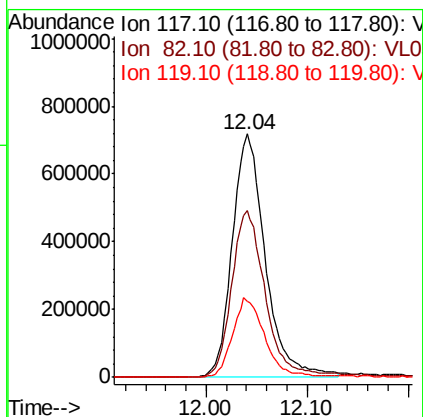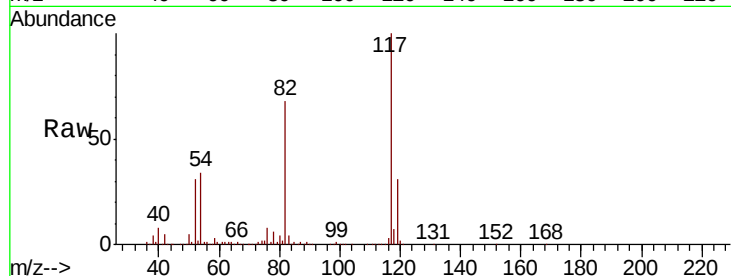

#68
1-Bromo-4-Fluorobenzene
Concen: 9.684 ppbv
RT: 14.37 min Scan# 3602
Delta R.T.: -0.02 min
Lab File: VL038530.D
Acq: 4 Mar 2022 1:41

Tgt Ion: 95 Resp: 1310085
Ion Ratio Lower Upper
95 100
174 59.6 49.0 73.4
175 4.3 3.6 5.4

