
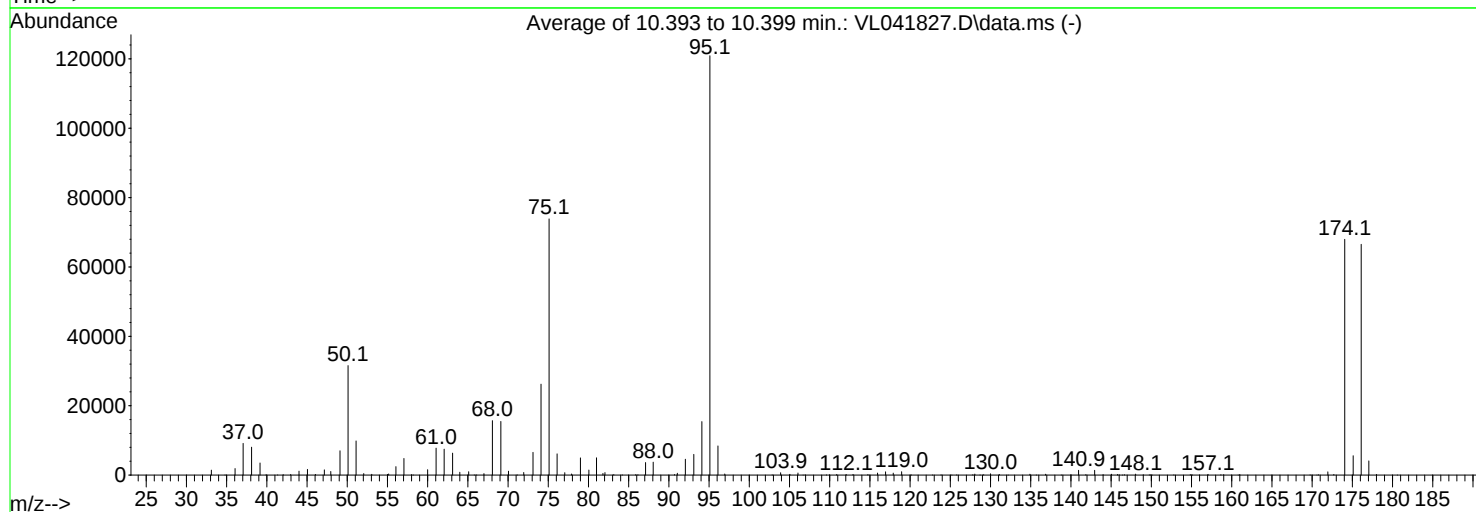


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL010325\
Data File : VL041827.D
Acq On : 03 Jan 2025 13:33
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Dec 19 07:32:09 2024

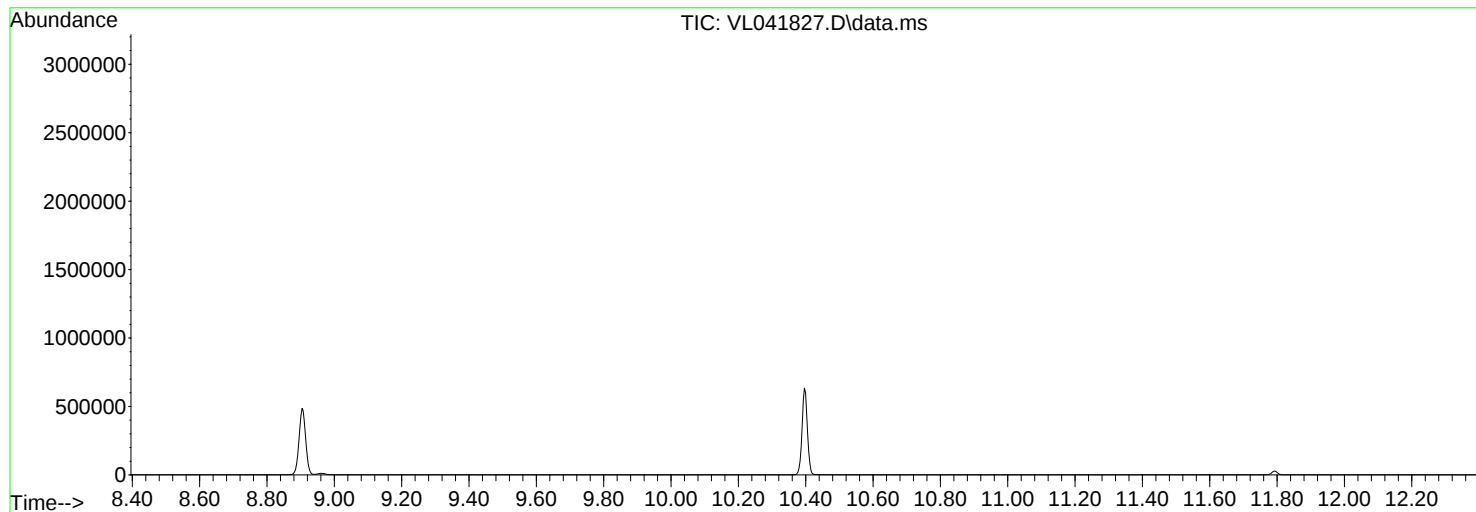

AutoFind: Scans 3184, 3185, 3186; Background Corrected with Scan 3168

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.1	31573	PASS
75	95	30	66	61.1	73861	PASS
95	95	100	100	100.0	120907	PASS
96	95	5	9	6.9	8403	PASS
173	174	0.00	2	0.3	187	PASS
174	95	50	120	56.2	67971	PASS
175	174	4	9	8.2	5580	PASS
176	174	93	101	97.9	66528	PASS
177	176	5	9	6.1	4081	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1428	45.05	1633	56.05	2441	66.10	24
34.80	24	46.05	180	57.05	4784	67.00	435
36.05	1891	47.15	1511	58.00	108	68.05	1569
37.05	9133	47.95	1041	58.20	34	69.10	1545
38.10	8041	49.10	7008	60.00	1548	70.05	1122
39.15	3489	50.10	31573	61.05	7760	71.15	51
39.90	66	51.10	9839	62.05	7481	71.95	752
41.35	45	52.05	443	63.10	6334	73.10	6542
42.05	84	53.05	225	64.00	814	74.10	26208
42.95	147	55.00	178	65.10	970	75.10	73861
44.00	1138	55.15	314	65.80	50	76.10	6120

Average of 10.393 to 10.399 min.: VL041827.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	693	87.10	3611	103.90	681	115.95	576
77.90	317	88.05	3721	105.05	221	116.95	938
79.00	4962	90.70	137	106.05	602	117.90	565
80.05	1460	91.05	530	106.70	18	118.95	967
81.00	4982	92.05	4567	106.95	60	120.15	44
81.80	469	93.10	5969	109.60	38	122.80	32
82.05	718	94.10	15422	110.00	60	123.85	61
83.15	142	95.10	120907	110.85	133	125.20	23
84.20	56	96.10	8403	112.05	160	125.80	59
85.85	98	96.95	325	112.90	190	127.80	99
86.15	99	102.85	58	114.75	166	128.05	295

Average of 10.393 to 10.399 min.: VL041827.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.70	41	141.85	120	149.90	52	169.75	55
129.15	109	142.95	1373	150.10	18	170.60	18
130.00	377	144.00	111	152.80	58	170.80	80
131.10	175	145.05	255	154.85	137	171.95	924
132.20	23	145.80	182	155.10	49	172.70	187
134.90	259	146.00	72	156.00	24	174.05	67971
135.70	24	146.40	20	157.05	206	175.10	5580
136.85	250	146.65	106	158.65	106	176.10	66528
138.80	24	148.05	272	159.00	101	177.05	4081
140.00	67	149.00	70	160.80	19	178.00	179
140.95	1374	149.75	71	161.00	159	180.60	23

Instrument :

MSVOA_L

ClientSampleId :

BFB