


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL010419\  
 Data File : VL033060.D  
 Acq On : 4 Jan 2019 8:36  
 Operator : SY/AP  
 Sample : BFB  
 Misc : 400ml/MSVOA L  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_L  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL010419AIR.M  
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Fri Jan 04 16:09:05 2019  
 Last Update : Fri Jan 04 16:09:05 2019

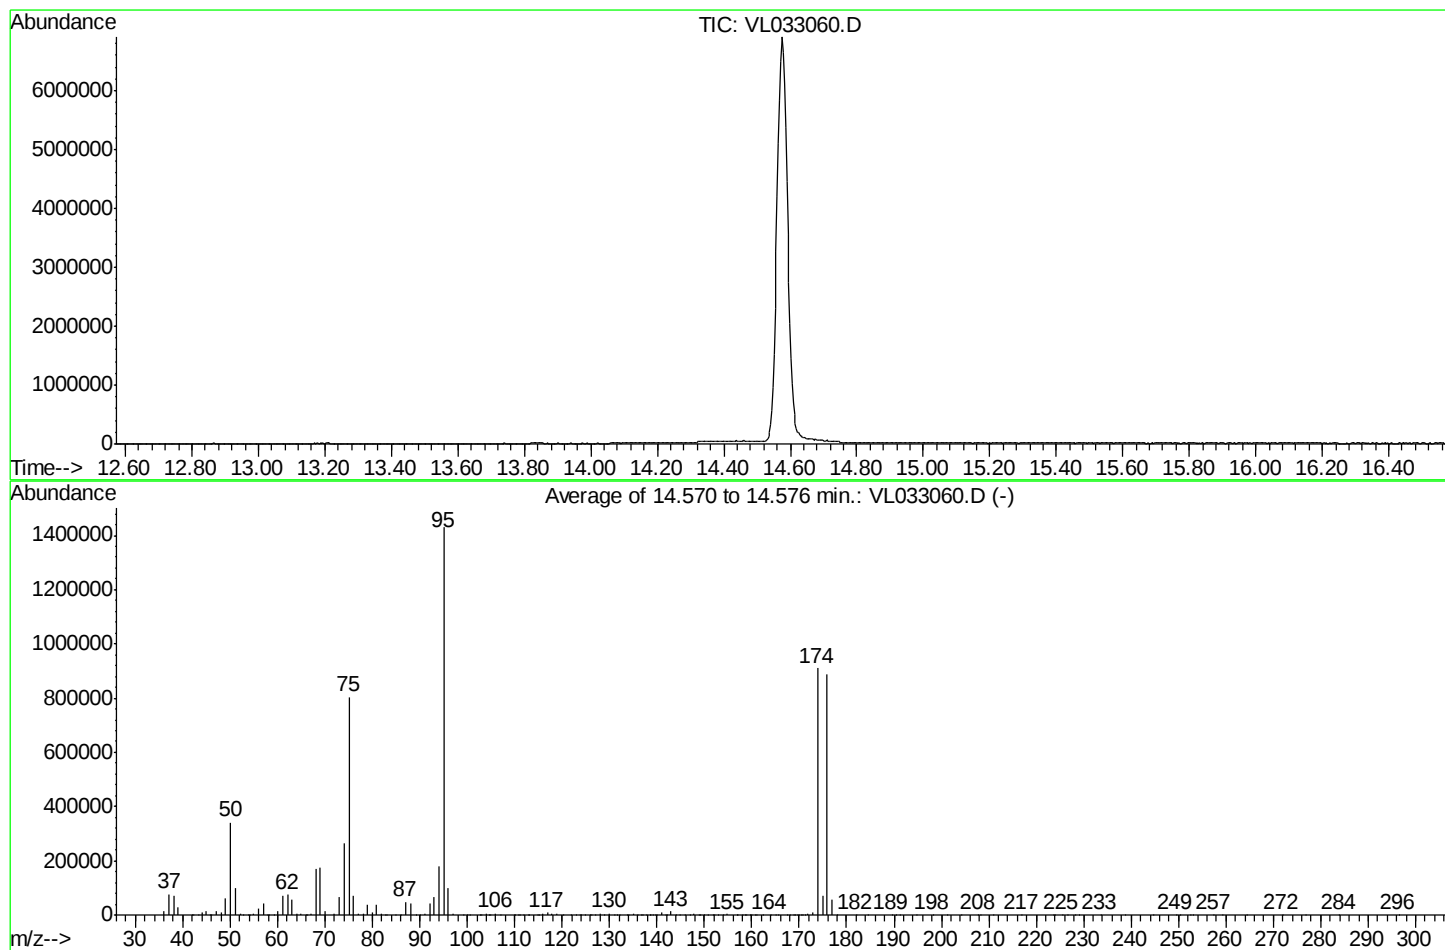

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3594

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 8            | 40           | 23.9      | 341120  | PASS             |
| 75          | 95           | 30           | 66           | 56.2      | 803264  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 1430016 | PASS             |
| 96          | 95           | 5            | 9            | 7.0       | 100621  | PASS             |
| 173         | 174          | 0.00         | 2            | 1.1       | 9549    | PASS             |
| 174         | 95           | 50           | 120          | 63.6      | 909376  | PASS             |
| 175         | 174          | 4            | 9            | 7.9       | 72141   | PASS             |
| 176         | 174          | 93           | 101          | 97.6      | 887786  | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 59122   | PASS             |