
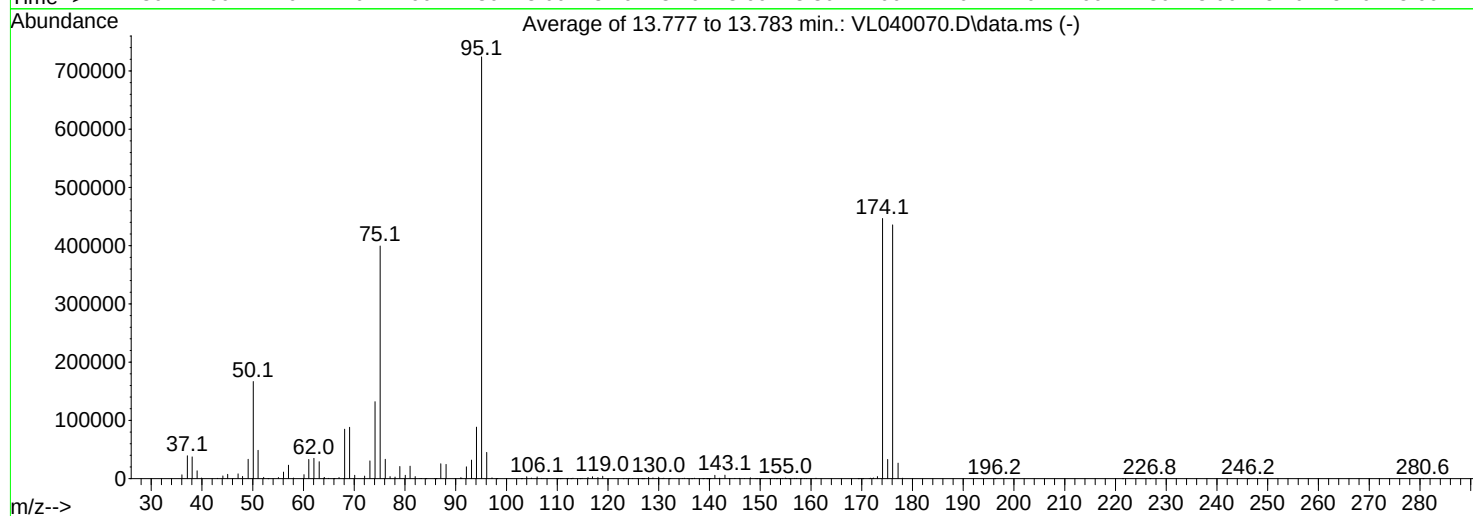


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL010923\
 Data File : VL040070.D
 Acq On : 9 Jan 2023 10:00
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121922AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Jan 10 00:22:08 2023

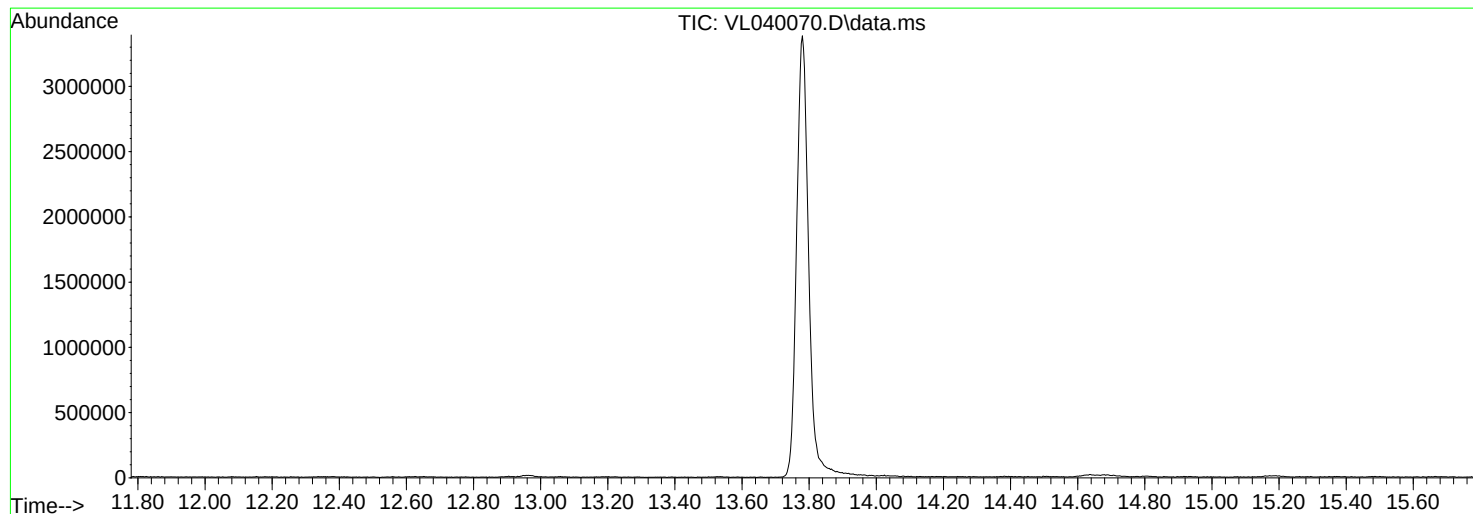

AutoFind: Scans 3475, 3476, 3477; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.0	166656	PASS
75	95	30	66	55.1	399339	PASS
95	95	100	100	100.0	724242	PASS
96	95	5	9	6.2	44973	PASS
173	174	0.00	2	0.8	3539	PASS
174	95	50	120	61.7	446720	PASS
175	174	4	9	7.4	32875	PASS
176	174	93	101	97.5	435669	PASS
177	176	5	9	6.1	26675	PASS

Average of 13.777 to 13.783 min.: VL040070.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6569	49.10	33387	62.05	34896	73.10	30471
37.10	39296	50.10	166656	63.10	29173	74.10	13213
38.05	37317	51.05	48597	64.00	1134	75.10	39933
39.05	13416	52.15	2112	64.15	1868	76.10	3321
39.90	1048	53.00	157	64.95	654	77.05	3504
43.05	469	55.05	1830	66.00	50	78.05	2870
44.10	4585	56.05	11191	67.00	1941	79.00	20827
45.05	7551	57.05	23048	68.10	85000	80.05	5890
46.10	359	58.05	1160	69.10	88184	81.00	21448
47.10	8205	60.10	6949	70.10	5794	82.00	3699
48.00	3816	61.05	32912	72.05	4367	82.95	277

Average of 13.777 to 13.783 min.: VL040070.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
83.20	235	94.10	88571	106.85	588	114.90	589
84.10	56	95.10	724242	107.20	385	116.05	2024
85.85	369	96.10	44973	109.90	287	116.95	3301
86.10	84	97.15	1367	110.10	120	118.00	1960
87.05	25589	98.10	53	110.60	112	118.95	4187
88.10	24579	102.90	93	111.10	296	120.00	134
89.90	162	103.00	264	111.90	155	123.00	56
90.95	1416	103.15	189	112.15	476	123.60	217
91.20	1108	104.00	3270	112.70	97	124.15	469
92.10	20245	104.90	1025	113.10	871	124.85	272
93.10	31869	106.05	3148	114.50	88	125.90	327

Average of 13.777 to 13.783 min.: VL040070.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.70	119	136.50	120	145.00	532	153.20	104
127.00	69	137.05	873	145.90	654	153.95	171
128.00	2223	138.70	139	146.90	229	154.40	178
128.85	1392	139.00	429	148.05	1379	155.00	1118
130.00	2557	139.50	69	149.00	444	155.20	256
130.70	293	139.80	182	149.30	55	155.70	125
131.00	857	140.10	140	149.80	279	156.80	552
132.10	116	141.05	5872	150.20	335	157.15	597
134.70	296	142.00	775	151.85	187	158.00	77
135.05	710	143.05	6149	152.30	202	158.75	318
135.70	251	143.95	255	152.80	380	159.10	421

Average of 13.777 to 13.783 min.: VL040070.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
161.00	903	176.10	435669				
169.30	53	177.15	26675				
169.65	257	178.00	884				
170.20	109	196.20	77				
171.50	161	221.40	84				
171.75	729	226.80	93				
172.20	512	246.20	57				
172.35	1127	280.60	53				
173.10	3539						
174.10	446720						
175.10	32875						