

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL010925\
 Data File : VL041867.D
 Acq On : 09 Jan 2025 16:00
 Operator : SY/MD
 Sample : VL0109ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0109ABL01

Quant Time: Jan 10 01:40:19 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL010925AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Jan 10 00:31:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.803	49	132442	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.981	114	397872	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.904	117	361279	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.393	95	290790	10.038	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL010925\
Data File : VL041867.D
Acq On : 09 Jan 2025 16:00
Operator : SY/MD
Sample : VL0109ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0109ABL01

Quant Time: Jan 10 01:40:19 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL010925AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Jan 10 00:31:30 2025
Response via : Initial Calibration




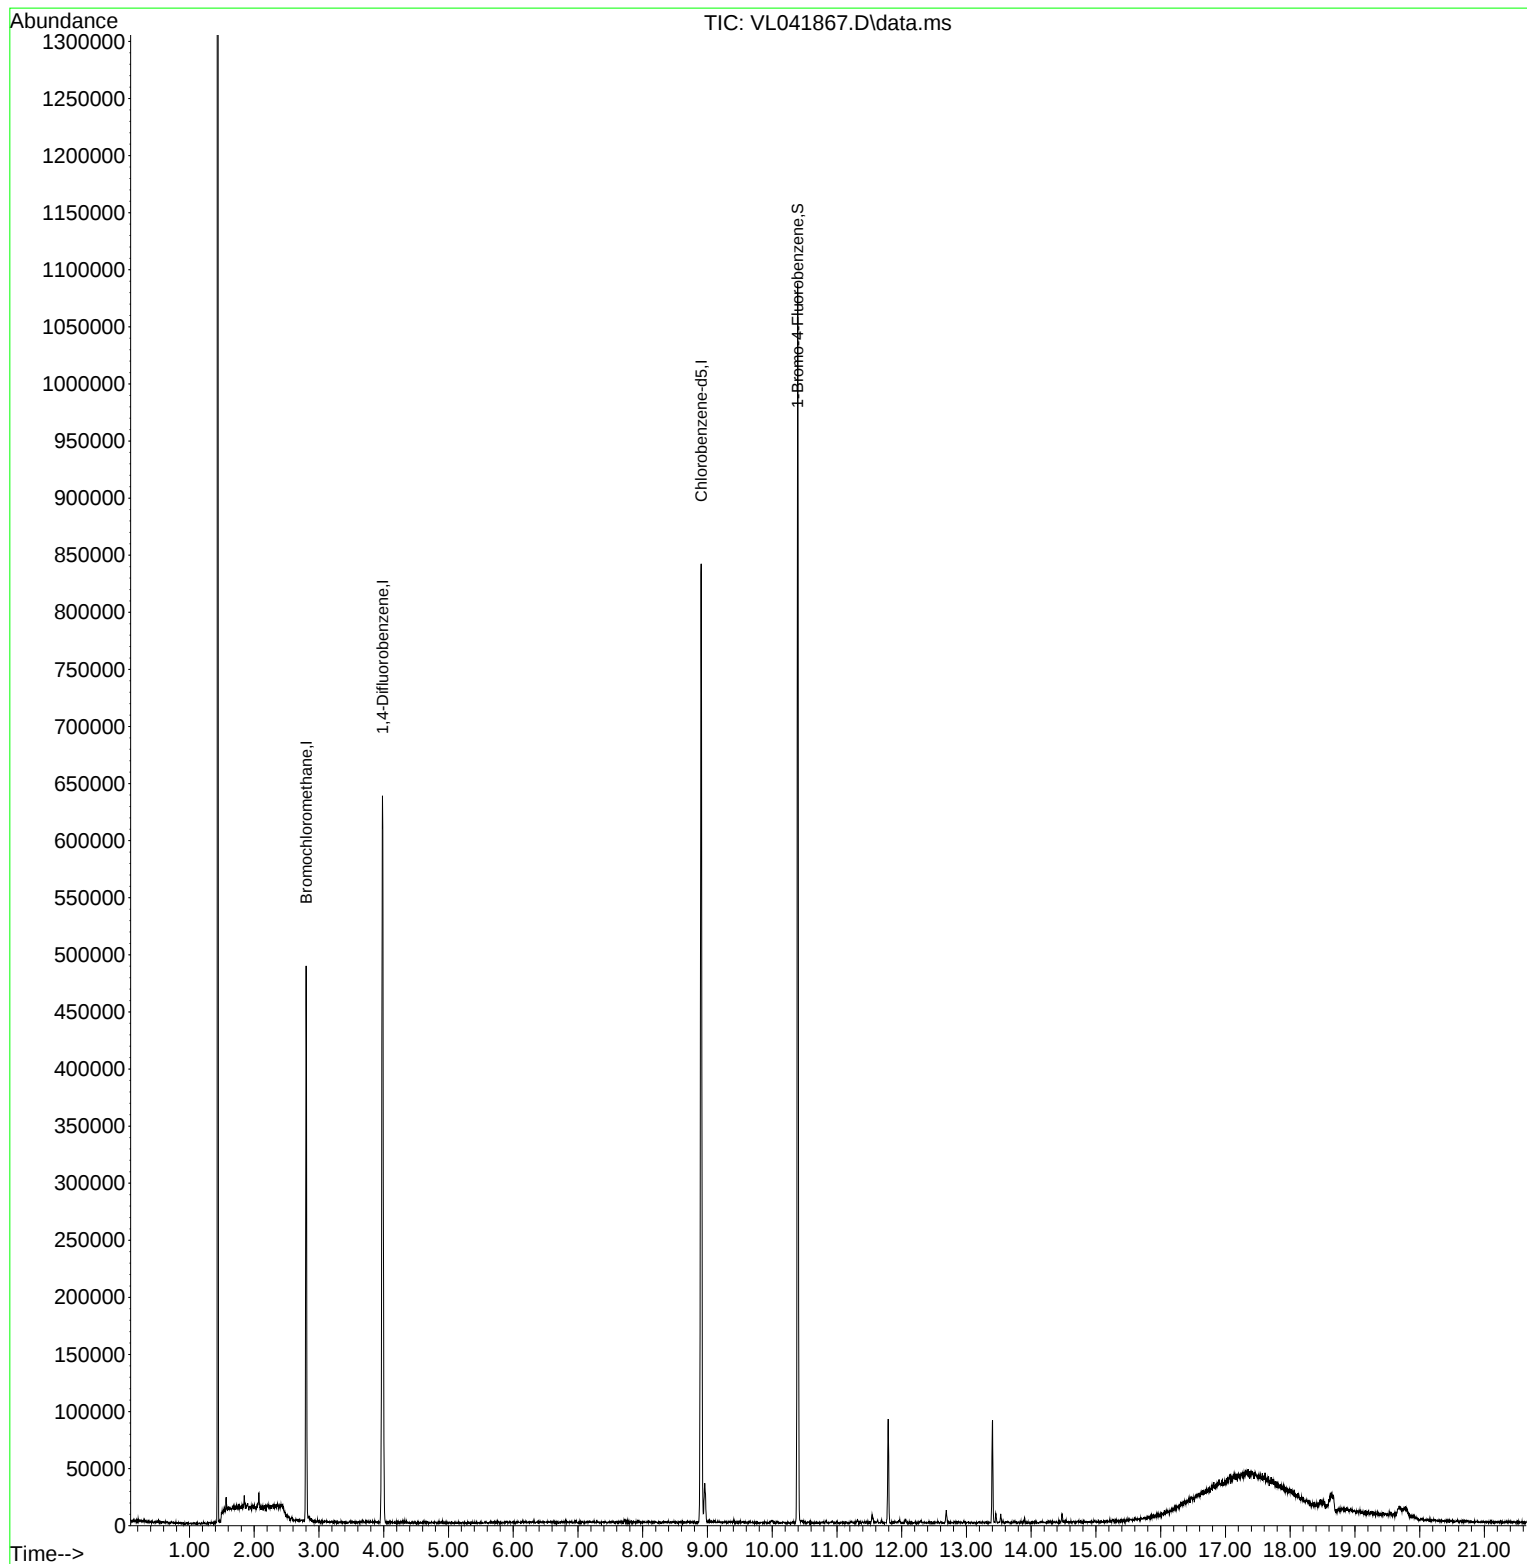


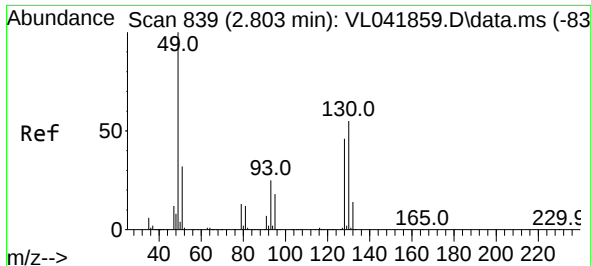

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.803 min Scan# 81
Delta R.T. 0.000 min
Lab File: VL041867.D
Acq: 09 Jan 2025 16:00




Instrument :
MSVOA_L
ClientSampleId :
VL0109ABL01


Tgt Ion: 49 Resp: 132442
Ion Ratio Lower Upper
49 100
128 48.0 23.2 69.5
130 61.1 29.9 89.8

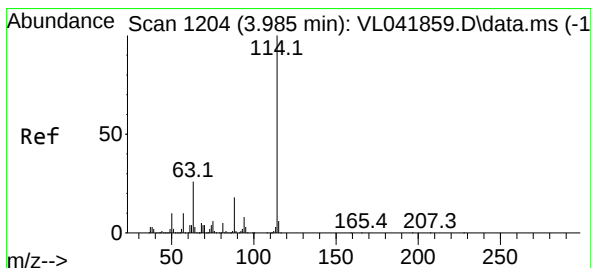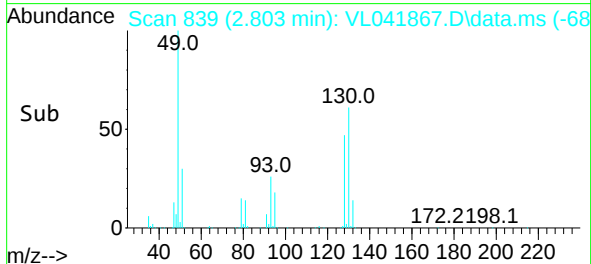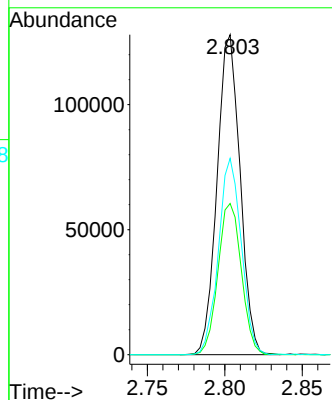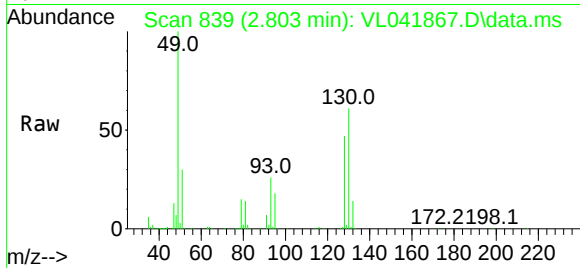

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.981 min Scan# 1203
Delta R.T. -0.003 min
Lab File: VL041867.D
Acq: 09 Jan 2025 16:00

Tgt Ion: 114 Resp: 397872
Ion Ratio Lower Upper
114 100
63 24.9 20.3 30.5
88 18.6 14.6 21.8


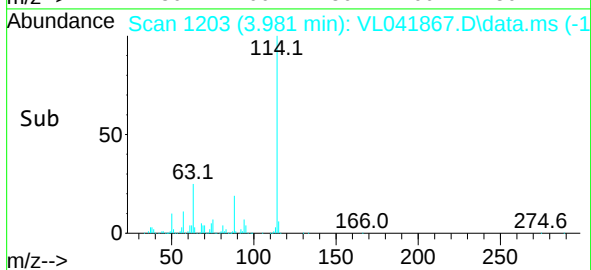
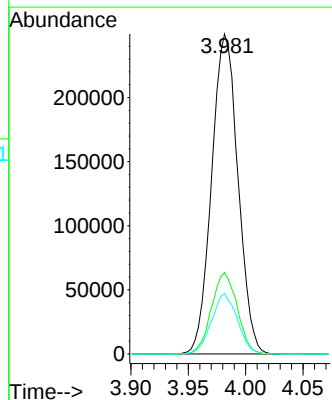
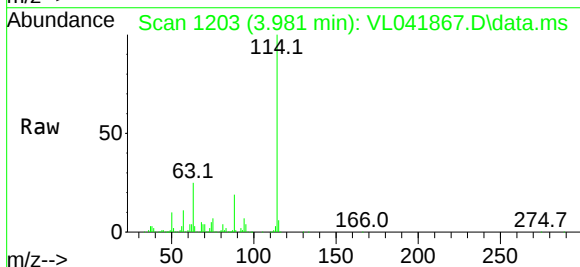


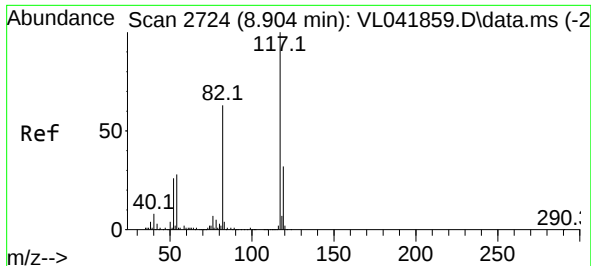

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.904 min Scan# 21
Delta R.T. 0.000 min
Lab File: VL041867.D
Acq: 09 Jan 2025 16:00

Instrument :
MSVOA_L
ClientSampleId :
VL0109ABL01

Tgt Ion:117 Resp: 361279
Ion Ratio Lower Upper
117 100
82 65.1 54.5 81.7
119 31.8 24.6 37.0

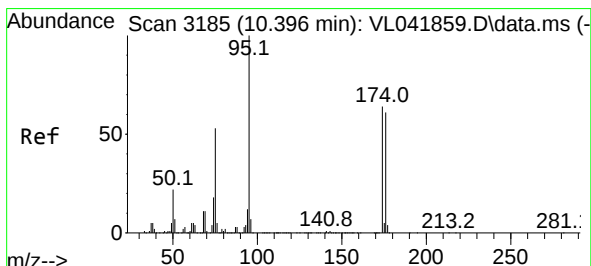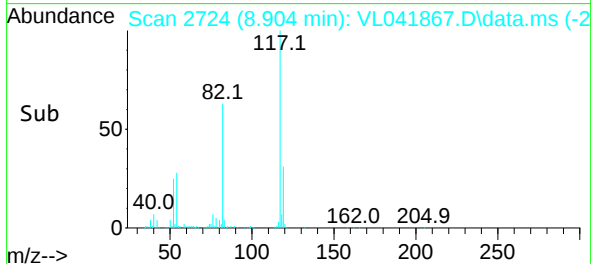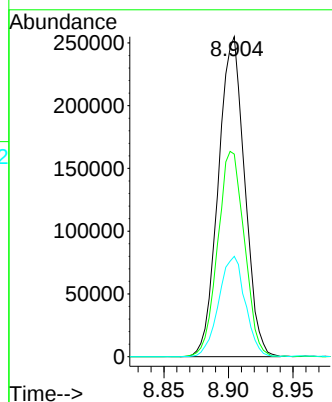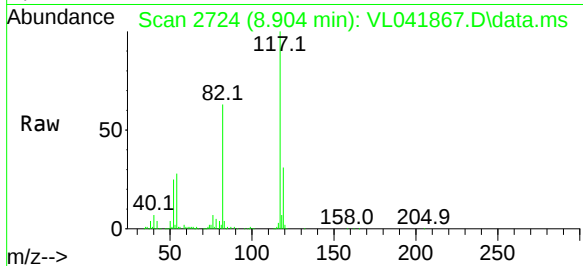

#68
1-Bromo-4-Fluorobenzene
Concen: 10.038 ppbv
RT: 10.393 min Scan# 3184
Delta R.T. -0.003 min
Lab File: VL041867.D
Acq: 09 Jan 2025 16:00

Tgt Ion: 95 Resp: 290790
Ion Ratio Lower Upper
95 100
174 62.8 51.1 76.7
175 4.8 3.8 5.8

