

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL010925\
 Data File : VL041876.D
 Acq On : 09 Jan 2025 20:46
 Operator : SY/MD
 Sample : QC010725 CAN 10601
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC010725 CAN 10601

Quant Time: Jan 10 01:48:39 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL010925AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Jan 10 00:31:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.800	49	114286	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.978	114	340666	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.898	117	300213	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.390	95	248334	10.316	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	103.200%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL010925\
Data File : VL041876.D
Acq On : 09 Jan 2025 20:46
Operator : SY/MD
Sample : QC010725 CAN 10601
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC010725 CAN 10601

Quant Time: Jan 10 01:48:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL010925AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Jan 10 00:31:30 2025
Response via : Initial Calibration




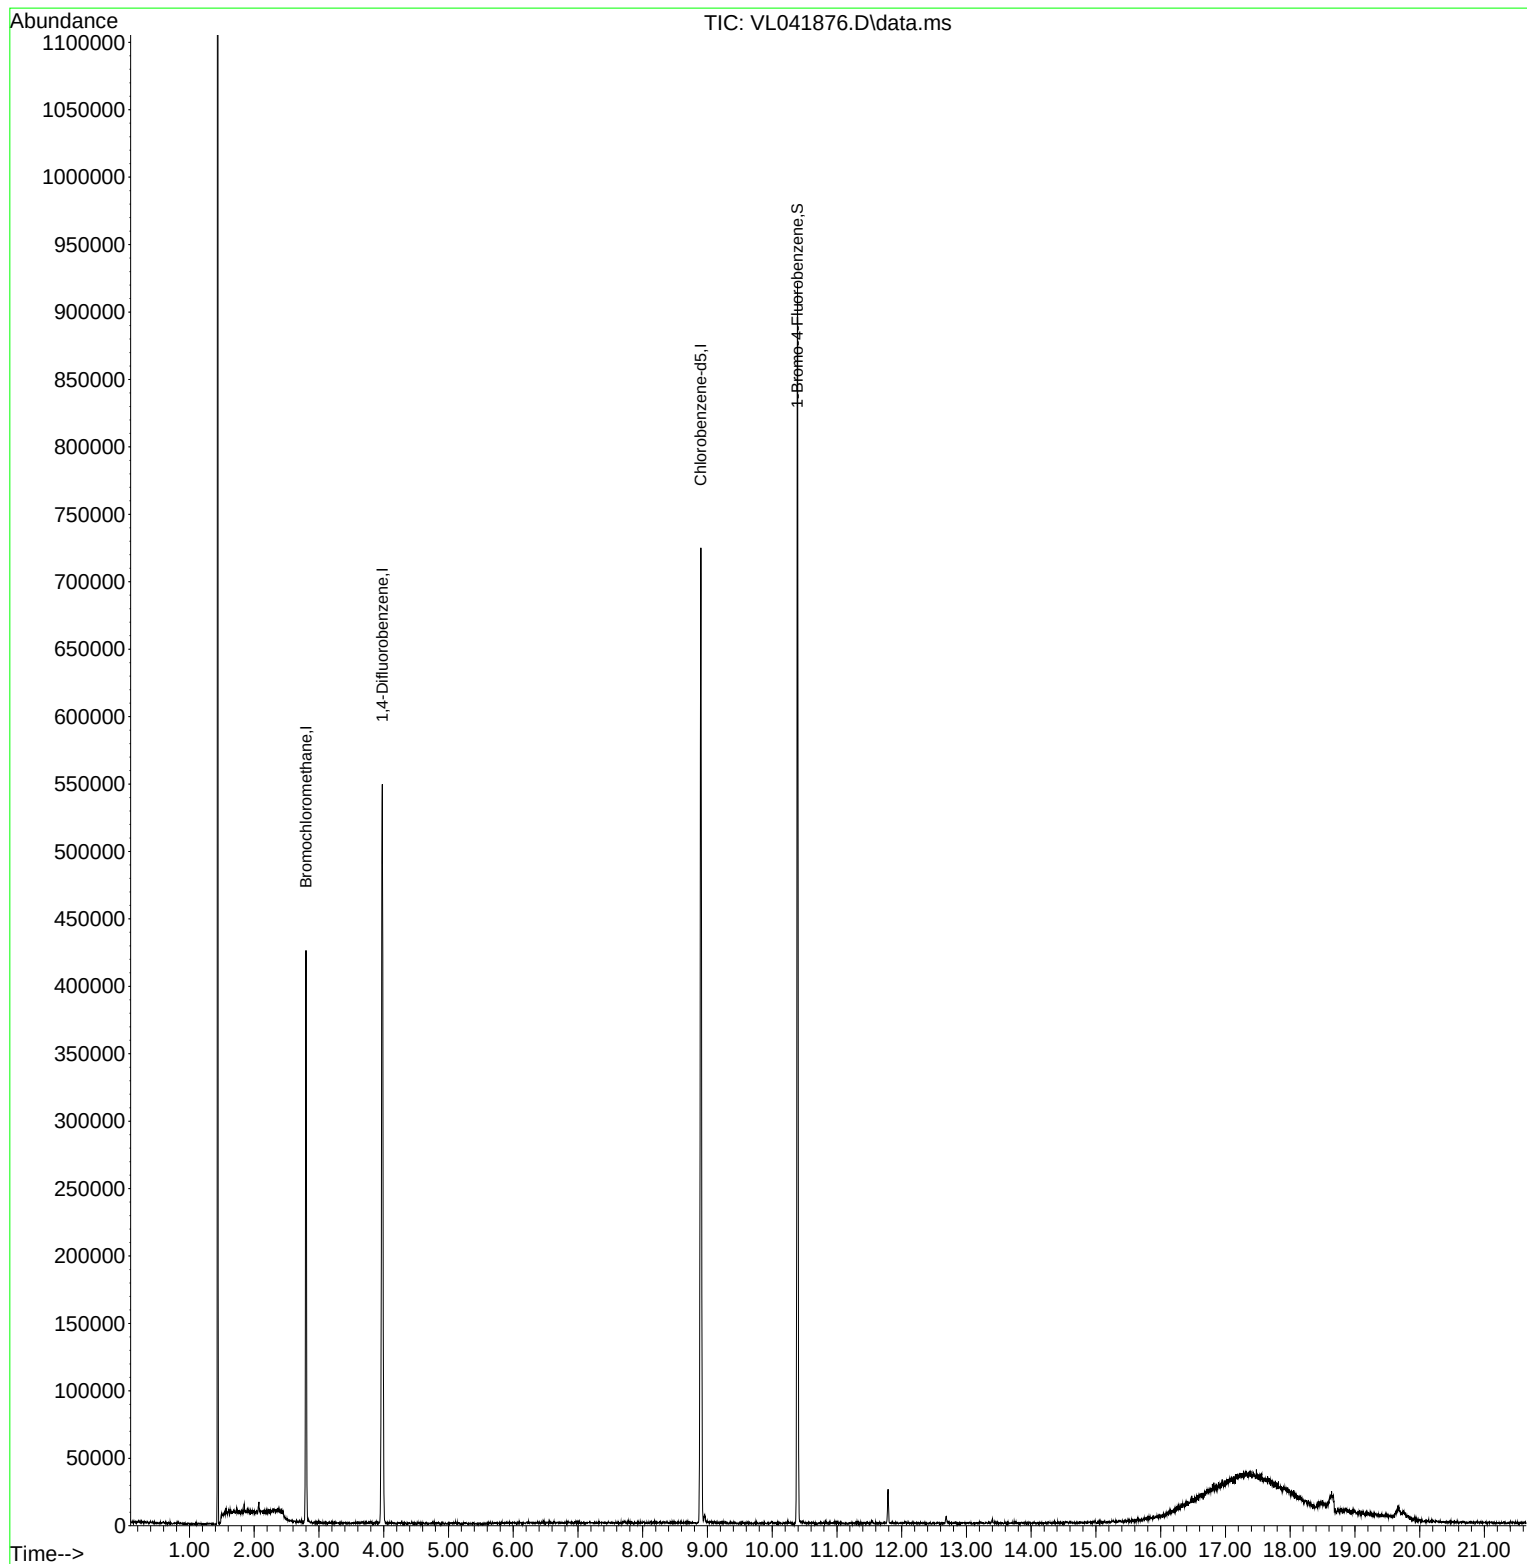


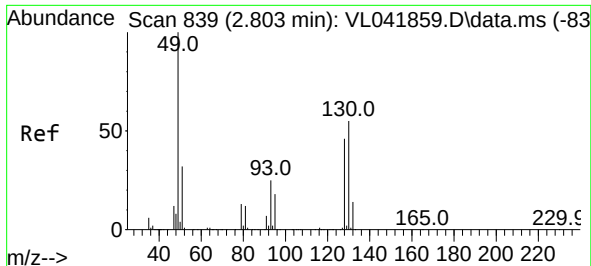

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.800 min Scan# 81
Delta R.T. -0.003 min
Lab File: VL041876.D
Acq: 09 Jan 2025 20:46




Instrument :
MSVOA_L
ClientSampleId :
QC010725 CAN 10601


Tgt Ion: 49 Resp: 114286
Ion Ratio Lower Upper
49 100
128 47.3 23.2 69.5
130 59.5 29.9 89.8

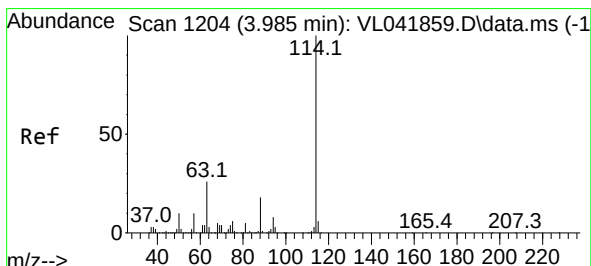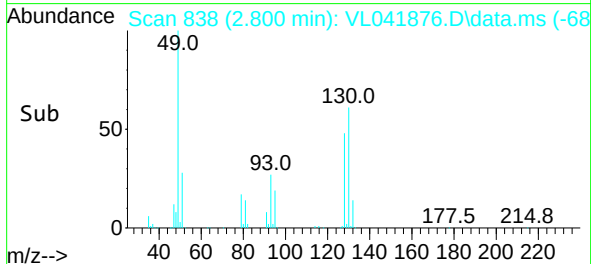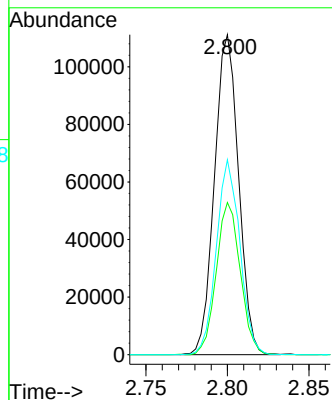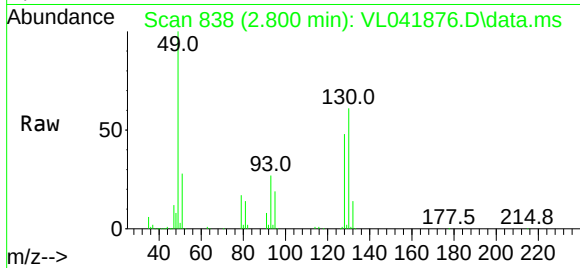

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.978 min Scan# 1202
Delta R.T. -0.007 min
Lab File: VL041876.D
Acq: 09 Jan 2025 20:46

Tgt Ion: 114 Resp: 340666
Ion Ratio Lower Upper
114 100
63 25.1 20.3 30.5
88 18.7 14.6 21.8


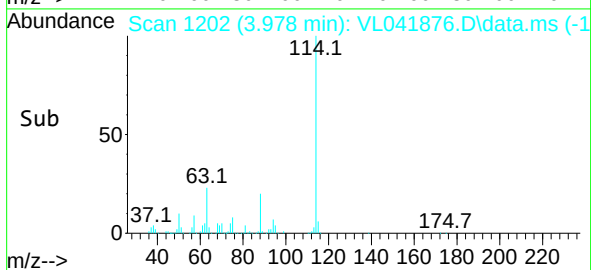
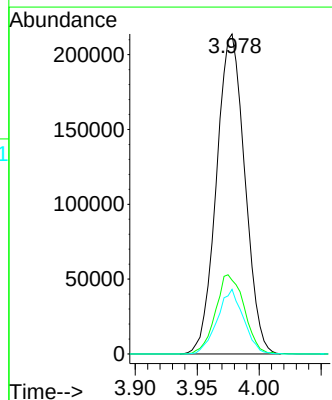
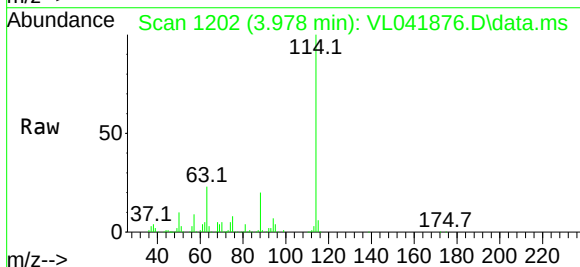


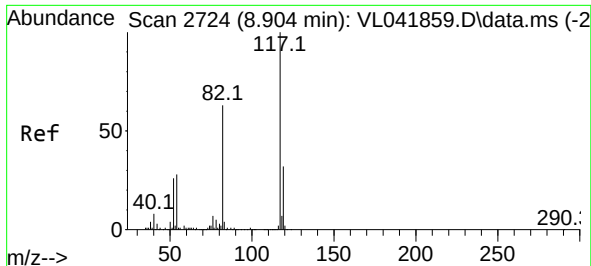

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.898 min Scan# 21
Delta R.T. -0.007 min
Lab File: VL041876.D
Acq: 09 Jan 2025 20:46

Instrument :
MSVOA_L
ClientSampleId :
QC010725 CAN 10601

Tgt Ion:117 Resp: 300213
Ion Ratio Lower Upper
117 100
82 66.4 54.5 81.7
119 32.4 24.6 37.0

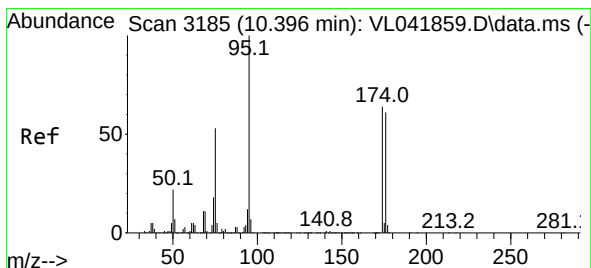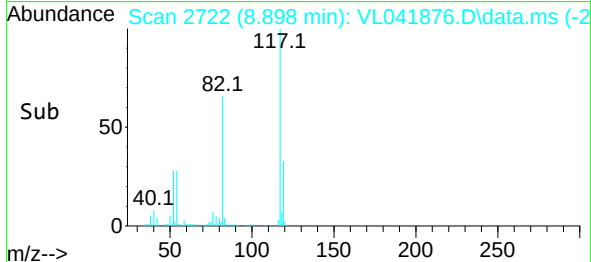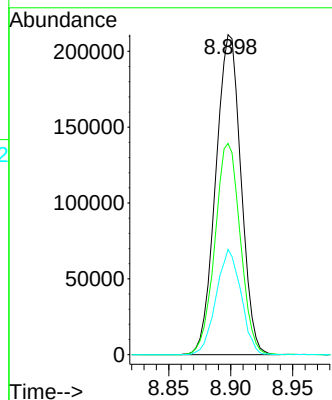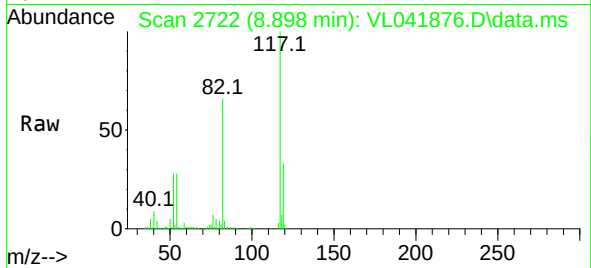

#68
1-Bromo-4-Fluorobenzene
Concen: 10.316 ppbv
RT: 10.390 min Scan# 3183
Delta R.T. -0.007 min
Lab File: VL041876.D
Acq: 09 Jan 2025 20:46

Tgt Ion: 95 Resp: 248334
Ion Ratio Lower Upper
95 100
174 61.5 51.1 76.7
175 4.7 3.8 5.8

