
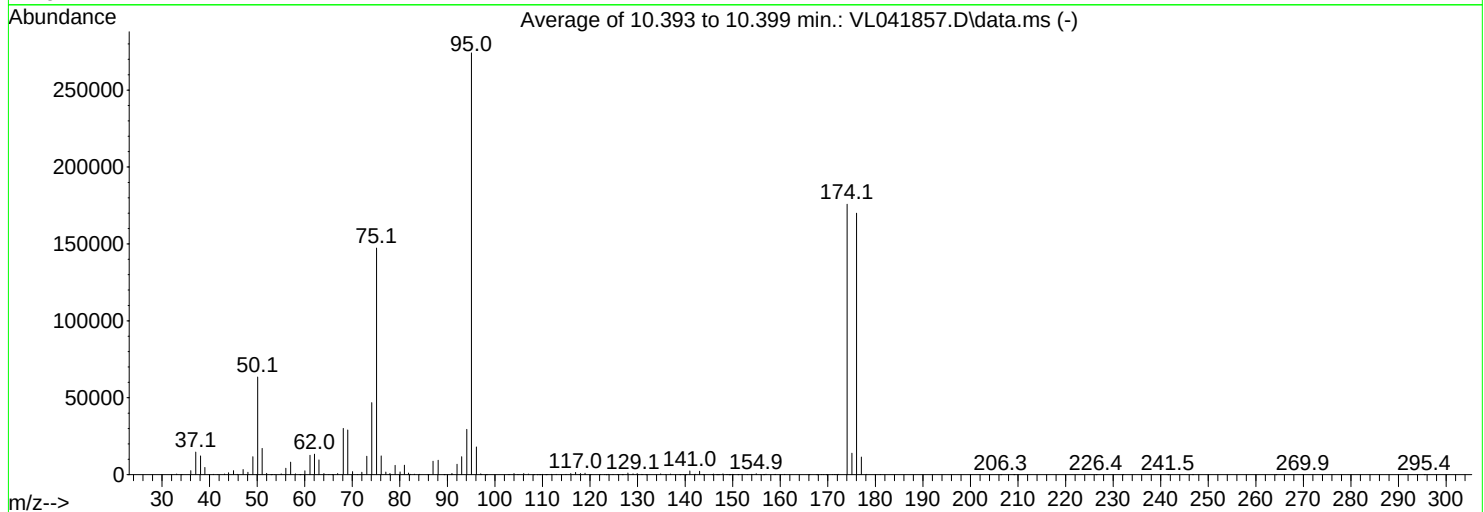


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL010925\
Data File : VL041857.D
Acq On : 09 Jan 2025 09:48
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL010925AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Jan 10 00:31:30 2025

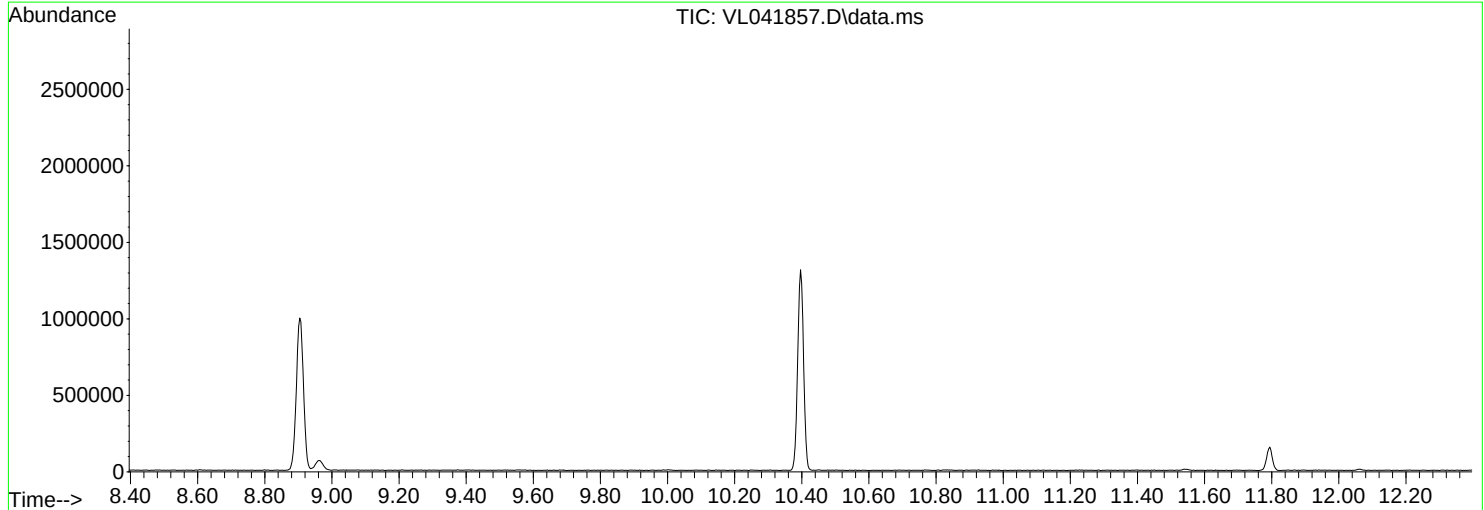

AutoFind: Scans 3184, 3185, 3186; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.1	63467	PASS
75	95	30	66	53.7	147285	PASS
95	95	100	100	100.0	274227	PASS
96	95	5	9	6.6	18052	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	64.1	175765	PASS
175	174	4	9	7.9	13949	PASS
176	174	93	101	96.7	170005	PASS
177	176	5	9	6.7	11408	PASS

Average of 10.393 to 10.399 min.: VL041857.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	413	45.85	187	56.05	4190	66.95	691
34.00	44	47.05	3379	57.05	8084	68.10	3006
36.05	2643	48.05	1579	58.05	496	69.05	2898
37.10	14662	49.10	11700	59.00	52	70.05	196
38.10	12187	50.10	63467	60.05	2526	71.10	141
39.00	4725	51.05	17058	61.10	12614	72.00	1581
40.80	175	52.00	857	62.05	13340	73.05	11942
41.75	153	52.90	26	63.00	9583	74.10	46781
43.15	470	53.20	122	64.05	742	75.10	147285
44.00	1297	53.70	64	65.10	71	76.10	12201
45.05	2561	55.05	522	65.80	36	77.05	1664

Average of 10.393 to 10.399 min.: VL041857.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.80	299	87.00	8731	97.20	220	109.40	26
77.95	778	88.05	9358	98.20	40	110.00	188
79.00	6026	89.30	19	102.80	69	110.70	49
80.05	1743	90.90	387	103.10	83	111.10	142
80.95	6206	91.00	605	104.00	782	111.90	264
81.85	1032	92.05	6806	104.80	75	112.90	249
82.20	250	93.00	11619	105.05	82	114.95	160
83.05	339	94.10	29451	106.05	759	115.95	711
84.15	208	95.05	274227	107.05	389	116.95	1408
85.90	21	96.10	18052	108.10	23	117.80	144
86.10	114	97.00	480	108.90	34	118.00	719

Average of 10.393 to 10.399 min.: VL041857.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	927	129.05	569	140.10	41	148.90	107
120.00	18	129.90	745	141.00	2372	149.20	38
122.15	95	130.10	100	142.10	314	149.40	37
123.10	117	130.90	224	143.05	2180	150.00	175
123.40	52	131.10	102	143.80	21	150.20	79
123.90	207	131.75	43	145.70	54	151.10	30
124.85	102	134.85	501	145.95	415	151.95	202
125.80	69	135.90	71	146.65	56	153.05	98
126.05	120	136.95	451	147.00	31	154.00	269
126.80	25	138.90	47	147.95	490	154.95	626
127.95	992	139.65	129	148.65	108	155.90	158

Average of 10.393 to 10.399 min.: VL041857.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.50	44	171.40	83	209.10	29		
157.00	338	171.70	85	226.40	18		
158.70	100	172.00	129	232.00	19		
159.00	253	172.20	183	241.50	47		
160.95	227	174.05	175765	246.70	29		
166.00	22	175.05	13949	264.20	27		
167.70	49	176.05	170005	269.90	64		
168.70	67	177.05	11408	295.40	18		
169.15	66	178.10	236				
169.70	29	181.05	73				
170.95	142	206.35	56				