


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL011321\
 Data File : VL036209.D
 Acq On : 13 Jan 2021 1:17
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL011321AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Jan 14 16:13:38 2021
 Last Update : Thu Jan 14 16:13:38 2021

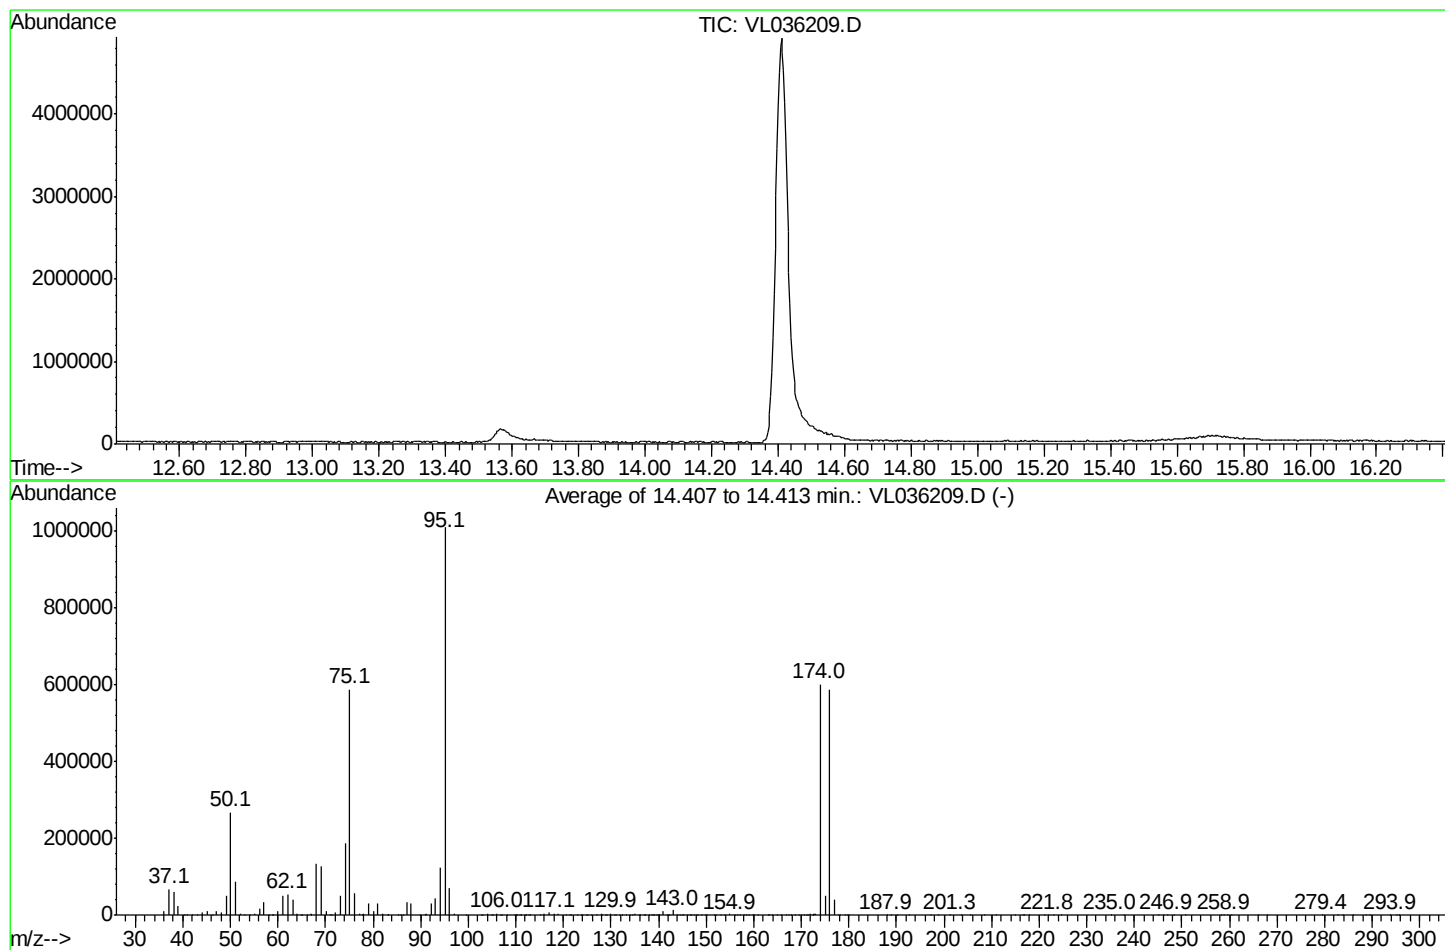

AutoFind: Scans 3614, 3615, 3616; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.6	268480	PASS
75	95	30	66	58.1	587242	PASS
95	95	100	100	100.0	1010154	PASS
96	95	5	9	7.0	70328	PASS
173	174	0.00	2	0.5	3172	PASS
174	95	50	120	59.5	601109	PASS
175	174	4	9	8.2	49570	PASS
176	174	93	101	97.5	585962	PASS
177	176	5	9	6.9	40213	PASS