

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011524\
 Data File : VL040967.D
 Acq On : 15 Jan 2024 12:58
 Operator : SY/MD
 Sample : QC010324 CAN 10329
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC010324 CAN 10329

Quant Time: Jan 16 03:34:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL122023AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Jan 16 03:31:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.182	49	1092460	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.639	114	3150291	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.445	117	2639742	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.754	95	1941745	9.986	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011524\
Data File : VL040967.D
Acq On : 15 Jan 2024 12:58
Operator : SY/MD
Sample : QC010324 CAN 10329
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC010324 CAN 10329


Quant Time: Jan 16 03:34:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL122023AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Jan 16 03:31:29 2024
Response via : Initial Calibration

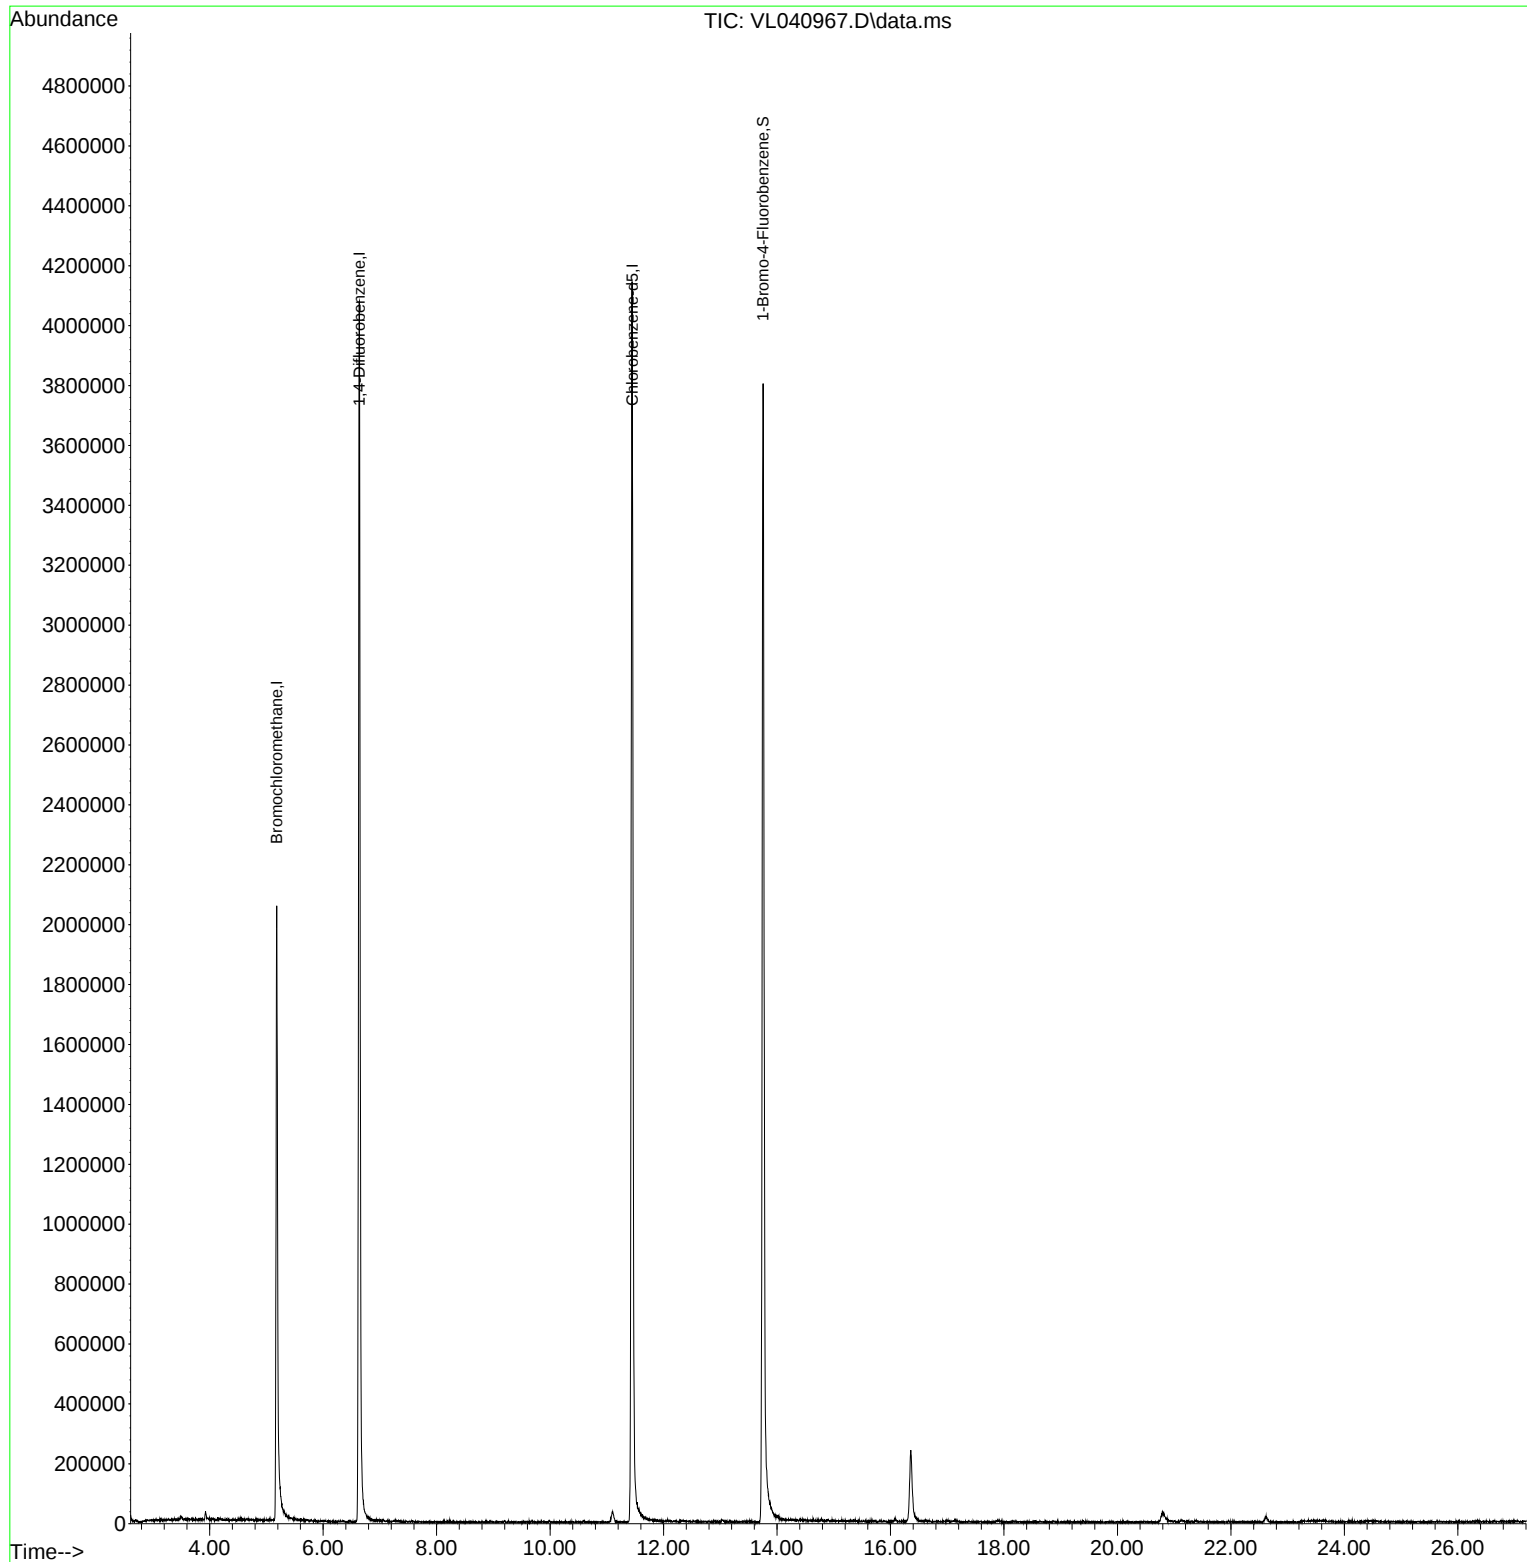



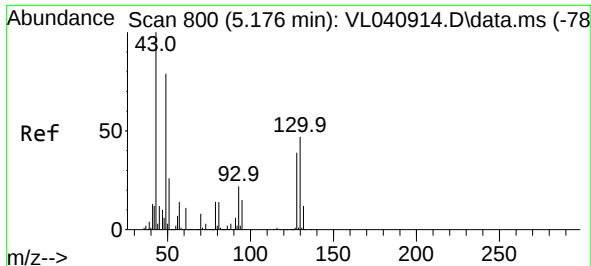


#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.182 min Scan# 80
Delta R.T. 0.006 min
Lab File: VL040967.D
Acq: 15 Jan 2024 12:58


Instrument :
MSVOA_L
ClientSampleId :
QC010324 CAN 10329

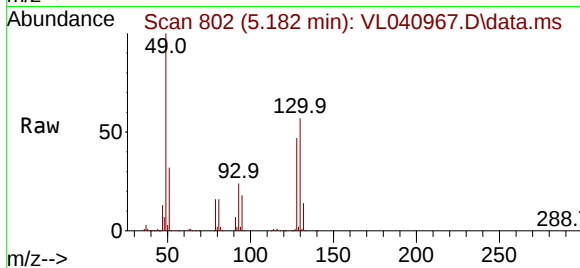



Tgt Ion: 49 Resp: 1092460
Ion Ratio Lower Upper
49 100
128 48.1 23.8 71.2
130 60.6 30.1 90.5

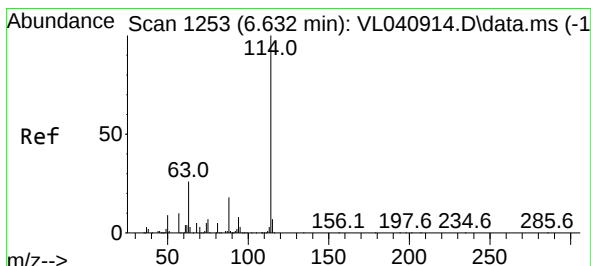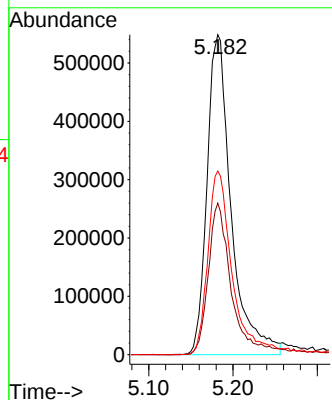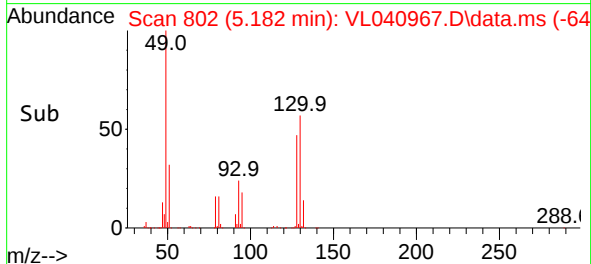


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.639 min Scan# 1255
Delta R.T. 0.003 min
Lab File: VL040967.D
Acq: 15 Jan 2024 12:58

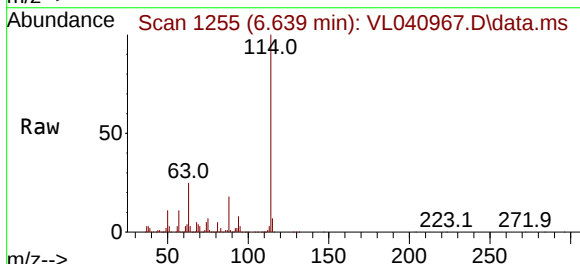

Tgt Ion: 114 Resp: 3150291
Ion Ratio Lower Upper
114 100
63 25.5 21.0 31.6
88 18.3 14.3 21.5



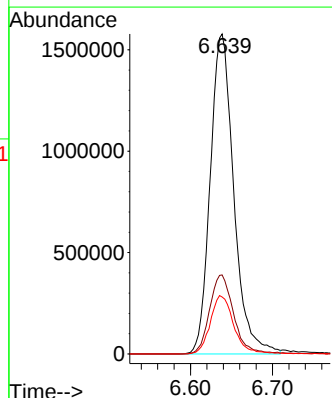
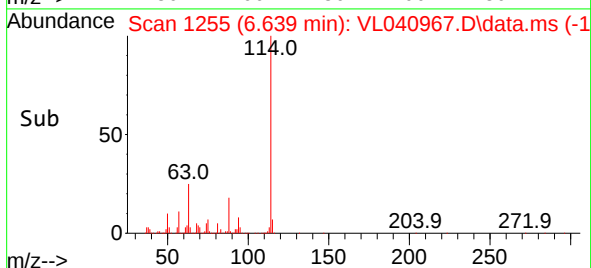


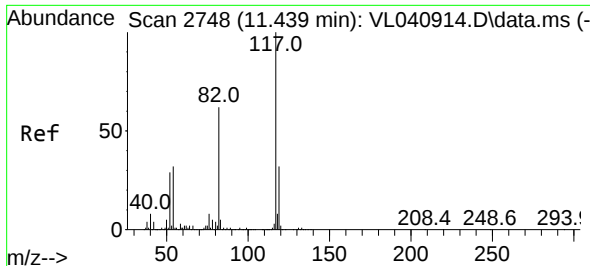

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.445 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL040967.D
Acq: 15 Jan 2024 12:58

Instrument :
MSVOA_L
ClientSampleId :
QC010324 CAN 10329

Tgt Ion:117 Resp: 2639742
Ion Ratio Lower Upper
117 100
82 67.6 49.6 74.4
119 33.6 23.4 35.0

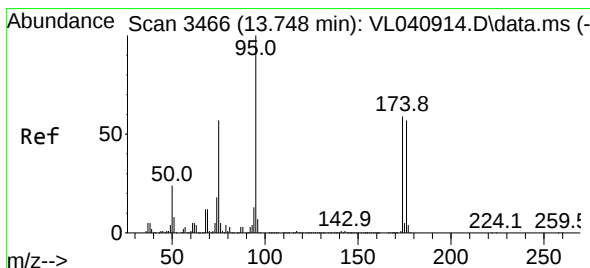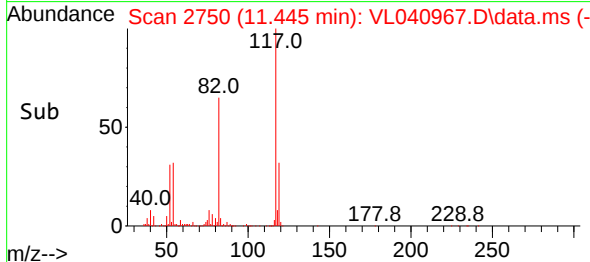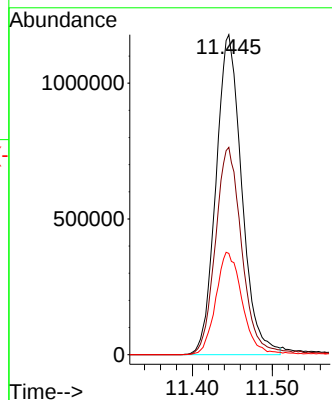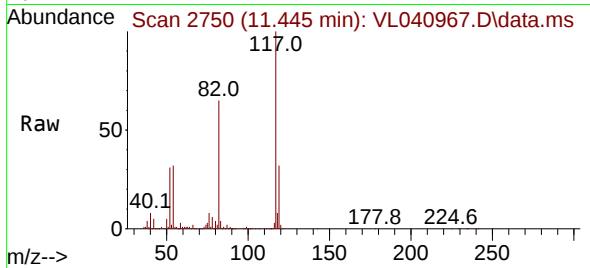

#68
1-Bromo-4-Fluorobenzene
Concen: 9.986 ppbv
RT: 13.754 min Scan# 3468
Delta R.T. -0.000 min
Lab File: VL040967.D
Acq: 15 Jan 2024 12:58

Tgt Ion: 95 Resp: 1941745
Ion Ratio Lower Upper
95 100
174 62.2 48.0 72.0
175 4.6 3.7 5.5

