
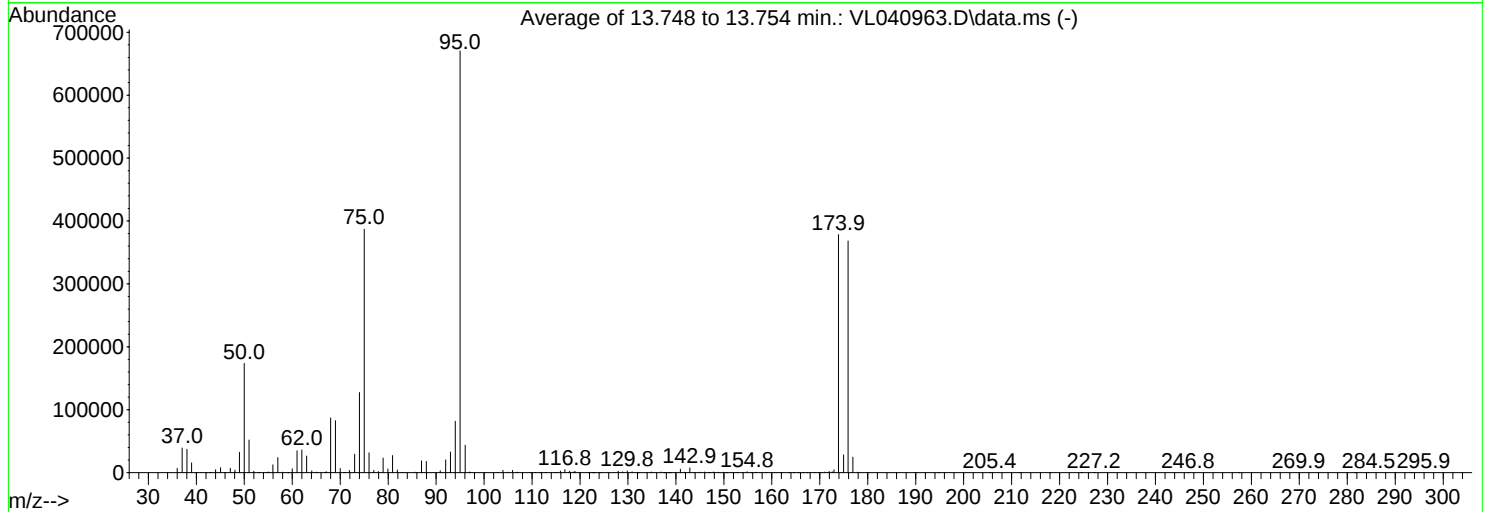


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011524\
Data File : VL040963.D
Acq On : 15 Jan 2024 8:16
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL122023AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Jan 16 03:31:29 2024

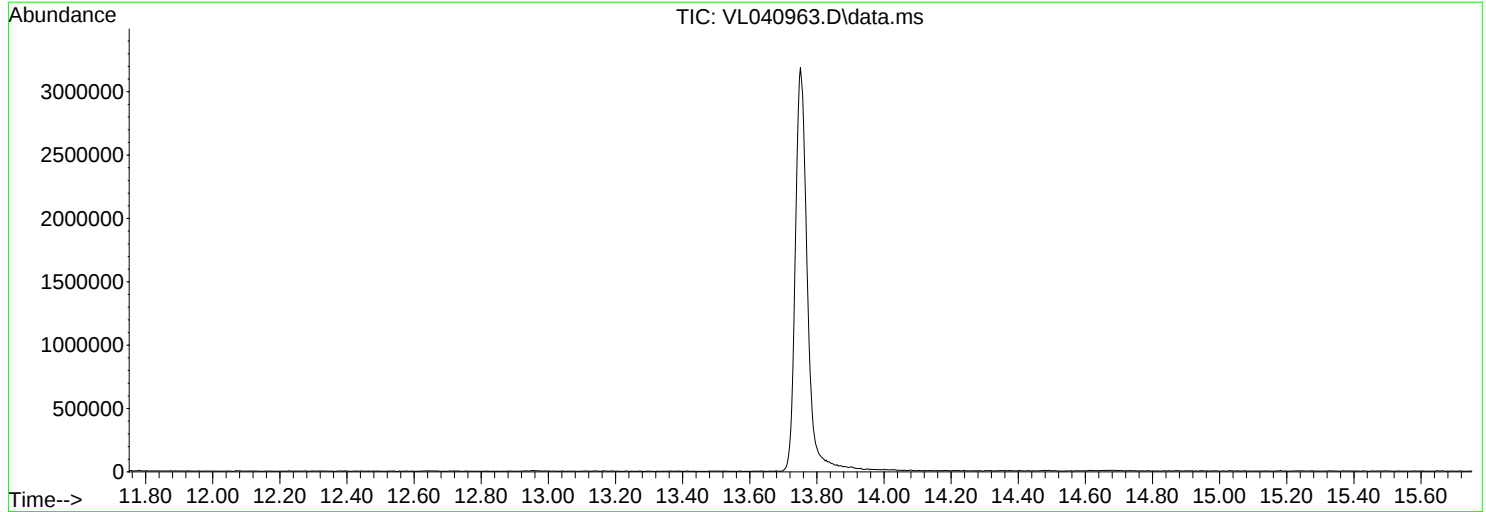

AutoFind: Scans 3466, 3467, 3468; Background Corrected with Scan 3444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.9	173611	PASS
75	95	30	66	57.7	387157	PASS
95	95	100	100	100.0	670443	PASS
96	95	5	9	6.5	43635	PASS
173	174	0.00	2	1.2	4494	PASS
174	95	50	120	56.4	378389	PASS
175	174	4	9	7.5	28331	PASS
176	174	93	101	97.3	368213	PASS
177	176	5	9	6.7	24797	PASS

Average of 13.748 to 13.754 min.: VL040963.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	6956	45.85	300	55.95	12602	66.90	761
37.05	39248	46.10	194	57.00	23877	67.15	127
38.05	37136	47.10	6781	57.95	923	68.00	8701
39.00	15511	48.05	4069	59.10	64	69.00	8281
39.95	322	49.00	32411	60.00	6120	70.00	6723
41.05	275	50.00	173611	61.00	34896	70.80	165
42.00	53	51.00	51964	62.00	36149	71.05	421
42.80	133	52.00	2319	63.00	26549	71.90	3496
43.05	536	52.95	144	64.05	2861	73.00	29269
44.00	4616	54.80	551	65.00	239	74.00	127331
45.05	7850	55.10	1095	65.15	712	75.00	387157

Average of 13.748 to 13.754 min.: VL040963.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.00	31635	86.95	18760	103.95	3779	113.00	505
77.00	3608	87.95	17881	104.95	801	114.60	288
77.95	1917	90.85	3097	105.95	3595	114.90	294
78.95	23115	92.00	20368	106.70	321	115.15	413
79.95	6008	93.00	32808	107.00	692	115.90	2498
80.90	27152	94.00	81755	109.70	321	116.85	4882
81.90	4311	95.00	670443	109.90	65	117.60	469
82.80	409	96.05	43635	110.75	613	117.85	2367
83.20	169	96.95	1132	111.70	127	118.70	1064
85.60	864	97.20	442	111.95	581	118.95	2097
86.05	303	102.85	397	112.80	399	119.80	113

Average of 13.748 to 13.754 min.: VL040963.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
121.80	63	129.85	2467	138.80	93	148.10	468
122.20	233	130.85	1332	139.85	656	148.90	611
122.60	111	132.10	96	140.95	5458	149.90	755
122.95	153	133.80	373	141.80	819	150.60	113
123.85	421	134.80	342	142.90	7606	151.65	174
124.10	129	134.95	1126	143.75	339	152.70	334
124.80	246	135.60	160	144.90	849	152.95	603
125.85	273	136.85	1126	145.95	1056	153.90	422
127.05	351	137.50	58	146.80	315	154.85	1576
127.95	2513	137.95	105	147.00	77	155.70	149
128.85	1345	138.50	133	147.85	960	156.00	311

Average of 13.748 to 13.754 min.: VL040963.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.60	368	166.50	55	172.95	4494	227.20	96
156.80	576	167.30	141	173.90	378389	246.80	58
157.75	215	168.00	410	174.95	28331	257.40	53
158.75	607	168.95	493	175.90	368213	269.90	89
159.00	353	169.80	392	176.90	24797	281.60	68
160.60	210	170.00	204	177.90	724	284.50	271
160.90	400	170.45	314	194.80	113	293.30	53
161.90	91	171.05	1037	205.45	134	295.95	205
163.50	65	171.60	313	211.70	75		
164.60	88	171.95	1753	218.00	78		
165.50	51	172.60	1263	224.50	65		