

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL011619\
Quantitation Report (Not Reviewed)

Data File : VL033091.D
Acq On : 16 Jan 2019 14:17
Operator : SY/AP
Sample : QC010919 CAN 10295
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC010919 CAN 10295

Quant Time: Jan 17 01:52:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL010419AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jan 04 16:09:05 2019
QLast Update : Fri Jan 04 16:09:05 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.75	49	1033470	10.00	ppbv	-0.01
33) 1,4-Difluorobenzene	7.28	114	2485666	10.00	ppbv	-0.02
55) Chlorobenzene-d5	12.24	117	2310251	10.00	ppbv	-0.01

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.57	95	1807661	10.21	ppbv	-0.01
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.10%


Target Compounds						Qvalue
4) Chloromethane	3.17	50	4372	0.065	ppbv	93
20) Methylene Chloride	4.40	84	2668	0.045	ppbv #	83
30) Cyclohexane	7.27	84	5581	0.066	ppbv #	1
39) 1,2-Dichloropropane	7.28	63	620339	8.110	ppbv #	23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VL033091.D
Acq On : 16 Jan 2019 14:17
Operator : SY/AP
Sample : QC010919 CAN 10295
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC010919 CAN 10295

Quant Time: Jan 17 01:52:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL010419AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jan 04 16:09:05 2019
QLast Update : Fri Jan 04 16:09:05 2019
Response via : Initial Calibration

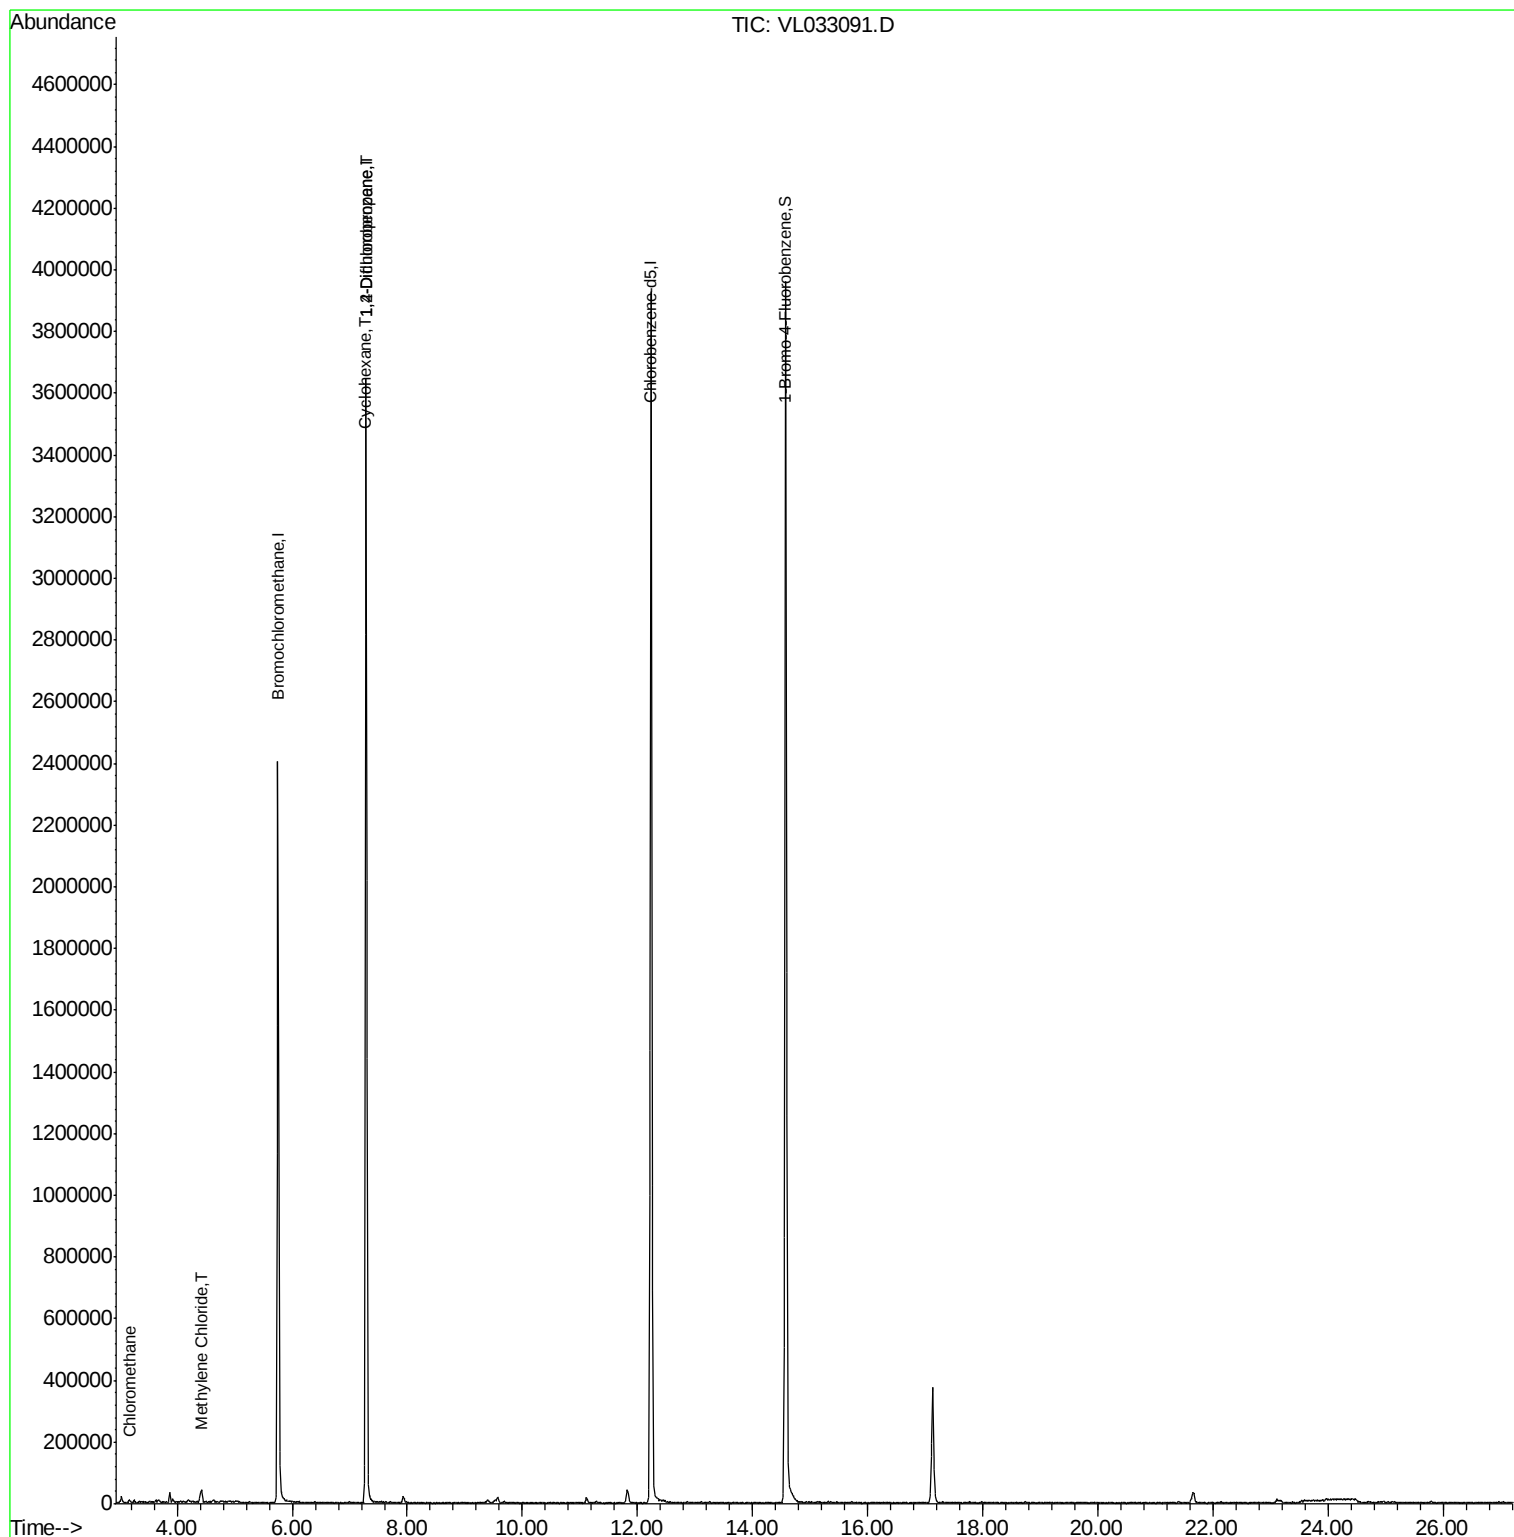

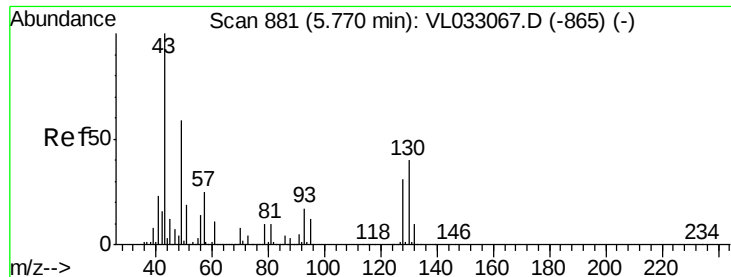

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.75 min Scan# 876

Delta R.T. -0.01 min

Lab File: VL033091.D

Acq: 16 Jan 2019 14:17

Instrument :

MSVOA_L

ClientSampleId :

QC010919 CAN 10295


Tgt Ion: 49 Resp: 1033470

Ion Ratio Lower Upper

49 100

128 53.3 26.2 78.5




130 67.0 33.6 100.6

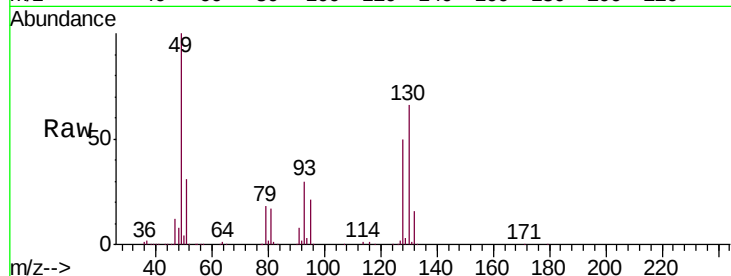

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

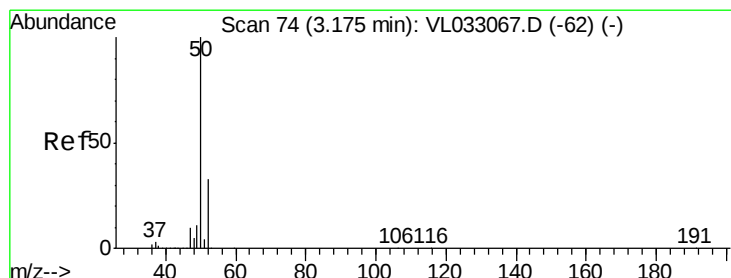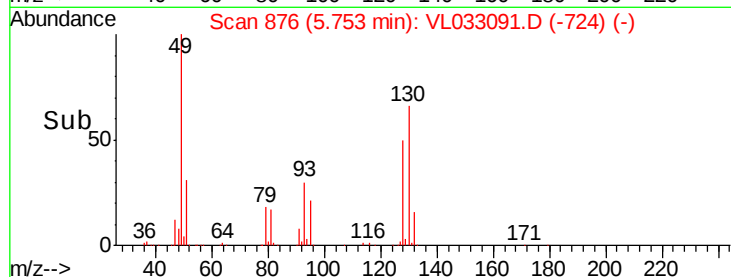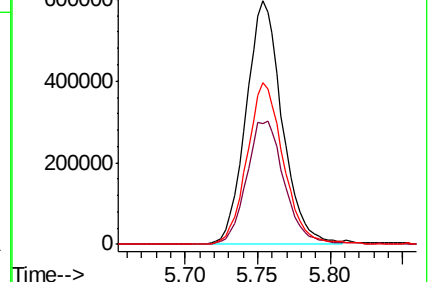

#4

Chloromethane

Concen: 0.065 ppbv

RT: 3.17 min Scan# 71

Delta R.T. -0.01 min

Lab File: VL033091.D


Acq: 16 Jan 2019 14:17

Tgt Ion: 50 Resp: 4372

Ion Ratio Lower Upper



50 100


52 29.7 26.9 40.3

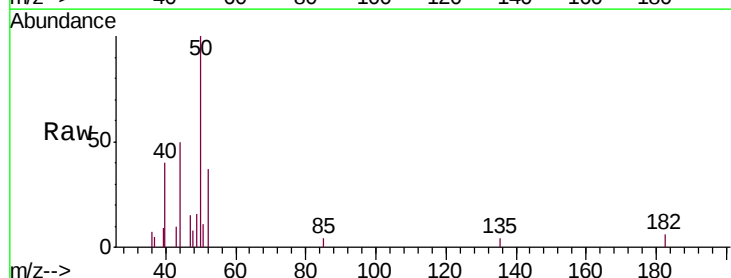

Abundance Ion 50.10 (49.80 to 50.80): VL0

Ion 52.10 (51.80 to 52.80): VL0



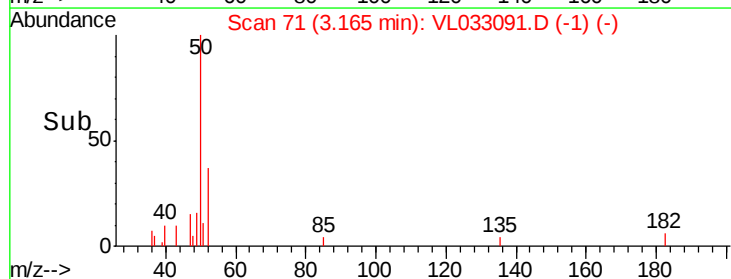
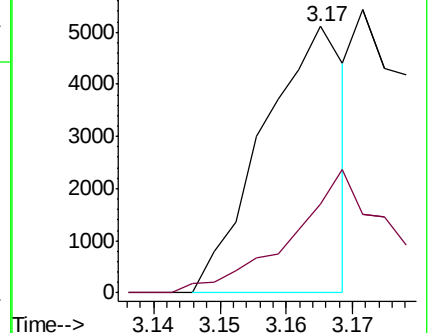


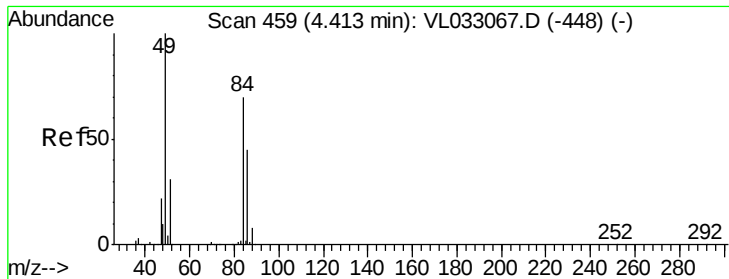

#20
Methylene Chloride
Concen: 0.045 ppbv
RT: 4.40 min Scan# 455
Delta R.T. -0.01 min
Lab File: VL033091.D
Acq: 16 Jan 2019 14:17




Instrument :
MSVOA_L
ClientSampleId :
QC010919 CAN 10295


Tgt Ion: 84 Resp: 2668
Ion Ratio Lower Upper
84 100
49 131.2 115.8 173.6
51 37.2 35.7 53.5
86 34.7 49.7 74.5#

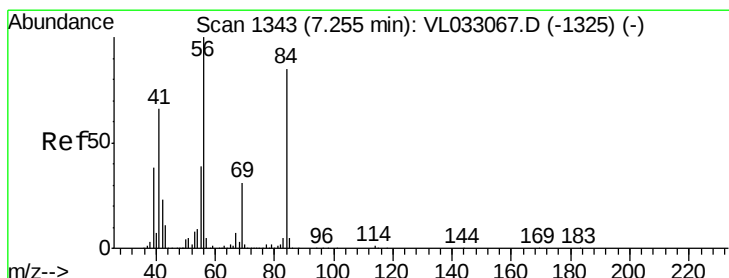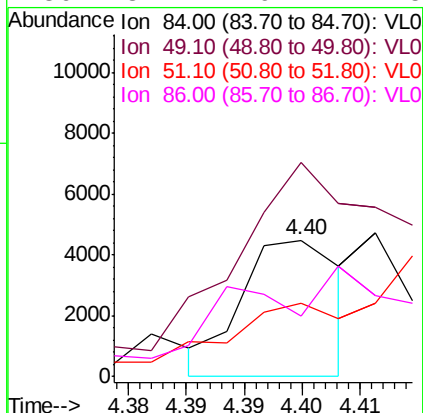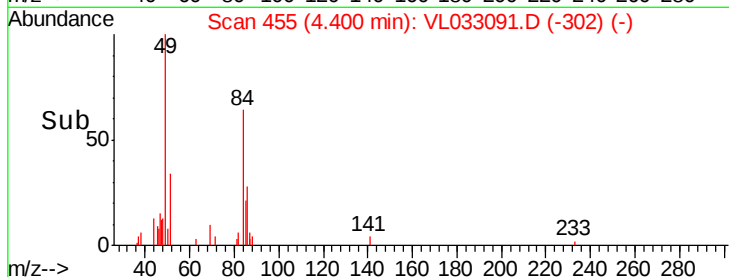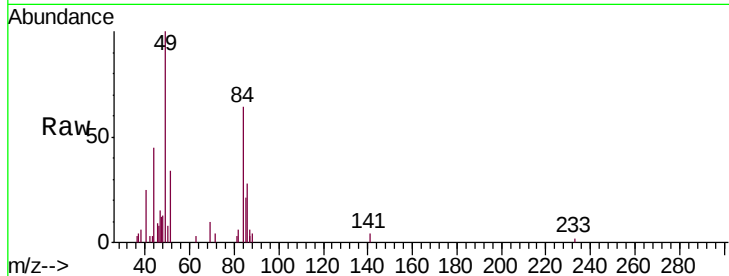

#30
Cyclohexane
Concen: 0.066 ppbv
RT: 7.27 min Scan# 1347
Delta R.T. 0.02 min
Lab File: VL033091.D
Acq: 16 Jan 2019 14:17

Tgt Ion: 84 Resp: 5581
Ion Ratio Lower Upper
84 100
56 0.0 101.8 152.6#
41 8.6 63.2 94.8#

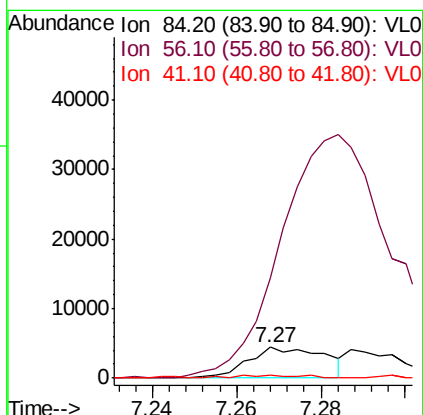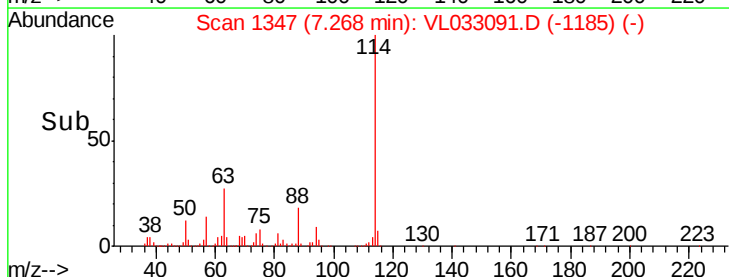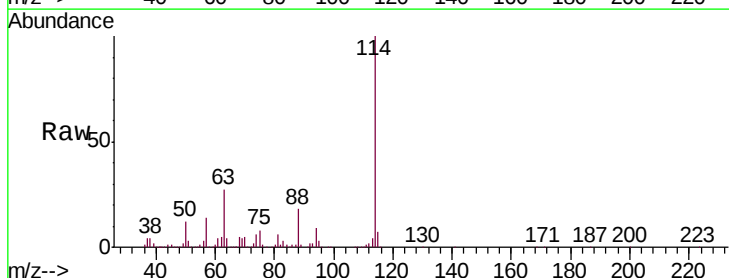

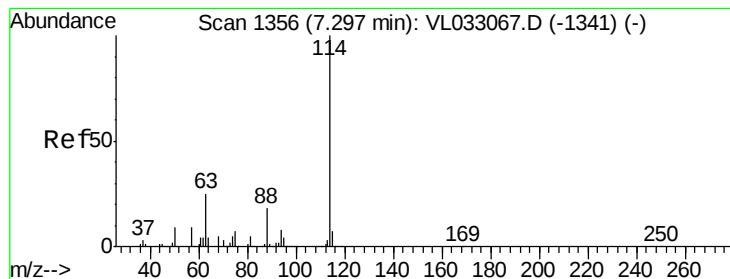

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.28 min Scan# 1351

Delta R.T. -0.02 min

Lab File: VL033091.D

Acq: 16 Jan 2019 14:17

Instrument :

MSVOA_L

ClientSampleId :

QC010919 CAN 10295


Tgt Ion:114 Resp: 2485666

Ion Ratio Lower Upper

114 100

63 25.2 20.1 30.1




88 17.9 14.0 21.0

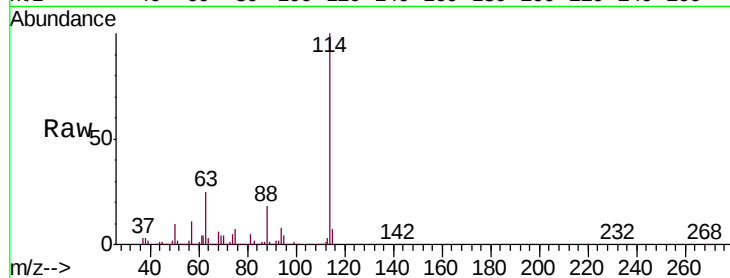

Abundance Ion 114.10 (113.80 to 114.80): V

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

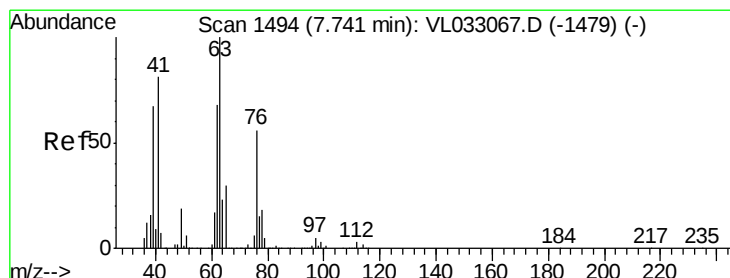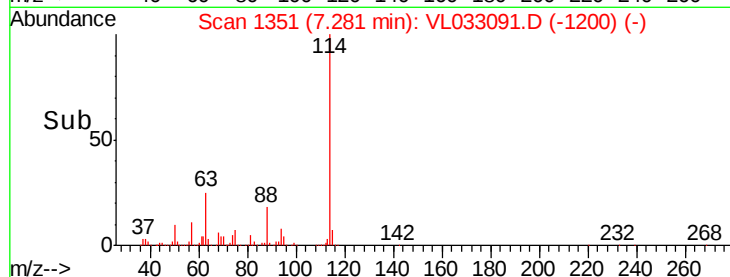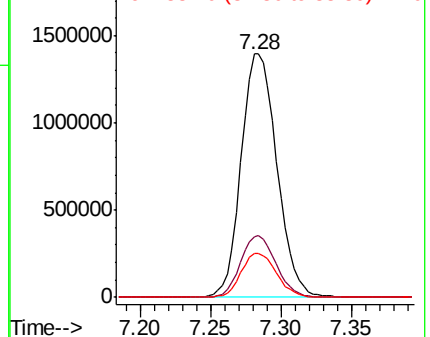

#39

1,2-Dichloropropane

Concen: 8.110 ppbv

RT: 7.28 min Scan# 1352

Delta R.T. -0.46 min

Lab File: VL033091.D

Acq: 16 Jan 2019 14:17


Tgt Ion: 63 Resp: 620339

Ion Ratio Lower Upper

63 100

41 0.0 61.9 92.9#



62 18.6 55.8 83.6#

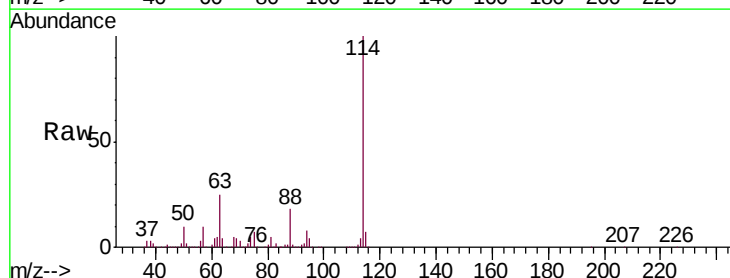


Abundance Ion 63.10 (62.80 to 63.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 62.10 (61.80 to 62.80): VL0



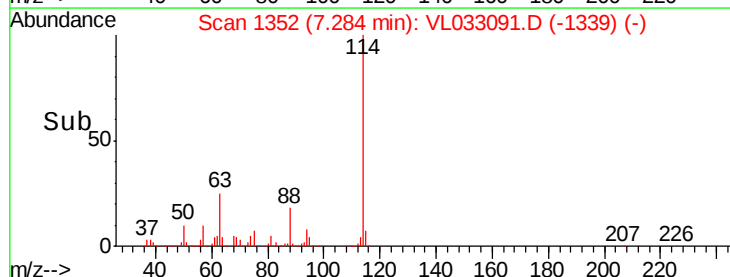
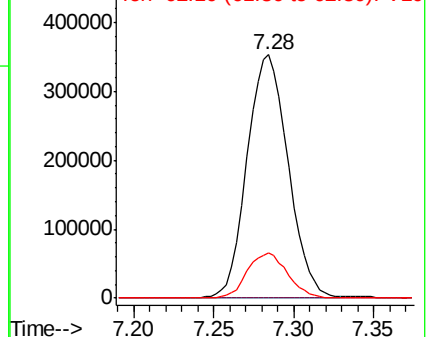


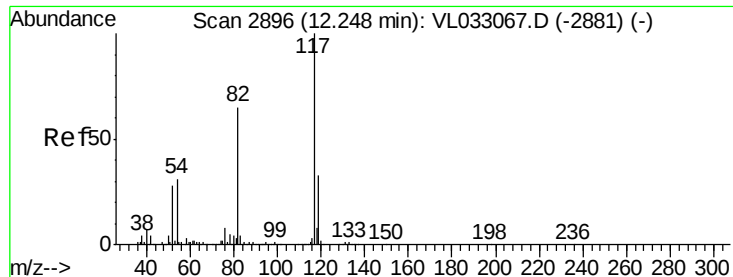

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.24 min Scan# 2892
Delta R.T. -0.01 min
Lab File: VL033091.D
Acq: 16 Jan 2019 14:17

Instrument :
MSVOA_L
ClientSampleId :
QC010919 CAN 10295

Tgt Ion: 117 Resp: 2310251
Ion Ratio Lower Upper
117 100
82 65.7 48.9 73.3
119 32.6 24.6 37.0

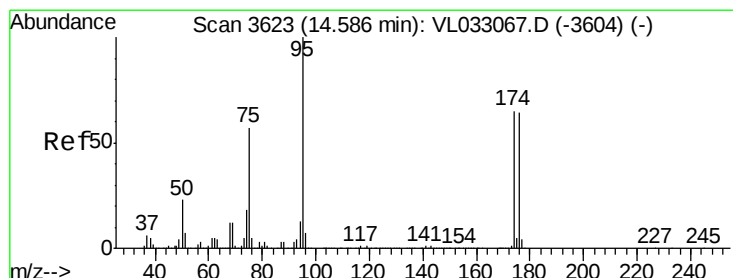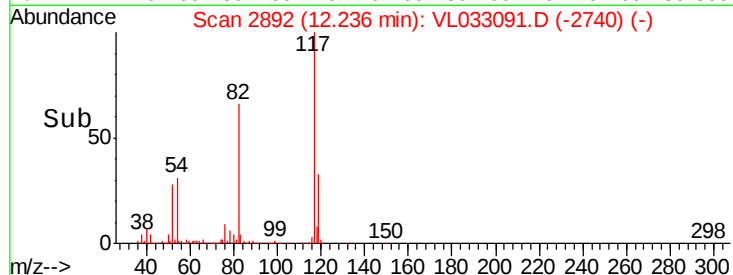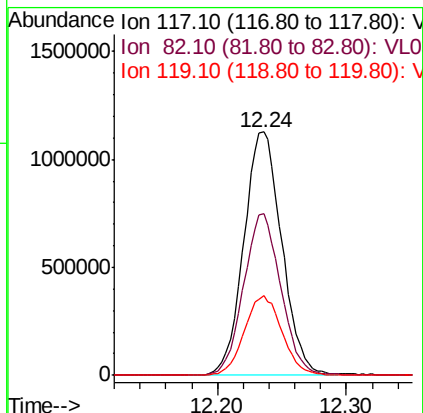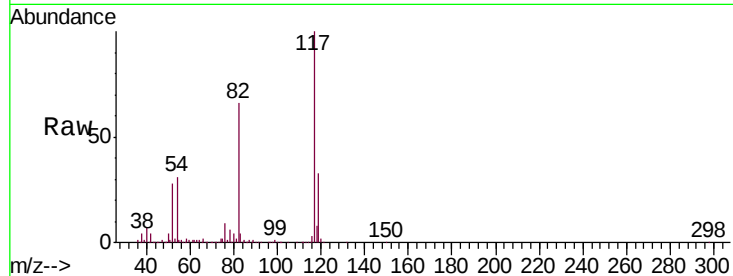

#68
1-Bromo-4-Fluorobenzene
Concen: 10.207 ppbv
RT: 14.57 min Scan# 3619
Delta R.T. -0.01 min
Lab File: VL033091.D
Acq: 16 Jan 2019 14:17

Tgt Ion: 95 Resp: 1807661
Ion Ratio Lower Upper
95 100
174 64.8 51.9 77.9
175 4.6 3.9 5.9

